

Data Path : Z:\HPCHEM1\BNA F\DATA\BF051917\
 Data File : BF095297.D
 Acq On : 20 May 2017 10:59
 Operator : SJ/MA
 Sample : I3199-04
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: May 22 01:56:10 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 18 17:07:53 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.76	152	93083	20.00	ng	0.00
21) Naphthalene-d8	9.78	136	355629	20.00	ng	0.00
38) Acenaphthene-d10	12.61	164	152968	20.00	ng	0.00
63) Phenanthrene-d10	15.02	188	215291	20.00	ng	0.00
75) Chrysene-d12	18.69	240	161465	20.00	ng	0.00
86) Perylene-d12	20.37	264	138929	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.72	112	771340	138.15	ng	-0.01
7) Phenol-d6	7.30	99	947485	141.44	ng	-0.01
23) Nitrobenzene-d5	8.66	82	545039	96.64	ng	-0.01
41) 2,4,6-Tribromophenol	13.91	330	134336	107.23	ng	0.00
44) 2-Fluorobiphenyl	11.55	172	952030	89.58	ng	-0.01
78) Terphenyl-d14	17.33	244	527657	71.98	ng	-0.02
Target Compounds						
10) Phenol	7.32	94	15371	2.18	ng	# 1
19) n-Nitroso-di-n-propylamine	8.66	70	64186	14.17	ng	# 78
49) Dimethylphthalate	12.25	163	174609	13.90	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF051917\
Data File : BF095297.D
Acq On : 20 May 2017 10:59
Operator : SJ/MA
Sample : I3199-04
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: May 22 01:56:10 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 18 17:07:53 2017
Response via : Initial Calibration

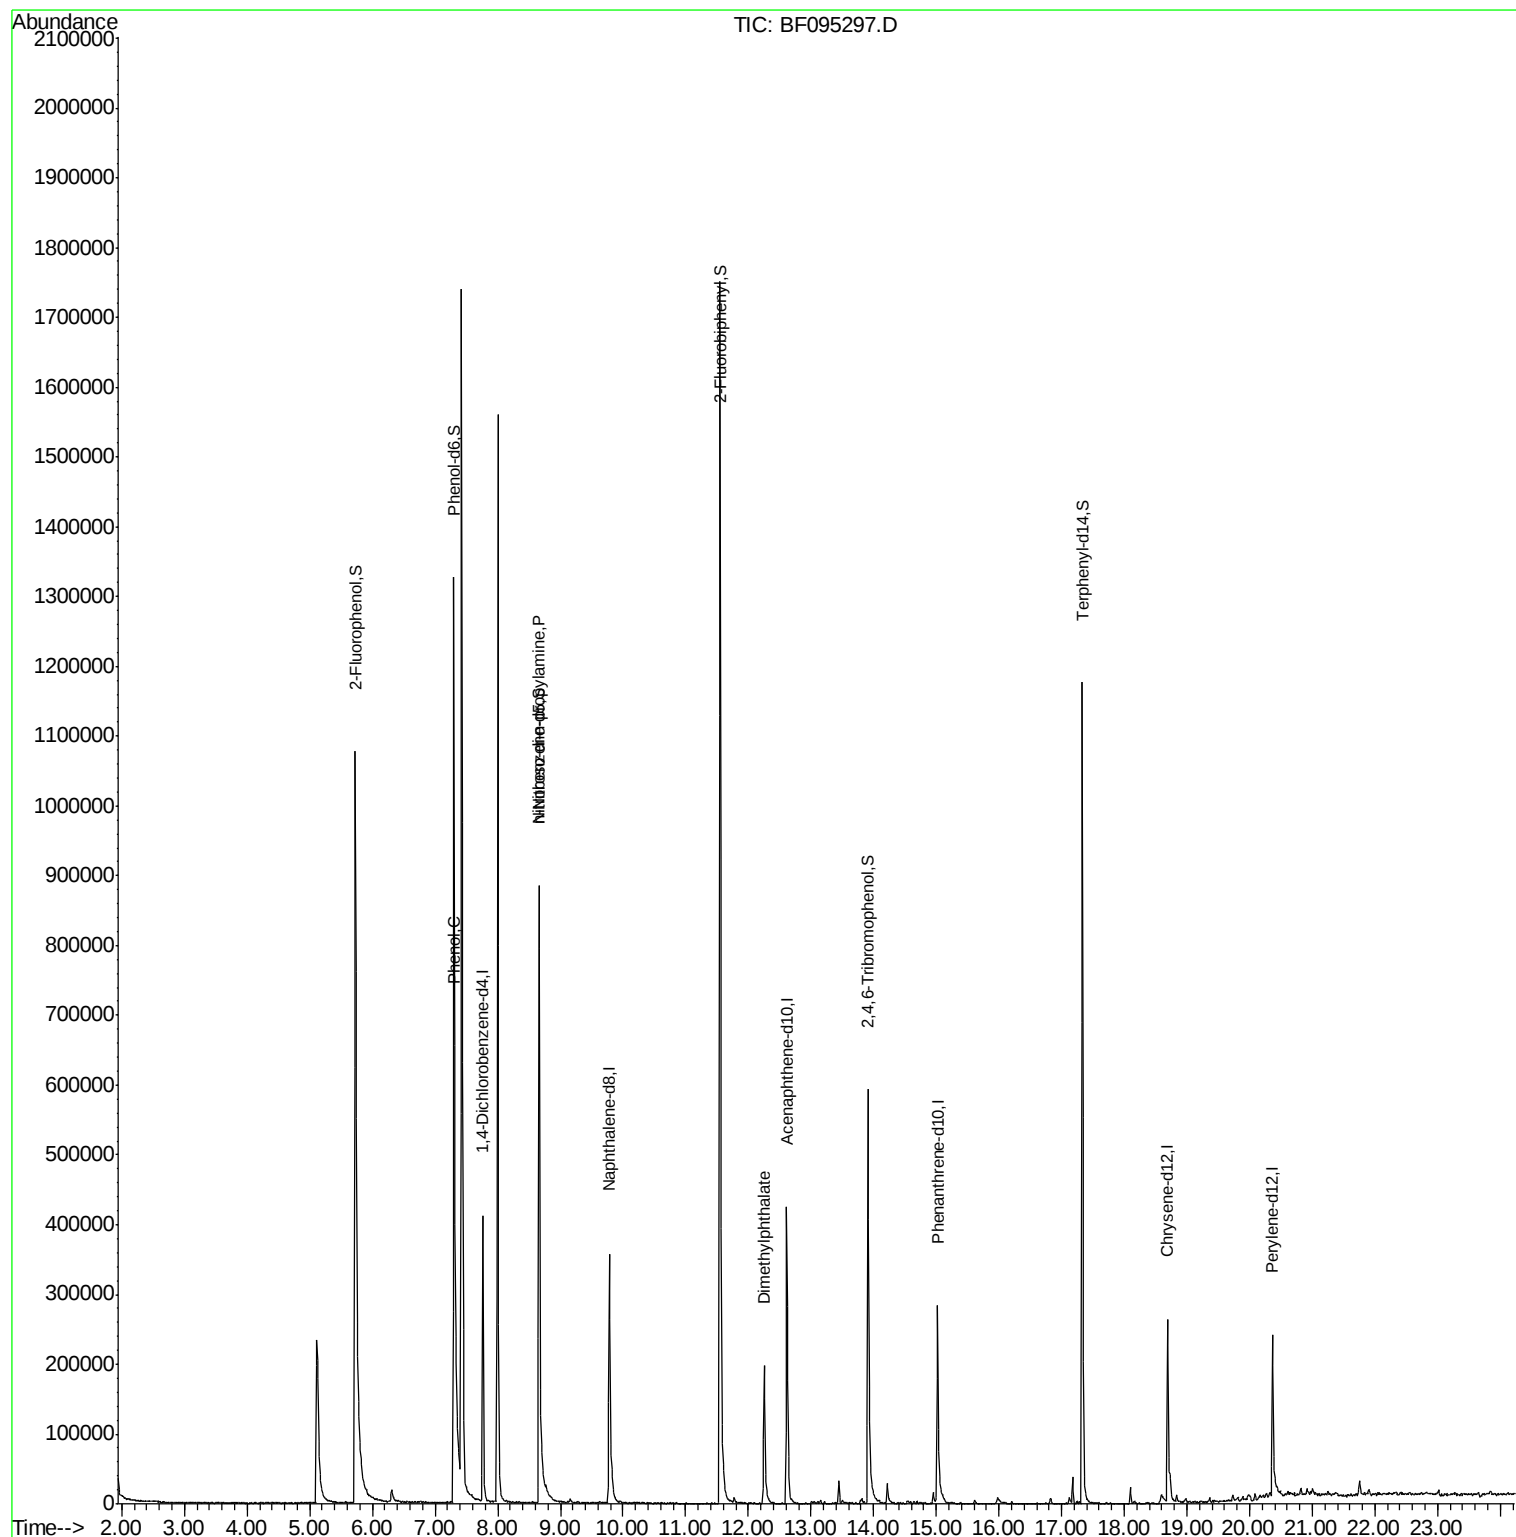

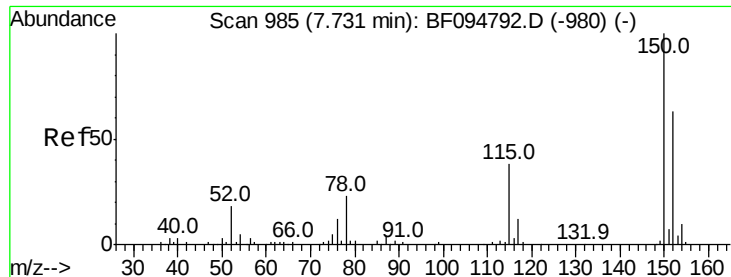


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.76 min Scan# 990
Delta R.T. -0.01 min
Lab File: BF095297.D
Acq: 20 May 2017 10:59

Instrument :
BNA_F
ClientSampleId :

Tot Ion:152 Resp: 93083
Ion Ratio Lower Upper
152 100
150 161.6 126.2 189.2
115 64.2 52.2 78.2

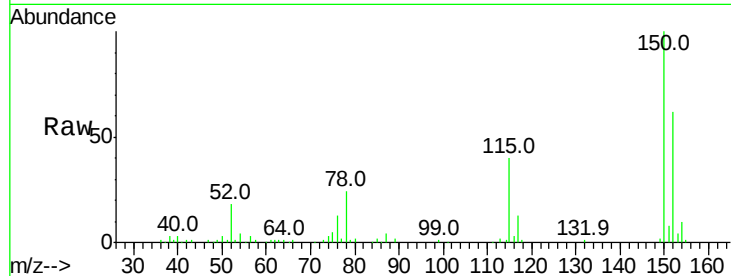


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

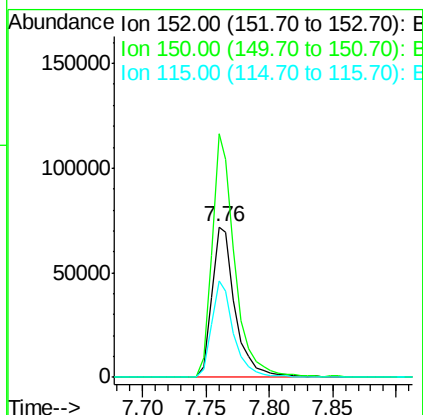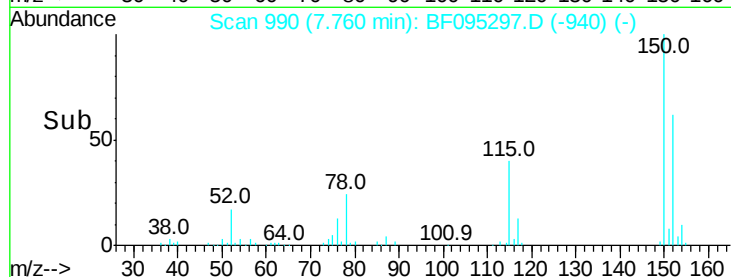



#5

2-Fluorophenol
Concen: 138.15 ng
RT: 5.72 min Scan# 644
Delta R.T. -0.01 min
Lab File: BF095297.D
Acq: 20 May 2017 10:59

Tgt Ion:112 Resp: 771340
Ion Ratio Lower Upper
112 100
64 55.2 46.0 69.0
63 27.2 23.4 35.0



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

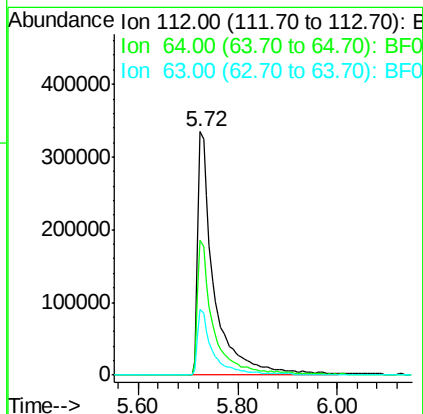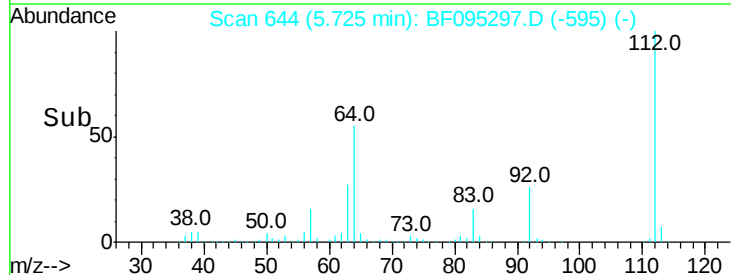



#7

Phenol-d6

Concen: 141.44 ng

RT: 7.30 min Scan# 912

Delta R.T. -0.01 min

Lab File: BF095297.D

Acq: 20 May 2017 10:59

Instrument :

BNA_F

ClientSampleId :





Tot Ion: 99 Resp: 947485

Ion Ratio Lower Upper

99 100

42 16.0 13.5 20.3

71 31.8 24.5 36.7

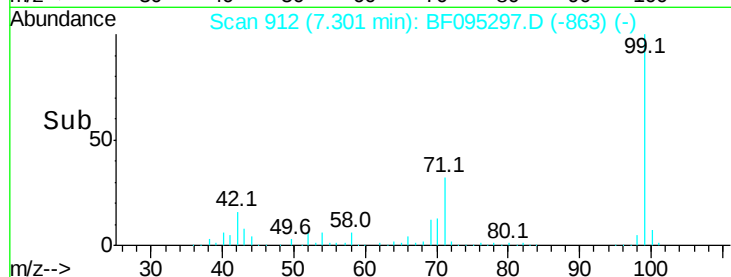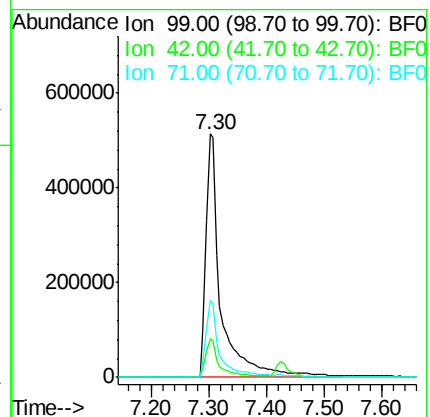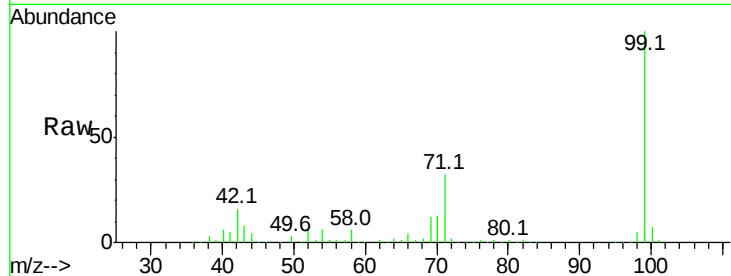

#10

Phenol

Concen: 2.18 ng

RT: 7.32 min Scan# 915

Delta R.T. -0.01 min

Lab File: BF095297.D

Acq: 20 May 2017 10:59




Tgt Ion: 94 Resp: 15371


Ion Ratio Lower Upper

94 100

65 49.2 9.9 49.9

66 135.0 23.1 63.1#

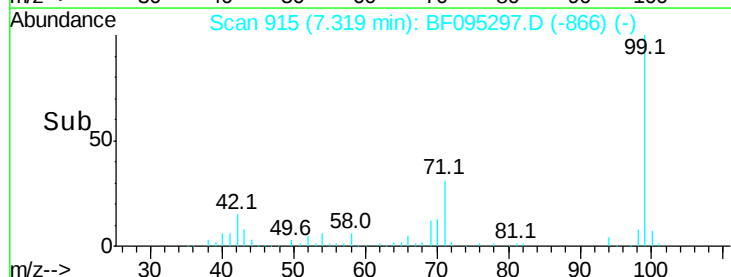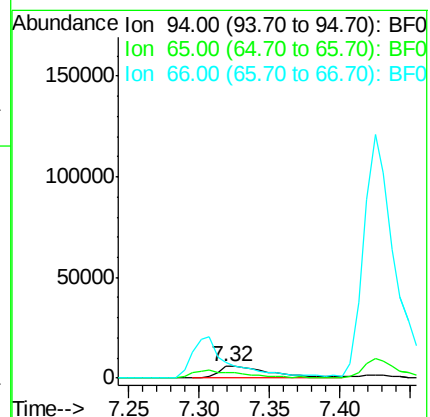

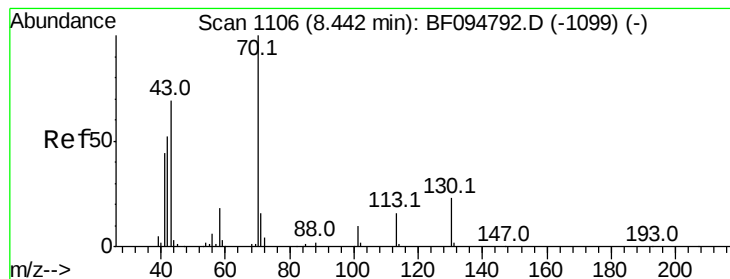

#19

n-Nitroso-di-n-propylamine

Concen: 14.17 ng

RT: 8.66 min Scan# 1143

Delta R.T. 0.18 min

Lab File: BF095297.D

Acq: 20 May 2017 10:59

Instrument :

BNA_F

ClientSampleId :

Tot Ion: 70 Resp: 64186





Ion Ratio Lower Upper

70 100

42 46.5 47.2 70.8#

101 0.0 7.2 10.8#

130 2.7 15.9 23.9#

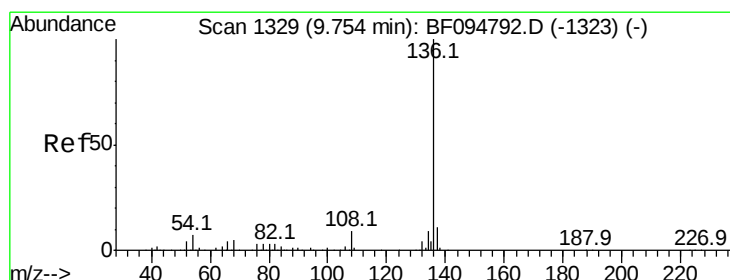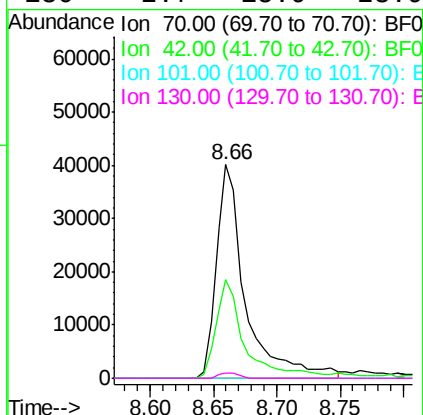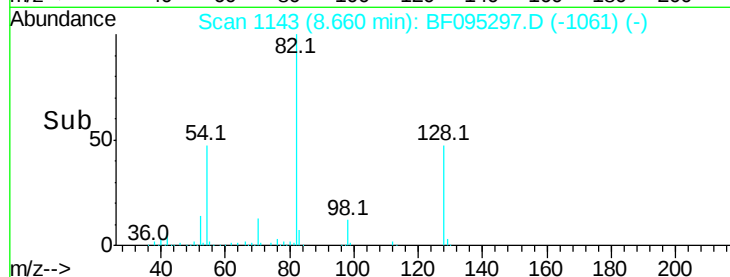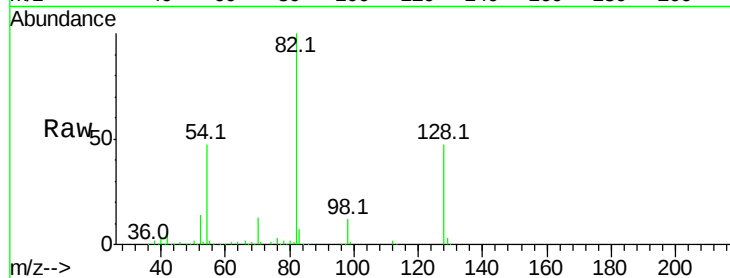

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 9.78 min Scan# 1334

Delta R.T. 0.00 min

Lab File: BF095297.D

Acq: 20 May 2017 10:59

Tgt Ion: 136 Resp: 355629




Ion Ratio Lower Upper


136 100

137 10.8 8.5 12.7

54 6.5 4.9 7.3

68 5.1 4.1 6.1


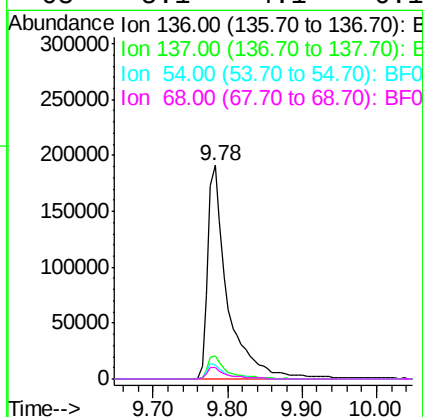
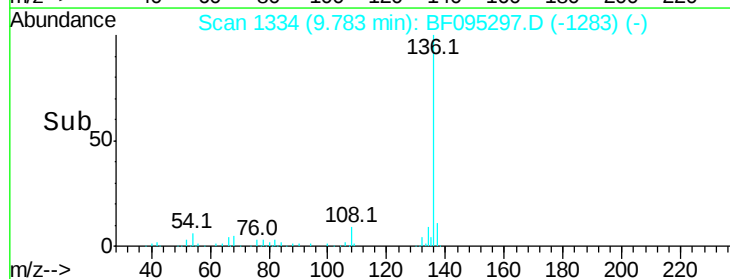
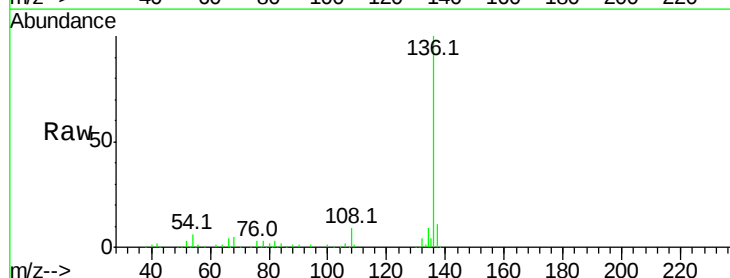


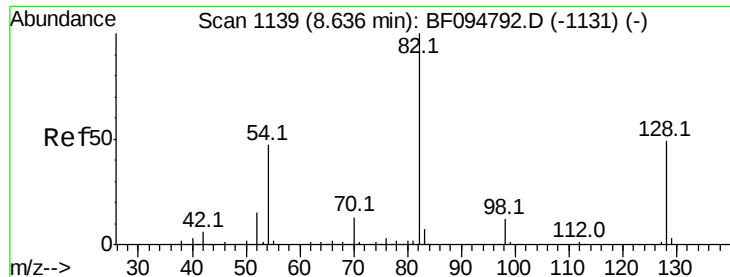

#23
Nitrobenzene-d5
Concen: 96.64 ng
RT: 8.66 min Scan# 1143
Delta R.T. -0.01 min
Lab File: BF095297.D
Acq: 20 May 2017 10:59




Instrument :
BNA_F
ClientSampleId :


Tot Ion: 82 Resp: 545039
Ion Ratio Lower Upper
82 100
128 47.2 34.0 51.0
54 47.1 42.2 63.2

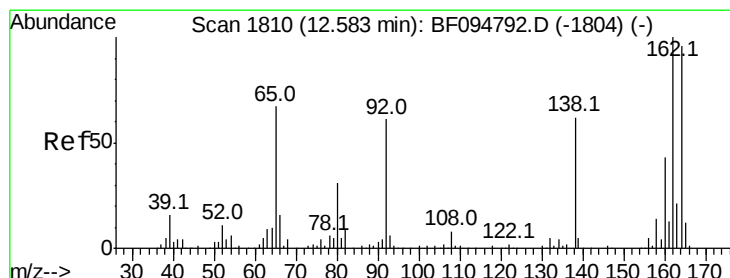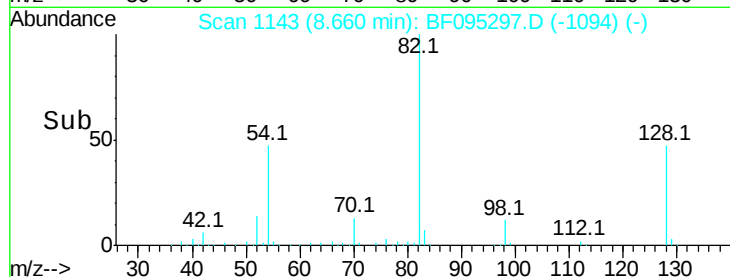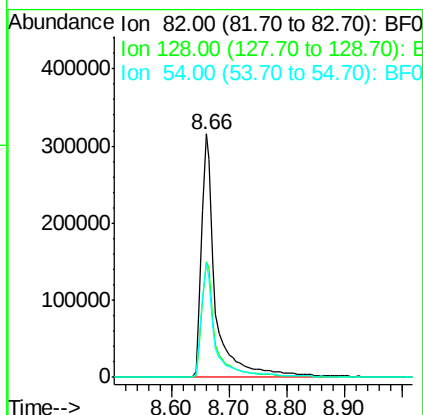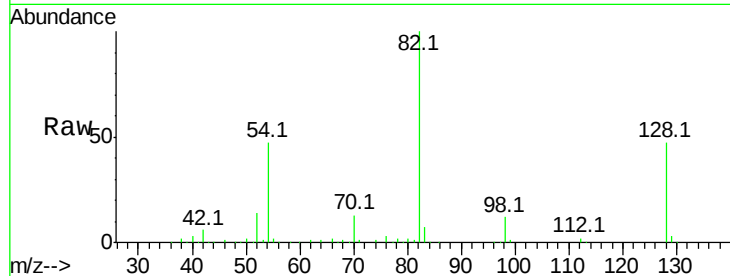

#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 12.61 min Scan# 1815
Delta R.T. -0.01 min
Lab File: BF095297.D
Acq: 20 May 2017 10:59

Tgt Ion:164 Resp: 152968
Ion Ratio Lower Upper
164 100
162 104.9 82.6 123.8
160 41.4 36.2 54.2

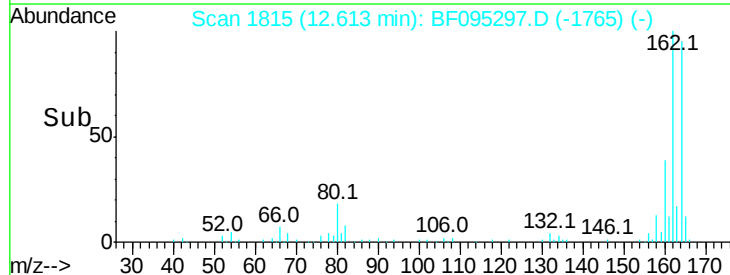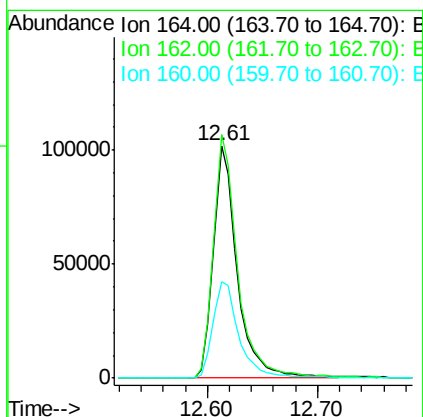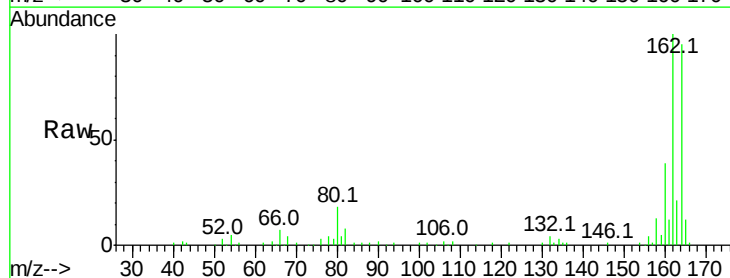


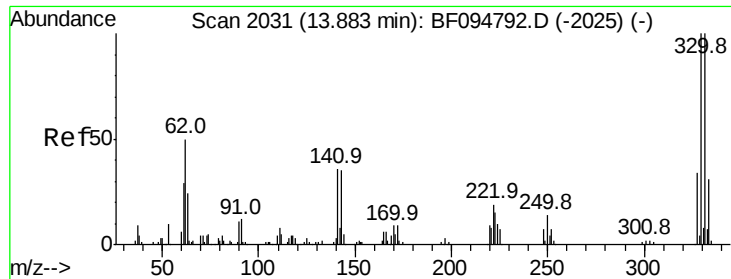




#41
 2,4,6-Tribromophenol
 Concen: 107.23 ng
 RT: 13.91 min Scan# 2036
 Delta R.T. -0.01 min
 Lab File: BF095297.D
 Acq: 20 May 2017 10:59

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
330	100		
332	100.5	76.6	115.0
141	37.7	31.4	47.2

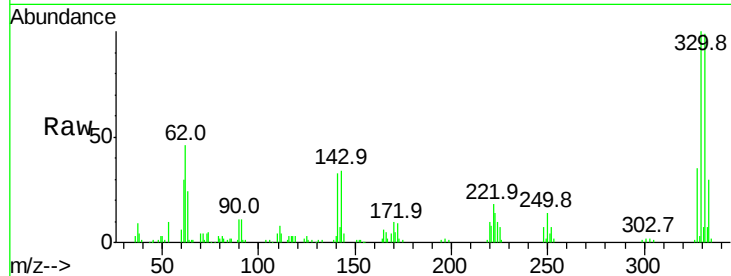


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

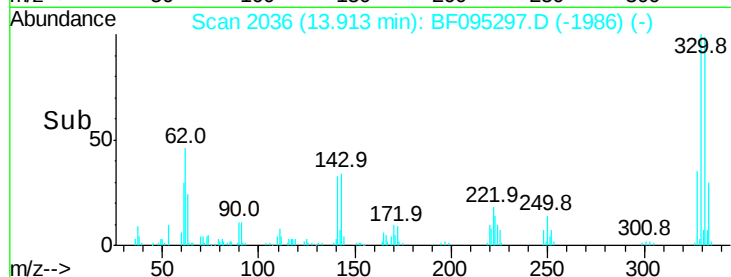
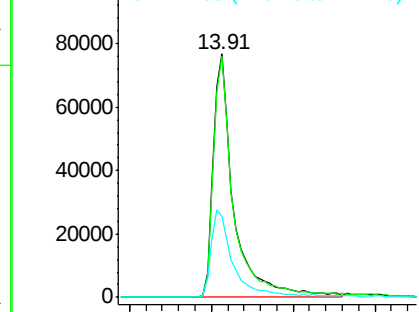



#44
 2-Fluorobiphenyl
 Concen: 89.58 ng
 RT: 11.55 min Scan# 1634
 Delta R.T. -0.01 min
 Lab File: BF095297.D
 Acq: 20 May 2017 10:59

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.9	29.6	44.4
170	23.1	19.8	29.8



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

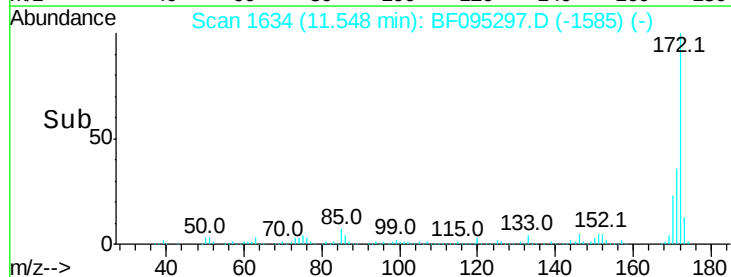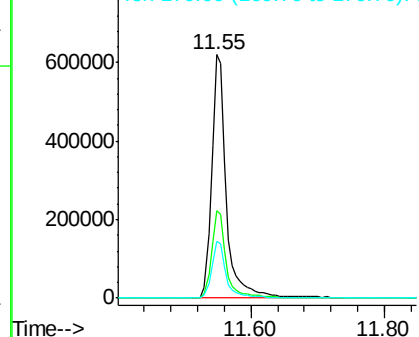

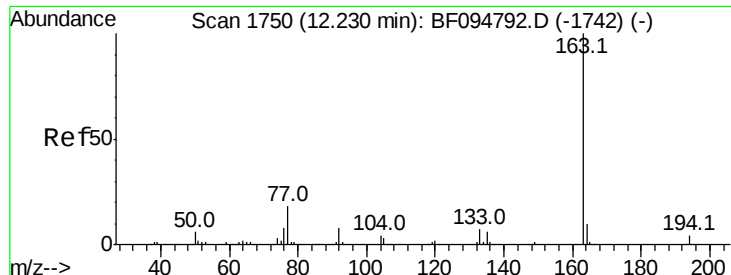

#49

Dimethylphthalate

Concen: 13.90 ng

RT: 12.25 min Scan# 1754

Delta R.T. -0.01 min

Lab File: BF095297.D

Acq: 20 May 2017 10:59

Instrument :

BNA_F

ClientSampled :


Tot Ion:163 Resp: 174609

Ion Ratio Lower Upper

163 100

194 3.7 2.6 4.0




164 9.6 8.4 12.6



Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

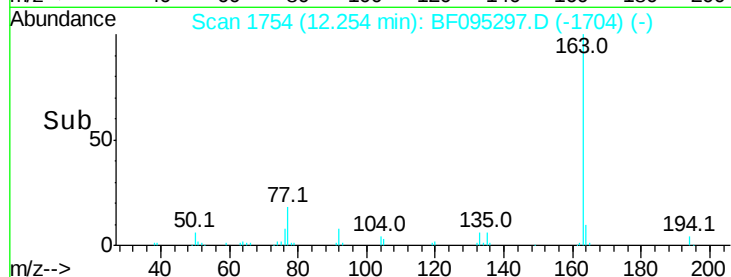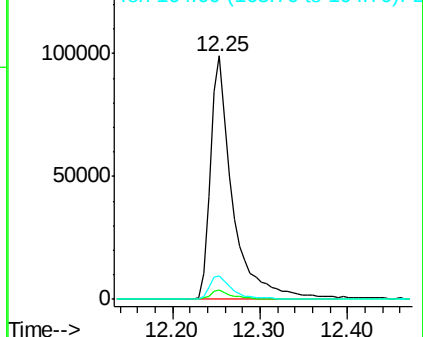

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 15.02 min Scan# 2224

Delta R.T. -0.01 min

Lab File: BF095297.D

Acq: 20 May 2017 10:59


Tgt Ion:188 Resp: 215291

Ion Ratio Lower Upper

188 100

94 10.5 9.4 14.2



80 11.1 10.2 15.2




Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

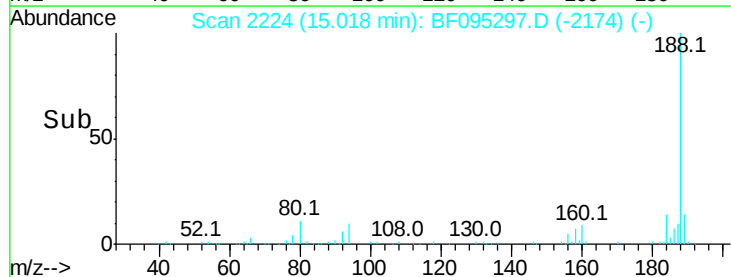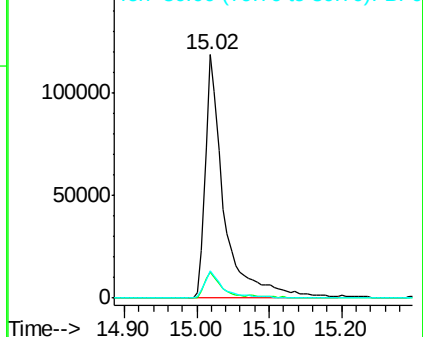

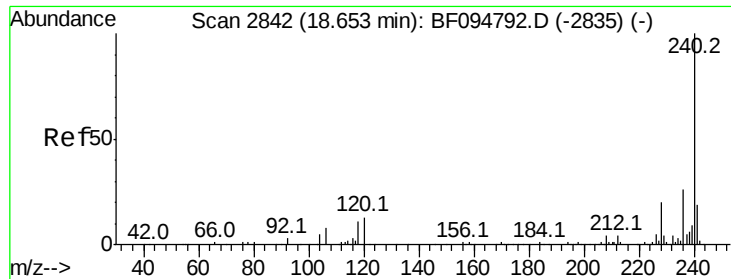

#75

Chrysene-d12

Concen: 20.00 ng

RT: 18.69 min Scan# 2848

Delta R.T. -0.01 min

Lab File: BF095297.D

Acq: 20 May 2017 10:59

Instrument :

BNA_F

ClientSampleId :


Tot Ion:240 Resp: 161465

Ion Ratio Lower Upper

240 100

120 14.2 5.8 8.8#




236 25.3 20.5 30.7

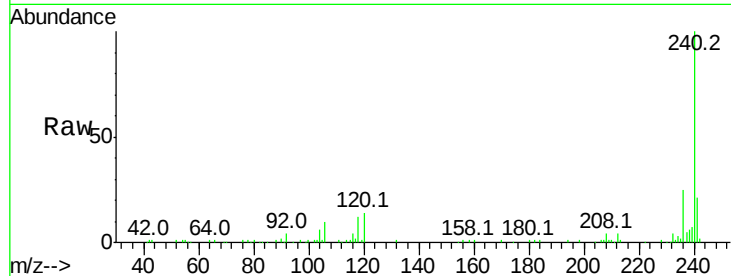

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

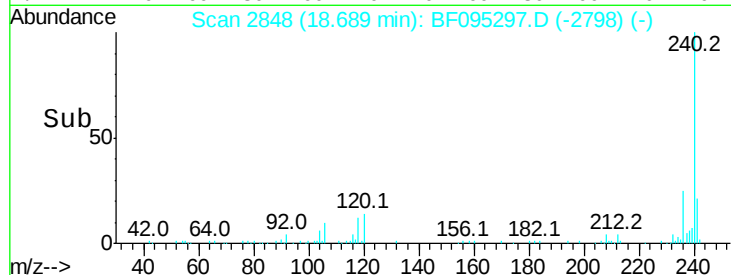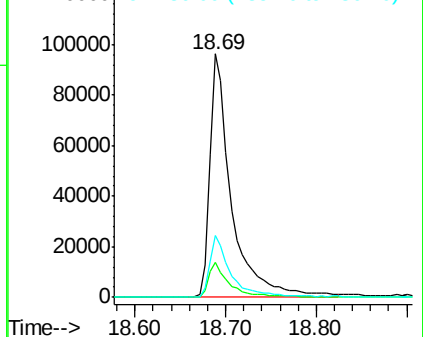

#78

Terphenyl-d14

Concen: 71.98 ng

RT: 17.33 min Scan# 2617

Delta R.T. -0.02 min

Lab File: BF095297.D

Acq: 20 May 2017 10:59


Tgt Ion:244 Resp: 527657

Ion Ratio Lower Upper

244 100

212 6.4 6.0 9.0



122 14.2 10.3 15.5




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

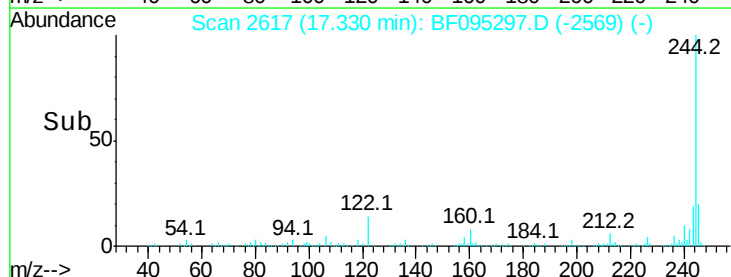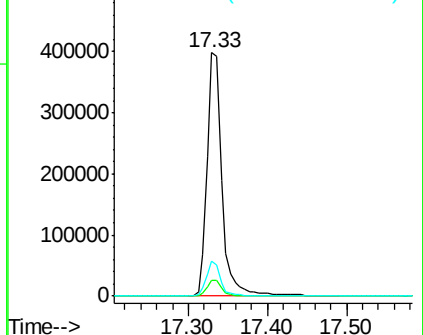


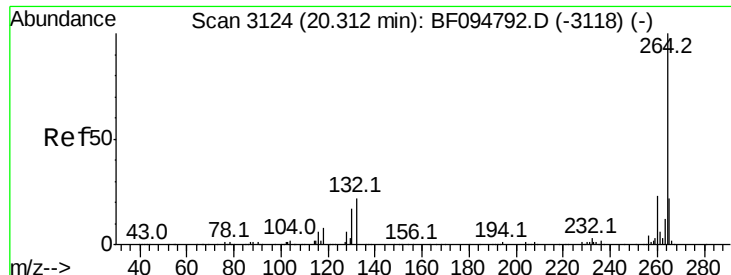

#86
Pervlene-d12
Concen: 20.00 ng
RT: 20.37 min Scan# 3133
Delta R.T. 0.00 min
Lab File: BF095297.D
Acq: 20 May 2017 10:59

Instrument :
BNA_F
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.0	19.5	29.3
265	21.0	17.2	25.8



Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

