
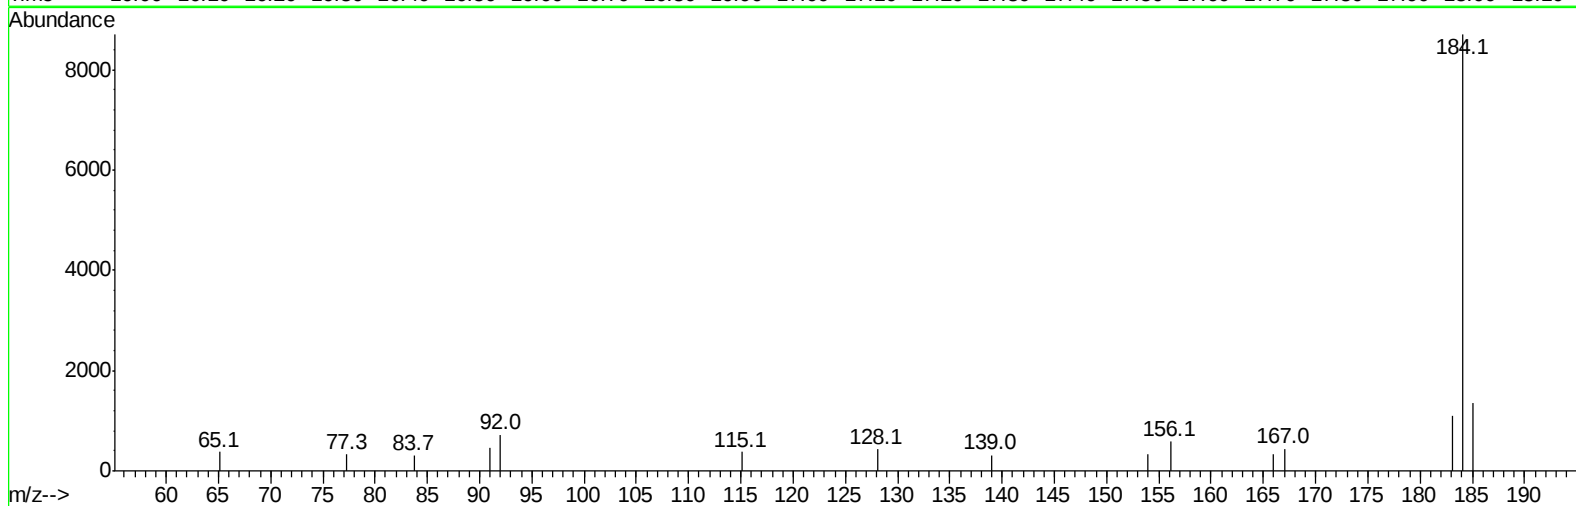


Data Path : Z:\HPCHEM1\BNA F\DATA\BF051917\
Data File : BF095265.D
Acq On : 19 May 2017 15:41
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 22 05:13:35 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 18 17:07:53 2017
Response via : Initial Calibration

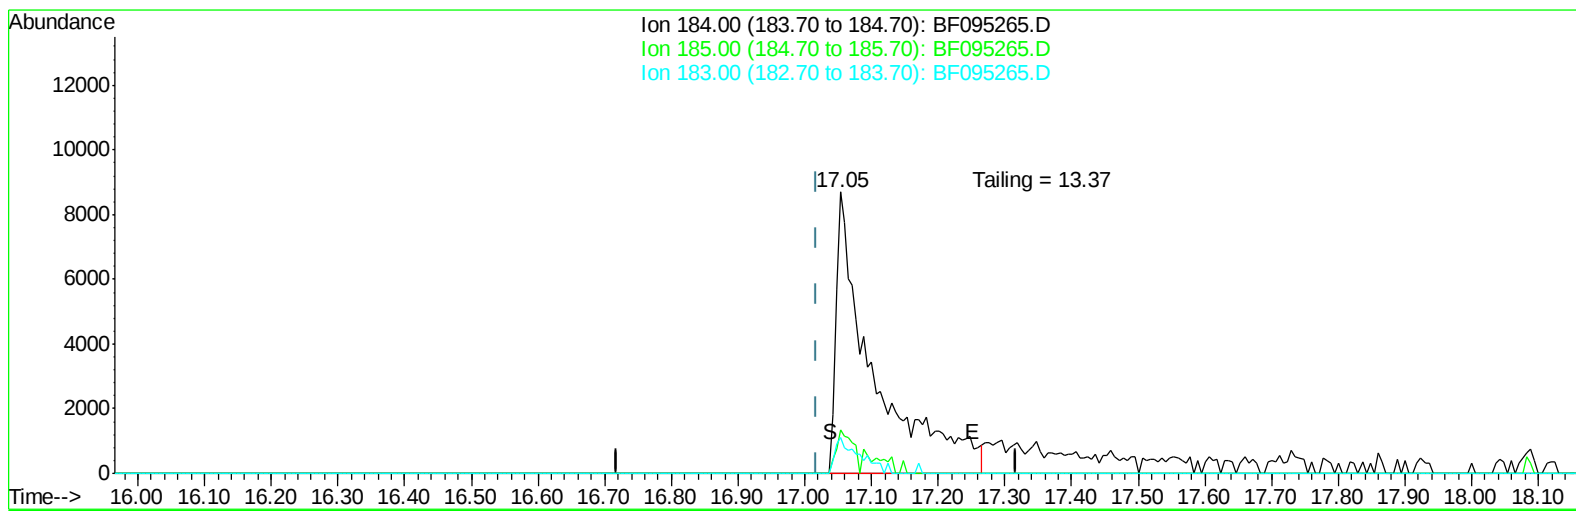

TIC: BF095265.D

(76) Benzidine




17.054min (+0.035) 0.00ng

response 26254

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	15.61
183.00	12.20	12.67
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF051917\
 Data File : BF095265.D
 Acq On : 19 May 2017 15:41
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 22 05:13:35 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 18 17:07:53 2017
 Response via : Initial Calibration

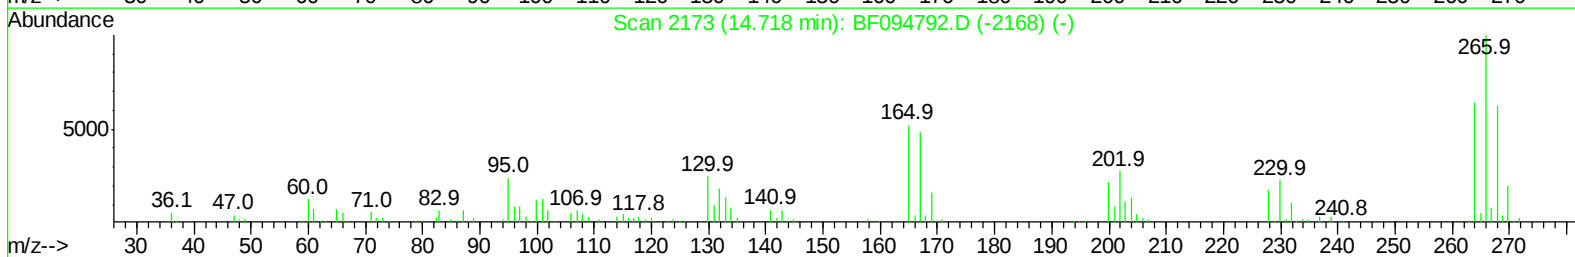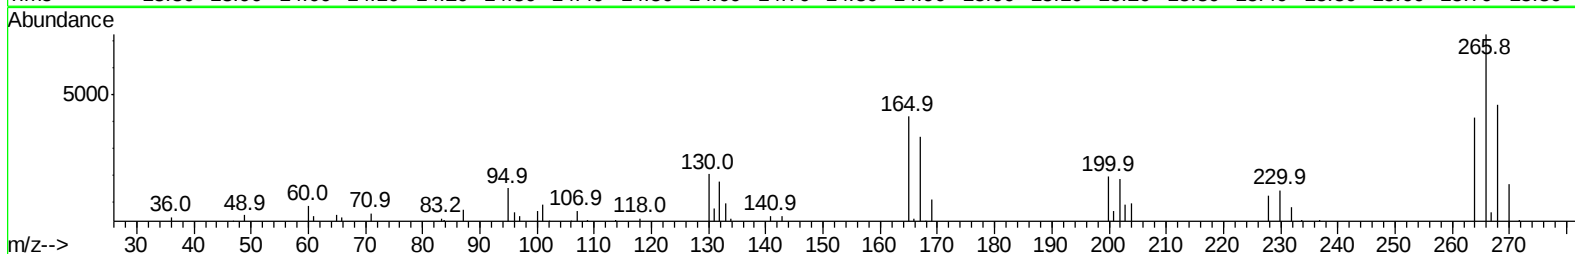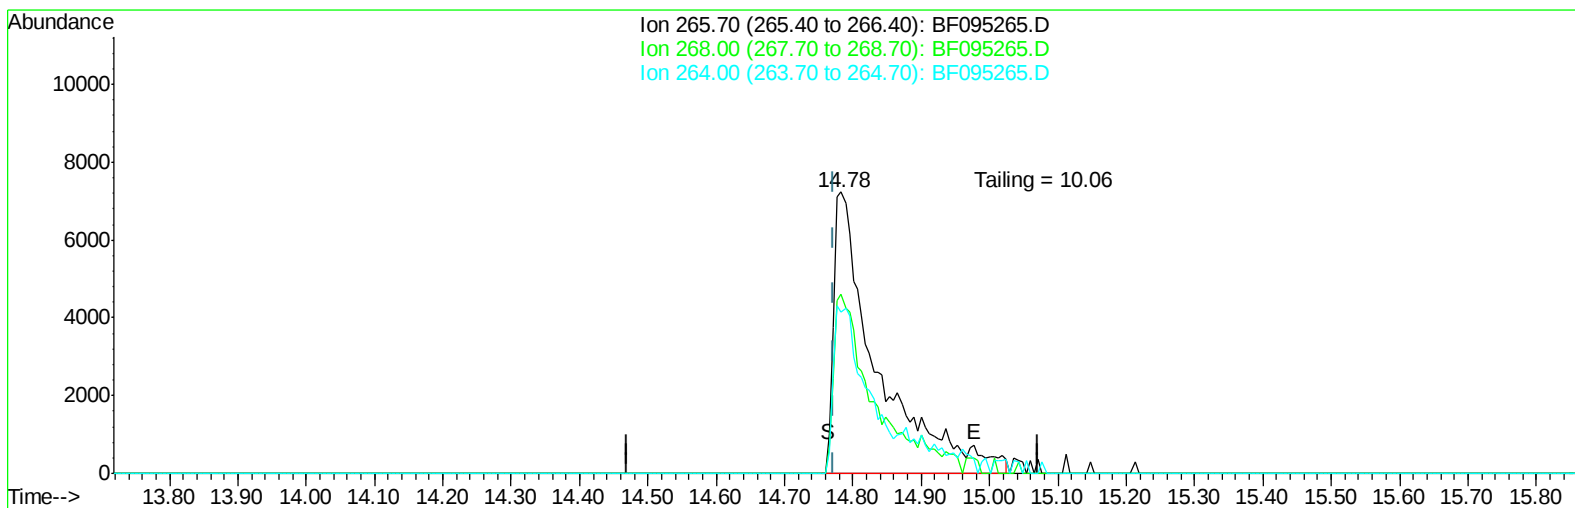

TIC: BF095265.D

(69) Pentachlorophenol (C)

14.783min (+0.012) 0.00ng

response 23206

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.84
264.00	64.60	57.24
0.00	0.00	0.00