
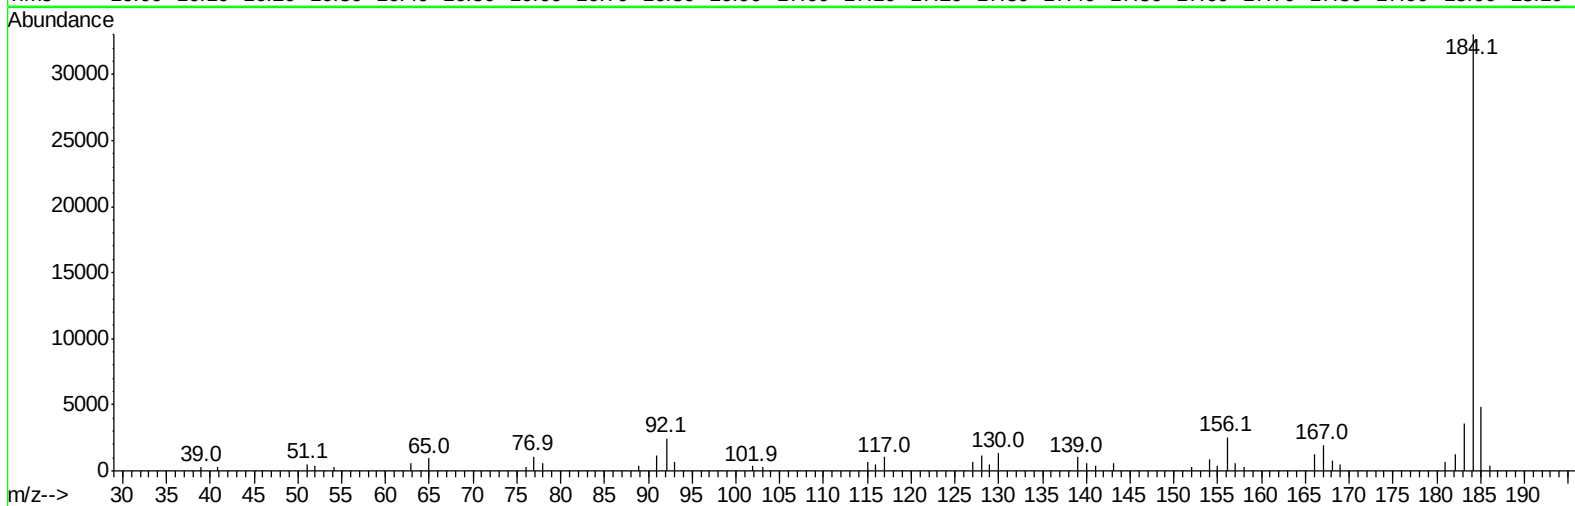


Data Path : Z:\HPCHEM1\BNA F\DATA\BF051917\
Data File : BF095287.D
Acq On : 20 May 2017 5:07
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 22 05:15:47 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 18 17:07:53 2017
Response via : Initial Calibration

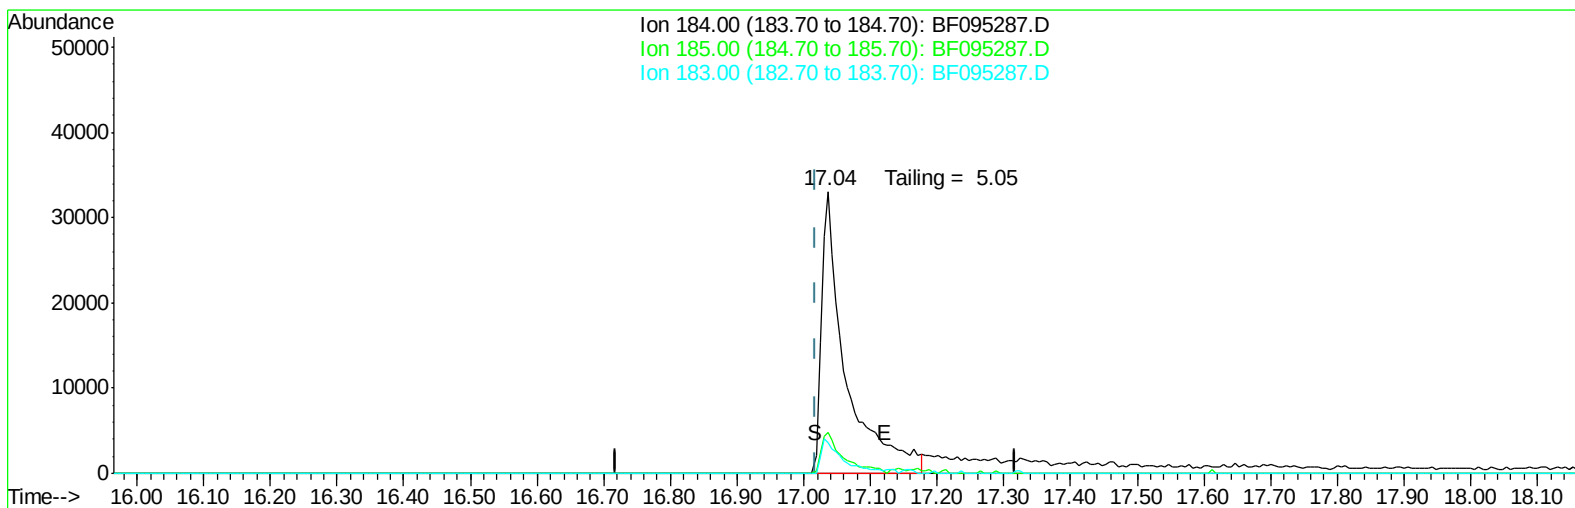

TIC: BF095287.D

(76) Benzidine



17.036min (+0.018) 0.00ng

response 82140

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.60#
183.00	12.20	10.83
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF051917\
Data File : BF095287.D
Acq On : 20 May 2017 5:07
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 22 05:15:47 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 18 17:07:53 2017
Response via : Initial Calibration

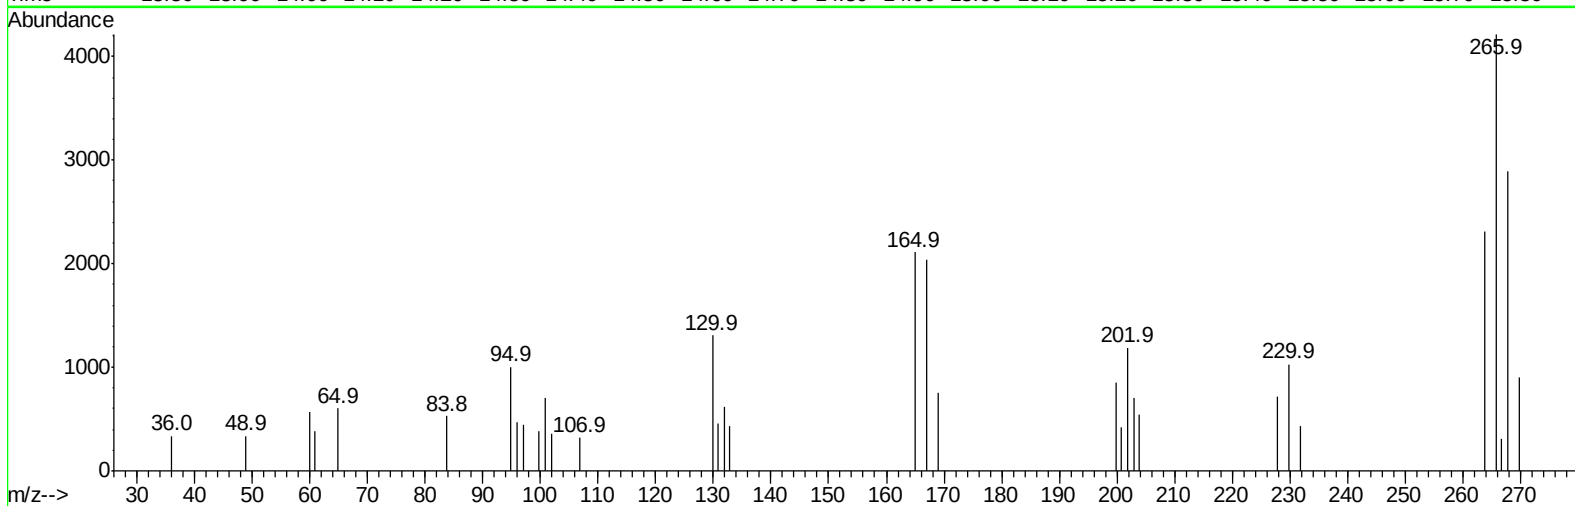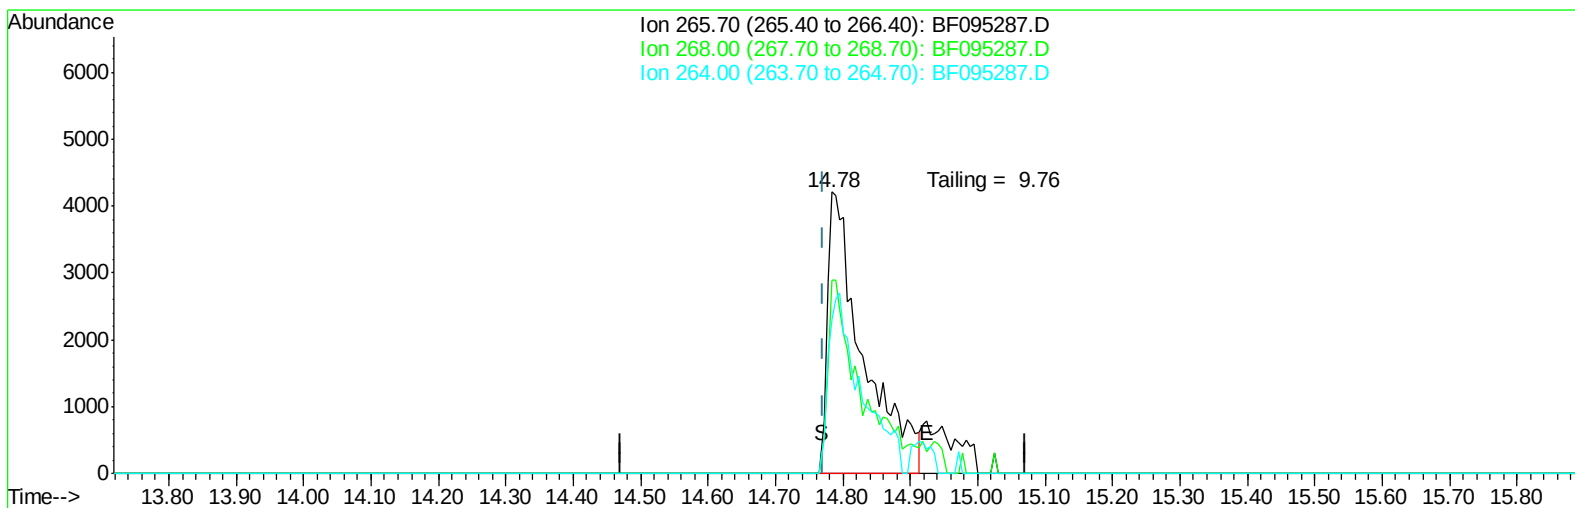

TIC: BF095287.D

(69) Pentachlorophenol (C)

14.783min (+0.012) 0.00ng m

response 15483

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	68.70
264.00	64.60	54.77
0.00	0.00	0.00