

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF051917\
 Data File : BF095278.D
 Acq On : 19 May 2017 23:15
 Operator : SJ/MA
 Sample : I3202-04
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-4COMP

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.113	537	540	561	rBV	186882	543162	21.61%	2.684%
2	5.731	642	645	679	rBV	824297	1944670	77.36%	9.609%
3	6.319	740	745	753	rBV2	12548	25415	1.01%	0.126%
4	7.301	909	912	929	rBV	1004603	1848858	73.55%	9.136%
5	7.431	929	934	951	rVB	1365091	2315272	92.10%	11.441%
6	7.766	987	991	1002	rBV	403848	514188	20.46%	2.541%
7	8.001	1026	1031	1046	rBV	1293897	1674053	66.60%	8.272%
8	8.660	1139	1143	1162	rBV	636394	1183514	47.08%	5.848%
9	9.783	1330	1334	1363	rBV	362201	721678	28.71%	3.566%
10	11.554	1629	1635	1653	rBV	1650737	2513750	100.00%	12.421%
11	12.260	1751	1755	1772	rBV	144775	251885	10.02%	1.245%
12	12.613	1811	1815	1839	rBV2	506467	851955	33.89%	4.210%
13	13.448	1952	1957	1963	rBV	24105	28231	1.12%	0.140%
14	13.907	2030	2035	2056	rBV	796600	1472249	58.57%	7.275%
15	14.218	2085	2088	2092	rBV	30338	39229	1.56%	0.194%
16	15.018	2218	2224	2237	rBV	487604	815294	32.43%	4.029%
17	15.971	2382	2386	2398	rBV2	27689	60884	2.42%	0.301%
18	17.336	2613	2618	2638	rBV	1999304	2346756	93.36%	11.596%
19	18.583	2825	2830	2844	rBV4	16945	56382	2.24%	0.279%
20	18.689	2844	2848	2864	rBV	362888	601936	23.95%	2.974%
21	20.371	3129	3134	3153	rBV	210960	427767	17.02%	2.114%


Sum of corrected areas: 20237128

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF051917\
Data File : BF095278.D
Acq On : 19 May 2017 23:15
Operator : SJ/MA
Sample : I3202-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampled :
SB-4COMP

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

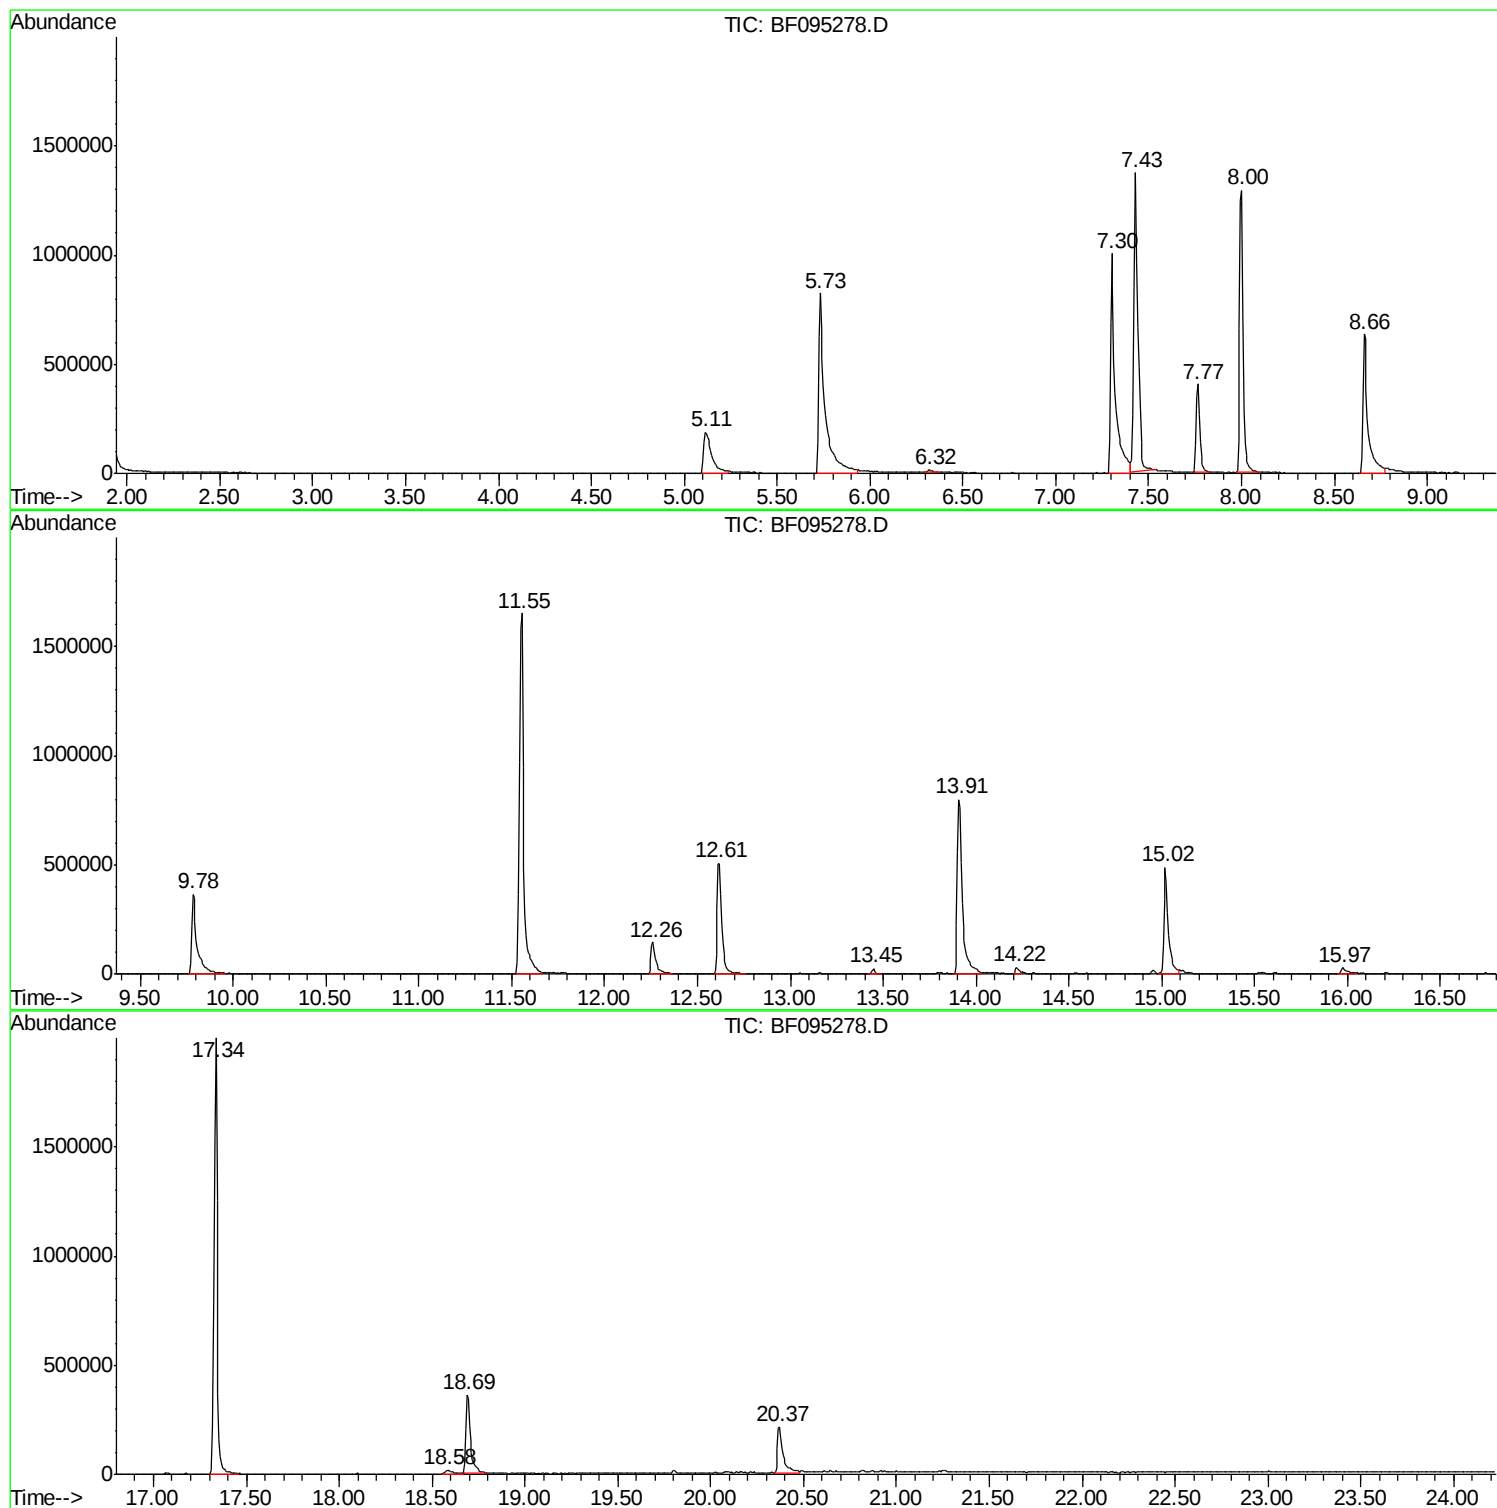

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF051917\
Data File : BF095278.D
Acq On : 19 May 2017 23:15
Operator : SJ/MA
Sample : I3202-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-4COMP










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.11	21.13 ng	543162	1,4-Dichlorobenzene-d4	7.77

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56
2			Acetic acid, 1,1-dimethylethyl e...	116	C6H12O2	000540-88-5	39
3			2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	17
4			Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	17
5			Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9

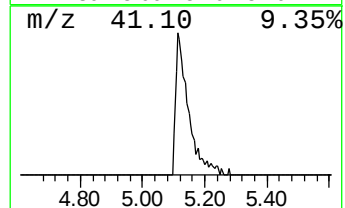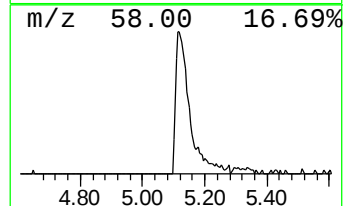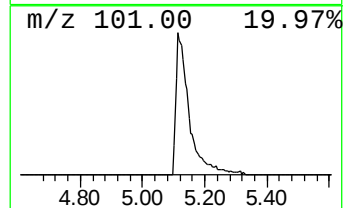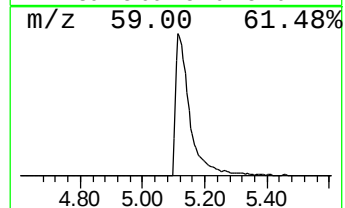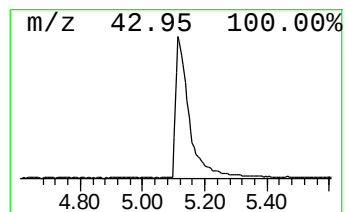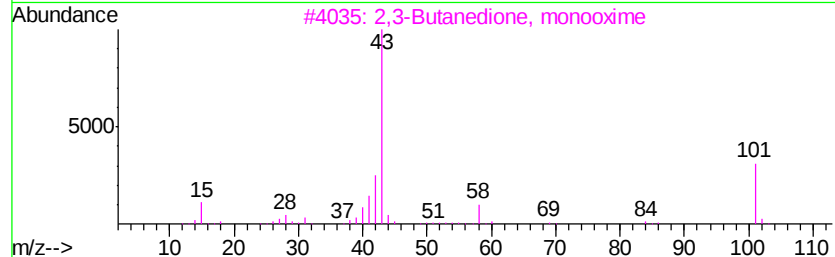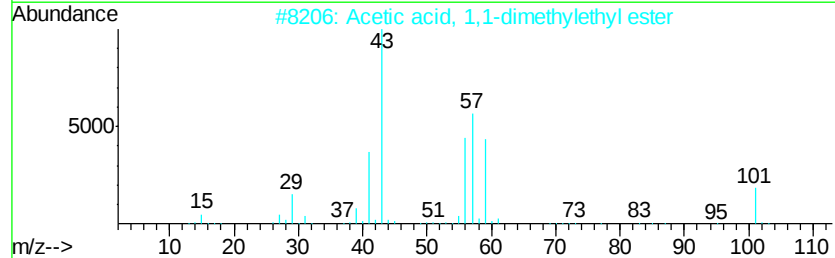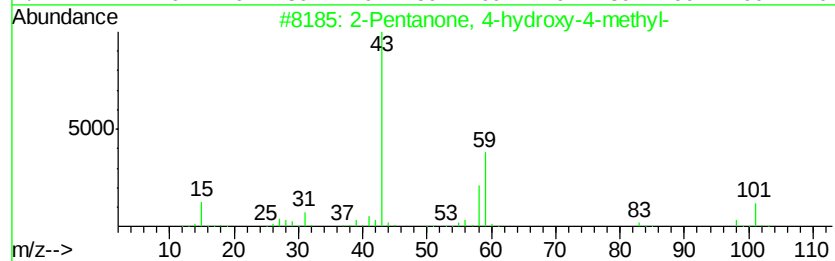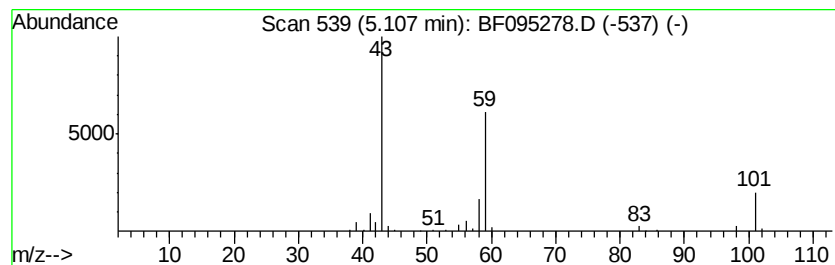

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF051917\
Data File : BF095278.D
Acq On : 19 May 2017 23:15
Operator : SJ/MA
Sample : I3202-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-4COMP










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown7.43 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.43	90.06 ng	2315270	1,4-Dichlorobenzene-d4	7.77

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	38
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	25
3		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	12
4		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	9
5		4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9

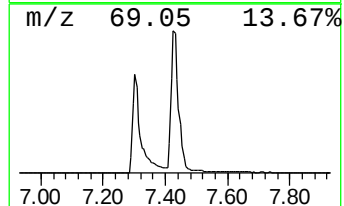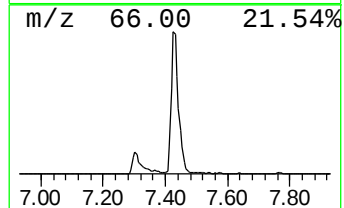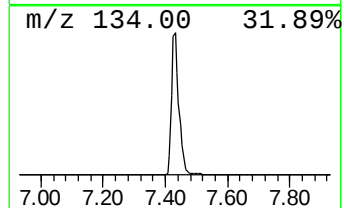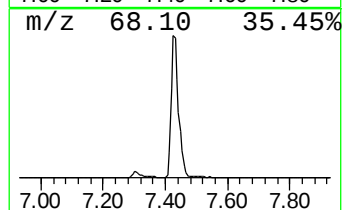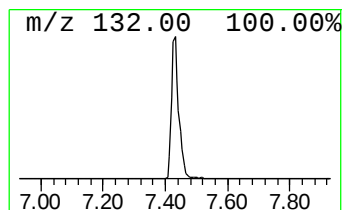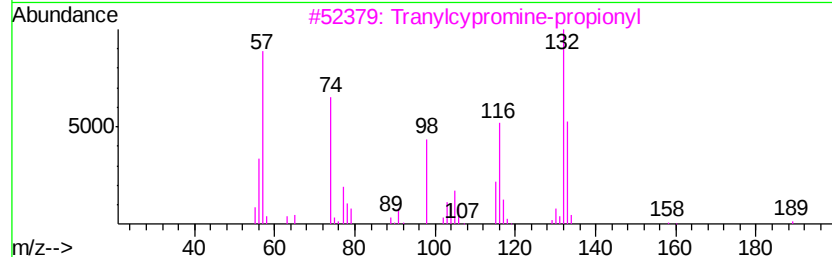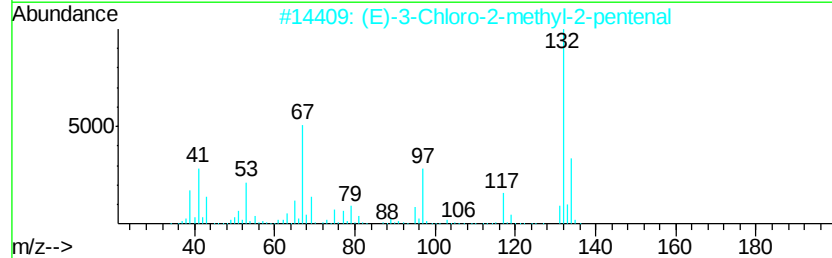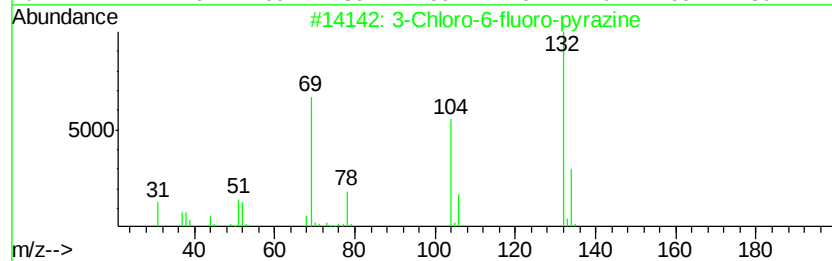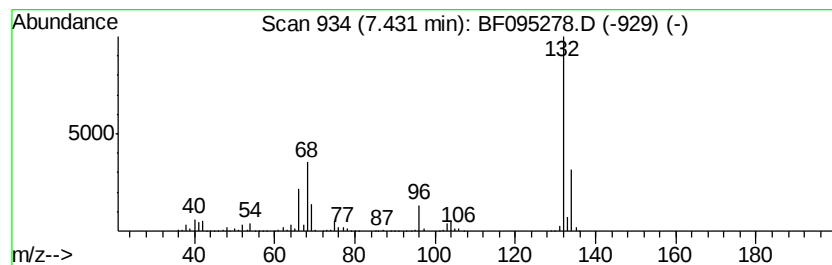

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF051917\
Data File : BF095278.D
Acq On : 19 May 2017 23:15
Operator : SJ/MA
Sample : I3202-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-4COMP

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	5.11	21.1	ng	543162	1	7.77	514188	20.0
unknown7.43	7.43	90.1	ng	2315270	1	7.77	514188	20.0