


Data Path : Z:\HPCHEM1\BNA_F\Data\BF051917\
 Data File : BF095265.D
 Acq On : 19 May 2017 15:41
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 18 17:07:53 2017

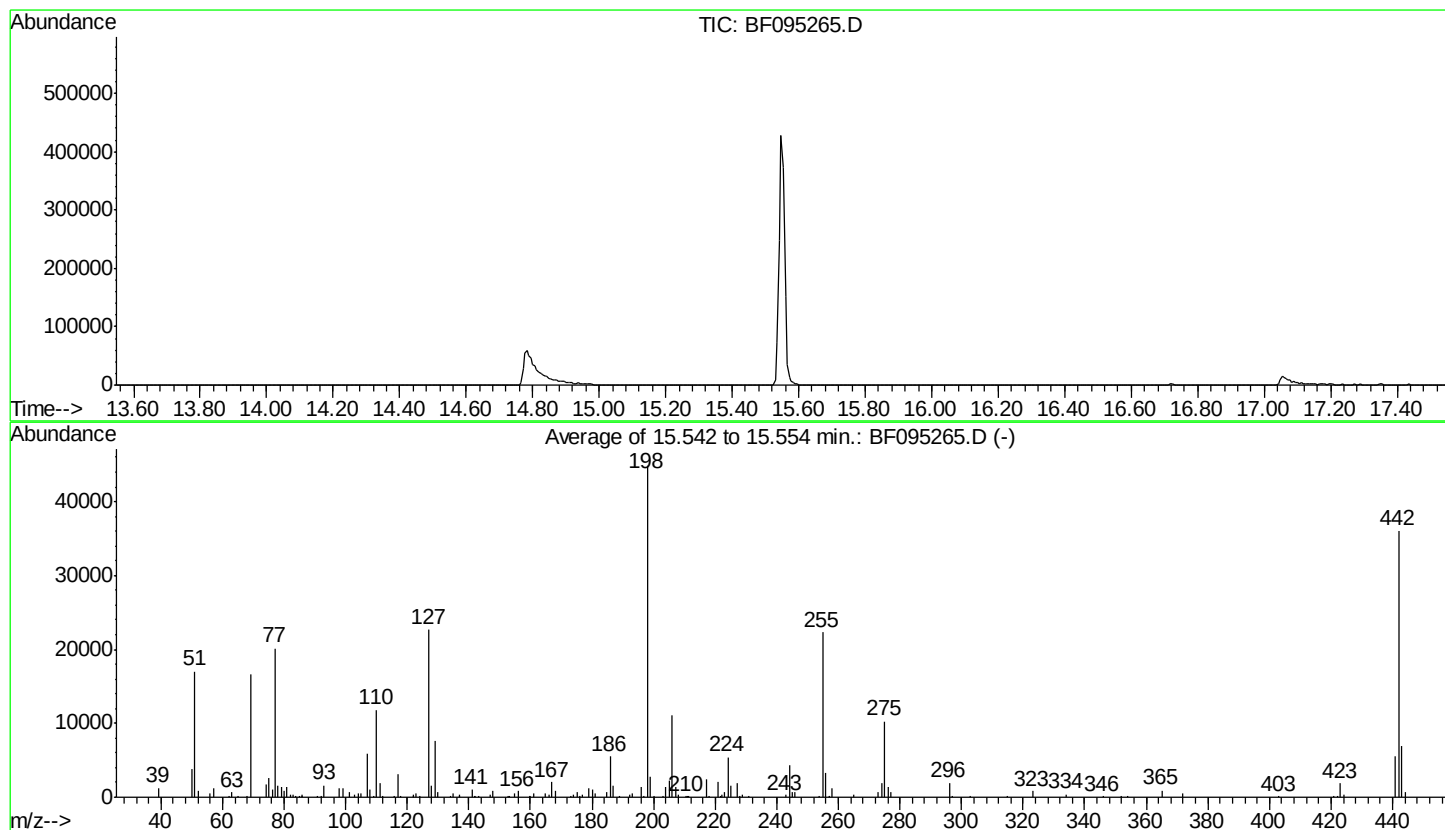

AutoFind: Scans 2313, 2314, 2315; Background Corrected with Scan 2308

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.9	17013	PASS
68	69	0.00	2	0.8	136	PASS
69	198	0.00	100	36.9	16569	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.5	22642	PASS
197	198	0.00	2	0.5	227	PASS
198	198	100	100	100.0	44877	PASS
199	198	5	9	6.2	2801	PASS
275	198	10	60	22.8	10236	PASS
365	198	1	100	2.0	910	PASS
441	442	0.01	24	15.4	5541	PASS
442	198	50	100	80.3	36042	PASS
443	442	15	24	19.4	6999	PASS