


Data Path : Z:\HPCHEM1\BNA_F\Data\BF051917\
 Data File : BF095287.D
 Acq On : 20 May 2017 5:07
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 18 17:07:53 2017

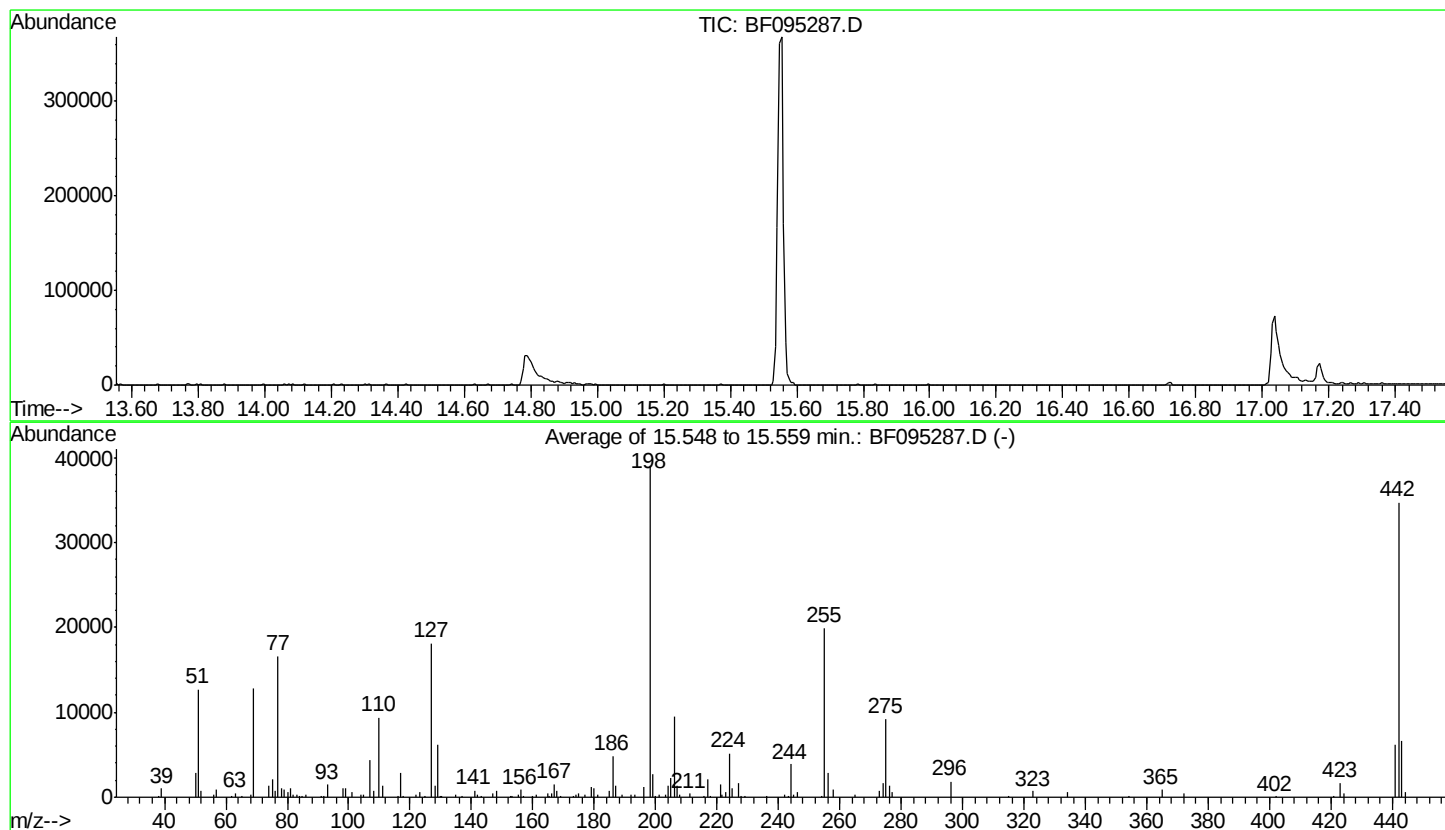

AutoFind: Scans 2314, 2315, 2316; Background Corrected with Scan 2308

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.6	12735	PASS
68	69	0.00	2	1.8	233	PASS
69	198	0.00	100	33.0	12891	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.4	18101	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	39045	PASS
199	198	5	9	7.0	2726	PASS
275	198	10	60	23.6	9231	PASS
365	198	1	100	2.2	866	PASS
441	442	0.01	24	17.8	6172	PASS
442	198	50	100	88.9	34701	PASS
443	442	15	24	19.2	6663	PASS