

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF051920\
 Data File : BF120359.D
 Acq On : 19 May 2020 13:07
 Operator : MA/SJ
 Sample : PB128986BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB128986BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051420.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.416	219	226	238	rBV	77221	160634	1.76%	0.284%
2	5.199	525	529	559	rBV	5595721	6421551	70.27%	11.351%
3	6.251	703	708	737	rBV	5322954	6596752	72.19%	11.661%
4	6.593	762	766	788	rBV	1192232	1472557	16.11%	2.603%
5	6.751	788	793	822	rVV	5062617	5405215	59.15%	9.555%
6	7.163	858	863	882	rBV	3164834	4056497	44.39%	7.171%
7	7.881	980	985	1013	rBV	1620203	1861722	20.37%	3.291%
8	8.963	1163	1169	1172	rBV	6708687	6957682	76.14%	12.299%
9	9.634	1278	1283	1303	rBV	2145551	2178795	23.84%	3.851%
10	10.428	1412	1418	1435	rBV	4228413	4675861	51.17%	8.266%
11	11.116	1531	1535	1556	rBV	2110687	2347108	25.68%	4.149%
12	12.716	1801	1807	1810	rBV	7804072	9138073	100.00%	16.154%
13	13.633	1960	1963	1968	rVB	142211	150589	1.65%	0.266%
14	13.757	1980	1984	1995	rBV	2459966	2653593	29.04%	4.691%
15	15.151	2216	2221	2234	rBV	1810698	2373899	25.98%	4.196%
16	15.568	2288	2292	2298	rVB2	74562	119625	1.31%	0.211%


Sum of corrected areas: 56570153

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF051920\
Data File : BF120359.D
Acq On : 19 May 2020 13:07
Operator : MA/SJ
Sample : PB128986BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB128986BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

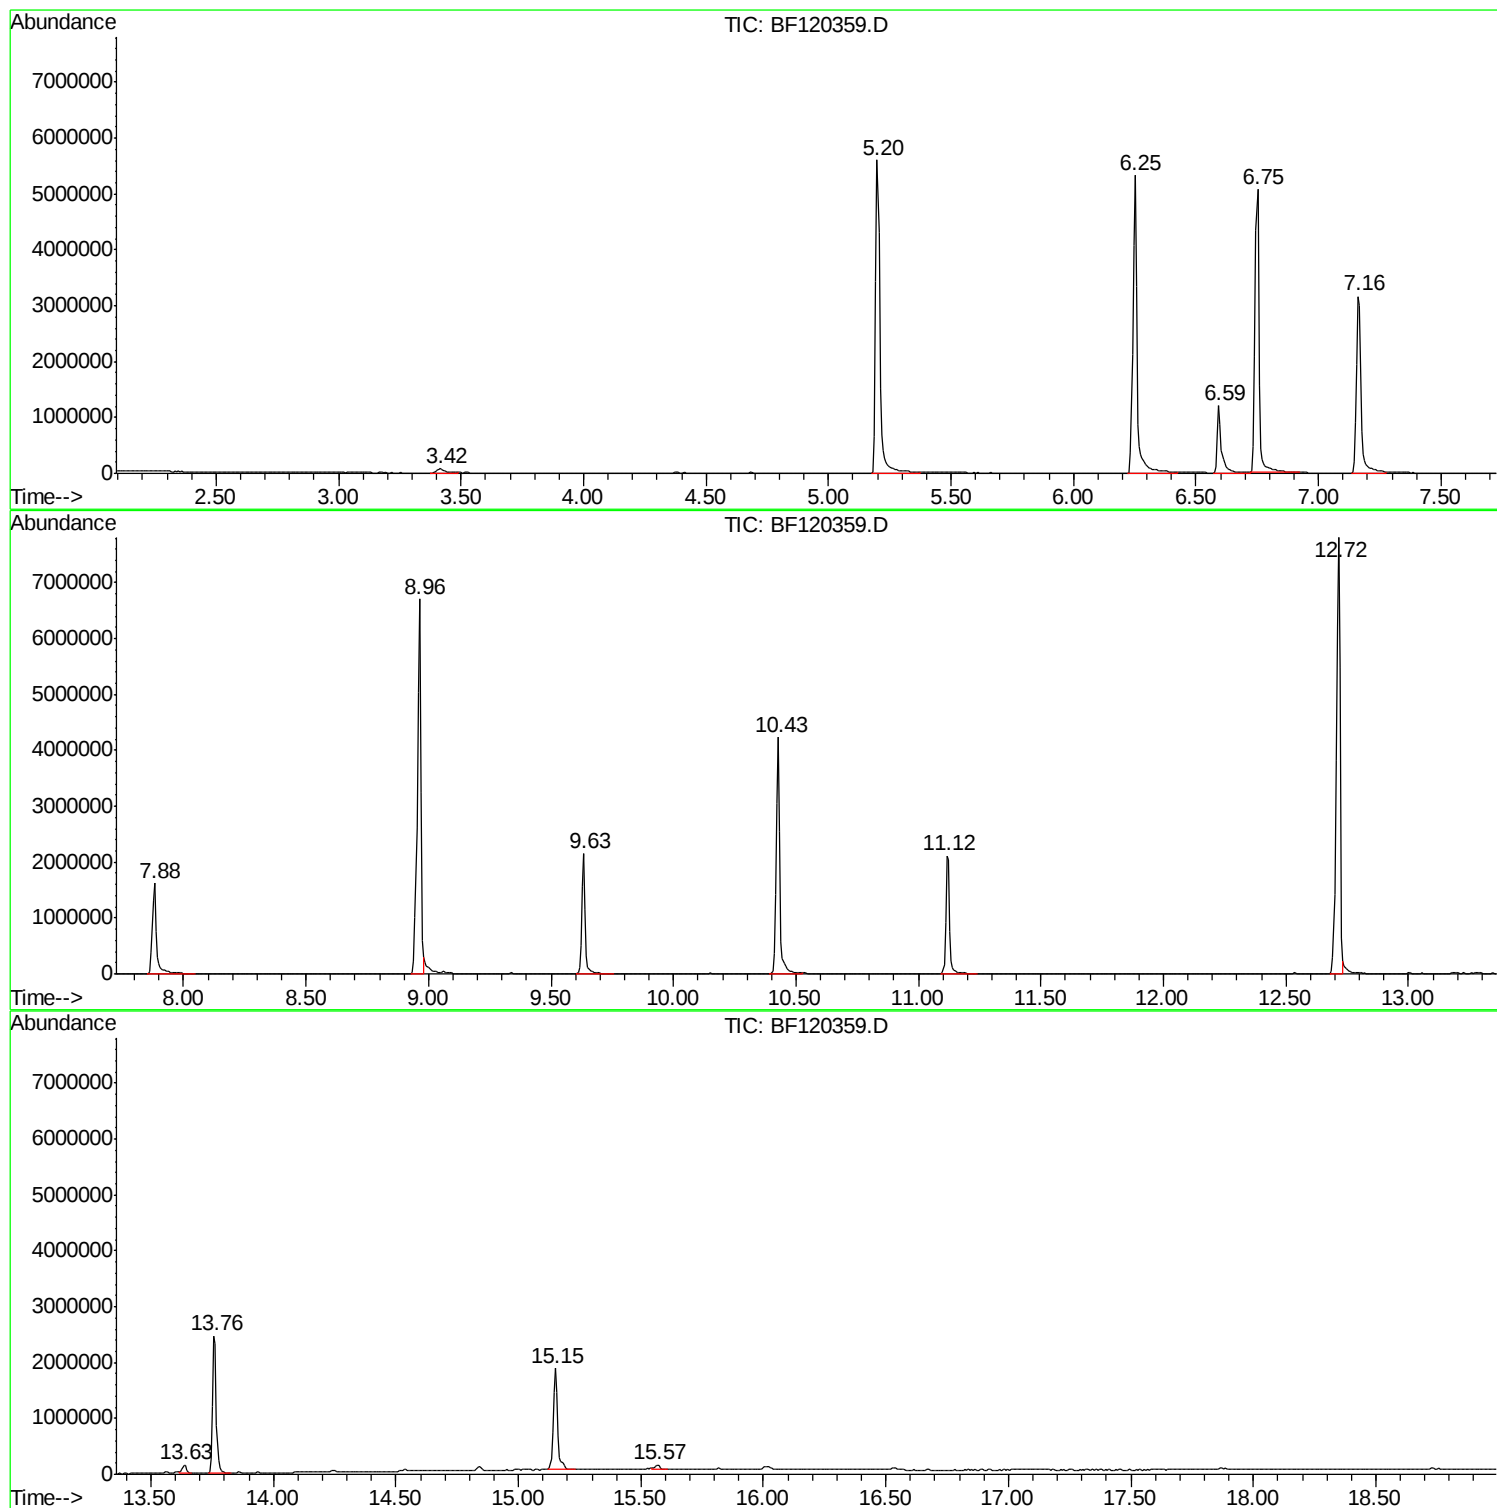

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF051920\
Data File : BF120359.D
Acq On : 19 May 2020 13:07
Operator : MA/SJ
Sample : PB128986BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB128986BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF051920\
Data File : BF120359.D
Acq On : 19 May 2020 13:07
Operator : MA/SJ
Sample : PB128986BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB128986BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc