


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051920\
 Data File : BF120357.D
 Acq On : 19 May 2020 11:35
 Operator : MA/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051420.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue May 19 13:17:29 2020

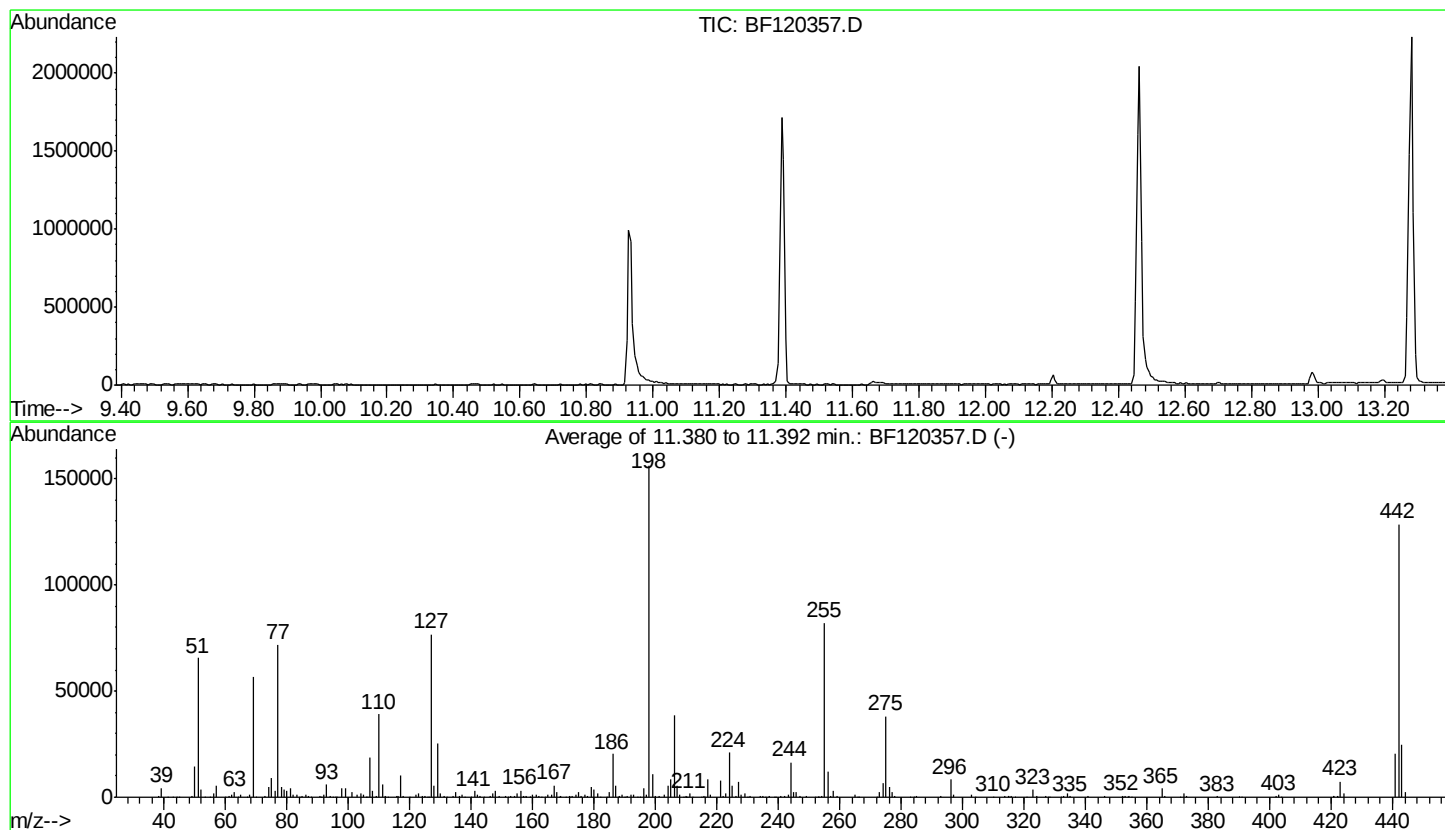

AutoFind: Scans 1580, 1581, 1582; Background Corrected with Scan 1575

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.0	65576	PASS
68	69	0.00	2	1.7	964	PASS
69	198	0.00	100	36.3	56733	PASS
70	69	0.00	2	0.5	282	PASS
127	198	10	80	49.1	76693	PASS
197	198	0.00	2	0.6	1015	PASS
198	198	100	100	100.0	156194	PASS
199	198	5	9	7.0	10920	PASS
275	198	10	60	24.5	38216	PASS
365	198	1	100	2.5	3967	PASS
441	198	0.01	100	13.3	20729	PASS
442	198	50	100	82.2	128458	PASS
443	442	15	24	19.4	24979	PASS