
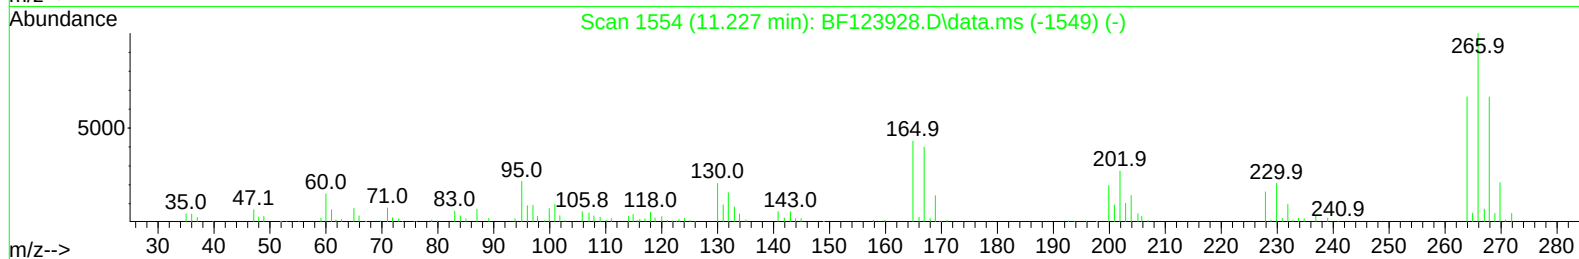
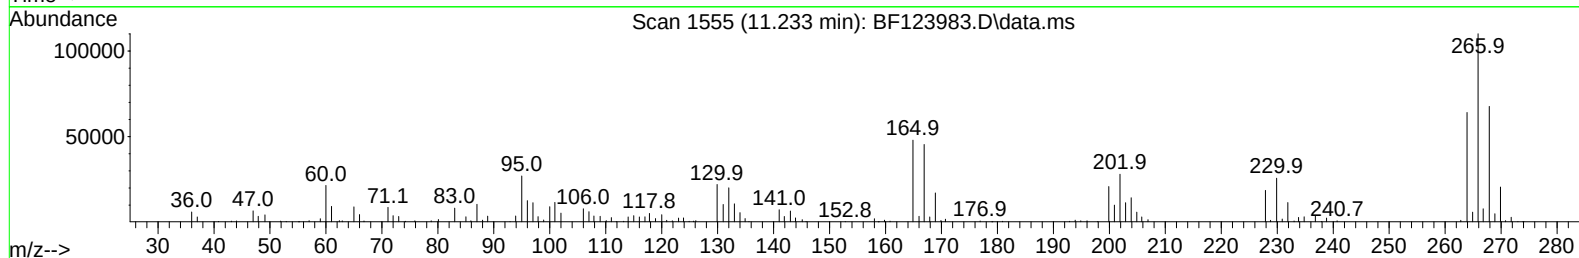


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051921\
Data File : BF123983.D
Acq On : 19 May 2021 10:48
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 19 12:49:55 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 14 19:05:57 2021
Response via : Initial Calibration

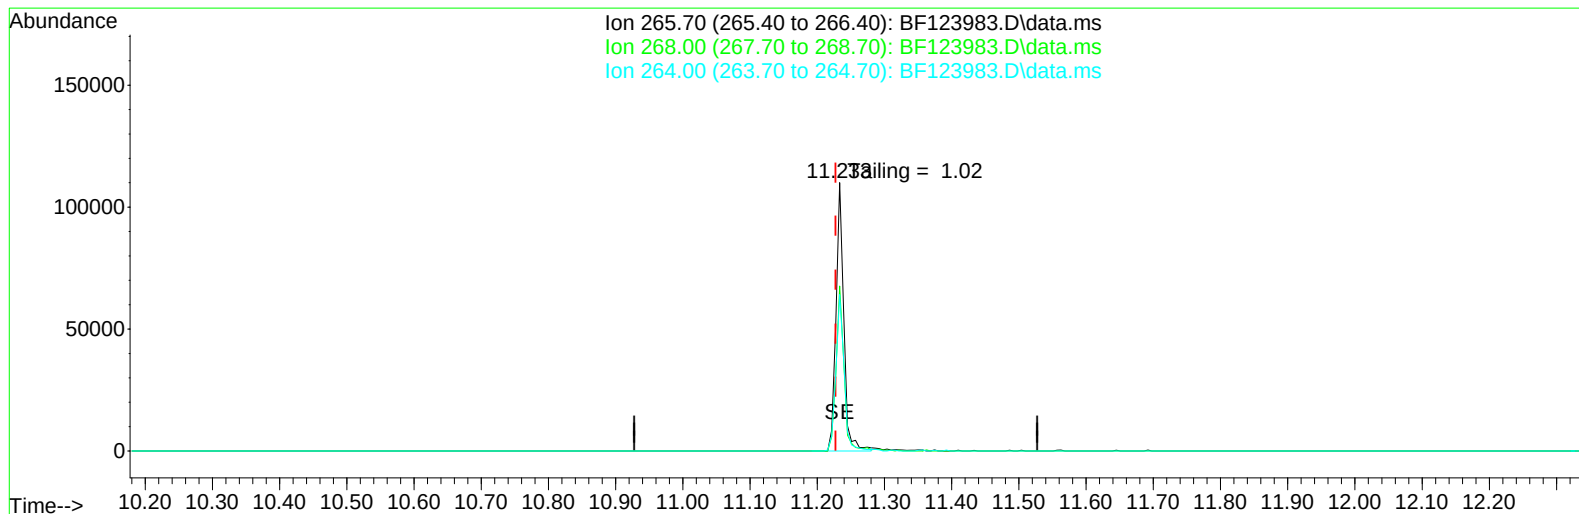

TIC: BF123983.D\data.ms

(70) Pentachlorophenol (C)




11.233min (+ 0.006) 25558.29 ng

response 91145

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	61.49
264.00	65.70	58.25
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051921\
Data File : BF123983.D
Acq On : 19 May 2021 10:48
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 19 12:49:55 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 14 19:05:57 2021
Response via : Initial Calibration

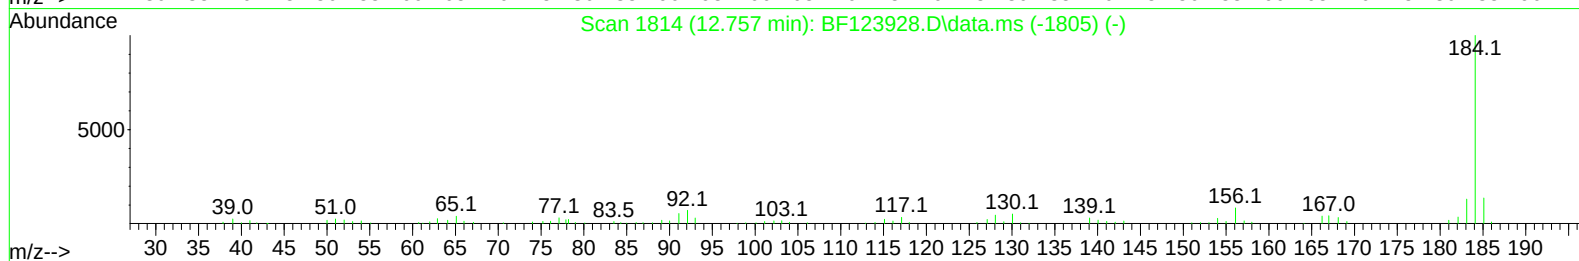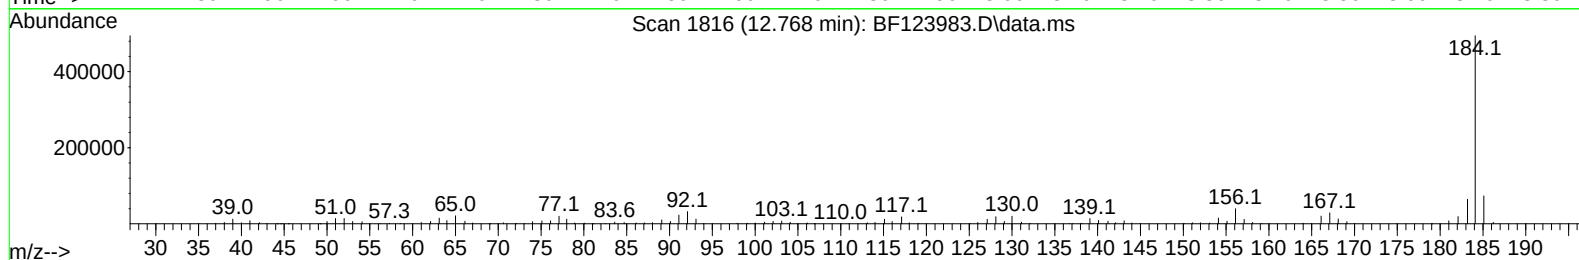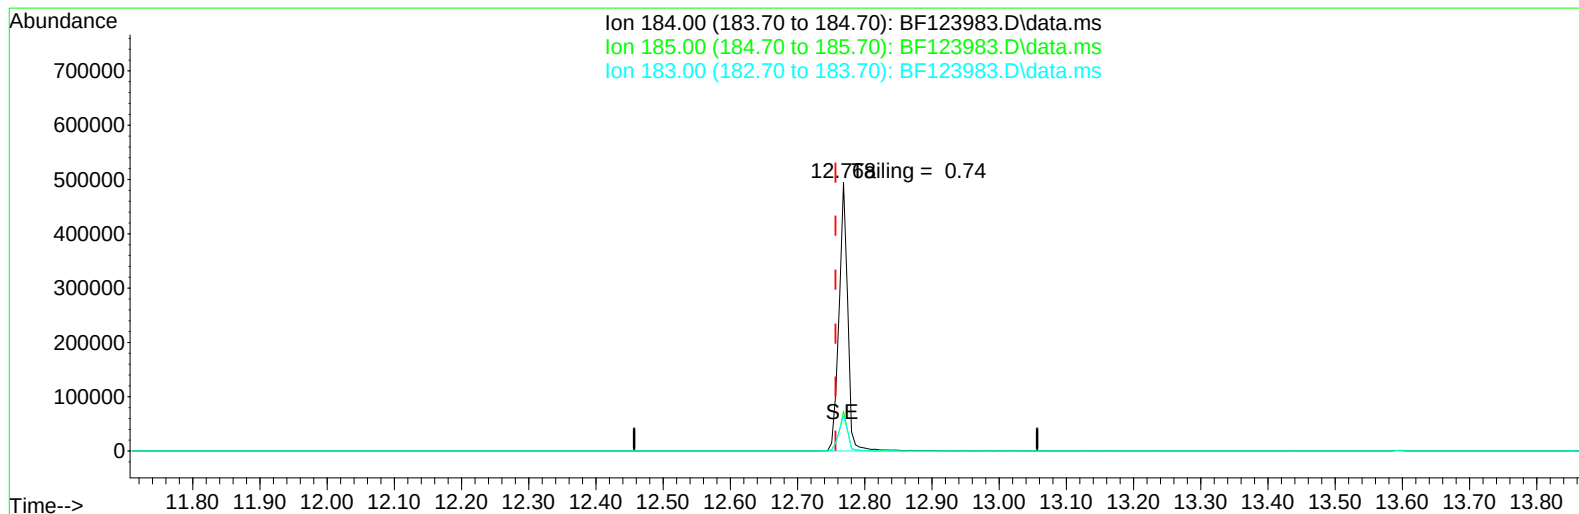

TIC: BF123983.D\data.ms

(77) Benzidine

12.768min (+ 0.012) 0.00 ng

response 446390

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.89
183.00	9.80	13.08#
0.00	0.00	0.00