

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051921\
 Data File : BF123998.D
 Acq On : 19 May 2021 19:30
 Operator : JU/CG
 Sample : M2437-05 5X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TP-2

Manual Integrations
 APPROVED

mohammad
 5/20/2021 11:35:09 AM

Quant Time: May 20 02:26:46 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 14 19:05:57 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.904	152	45088	20.00	ng	0.00
21) Naphthalene-d8	8.186	136	175570	20.00	ng	# 0.00
39) Acenaphthene-d10	9.945	164	92610	20.00	ng	0.00
64) Phenanthrene-d10	11.427	188	145859	20.00	ng	# 0.00
76) Chrysene-d12	14.074	240	104787	20.00	ng	0.00
86) Perylene-d12	15.562	264	75656	20.00	ng	0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.510	112	60603	18.87	ng	0.00
7) Phenol-d6	6.516	99	76884	18.46	ng	0.00
23) Nitrobenzene-d5	7.457	82	57131	14.02	ng	0.00
42) 2,4,6-Tribromophenol	10.727	330	19141	17.21	ng	0.00
45) 2-Fluorobiphenyl	9.263	172	102158	13.57	ng	0.00
79) Terphenyl-d14	13.016	244	79237	11.45	ng	0.00
Target Compounds						Qvalue
71) Phenanthrene	11.451	178	60990m	6.60	ng	
75) Fluoranthene	12.645	202	94889	9.91	ng	97
78) Pyrene	12.874	202	136704	14.69	ng	98
81) Benzo(a)anthracene	14.063	228	59471m	7.85	ng	
83) Chrysene	14.098	228	63347	8.69	ng	97
87) Indeno(1,2,3-cd)pyrene	17.062	276	28673	4.91	ng	94
88) Benzo(b)fluoranthene	15.127	252	65176m	11.14	ng	
89) Benzo(k)fluoranthene	15.151	252	15694m	2.94	ng	
90) Benzo(a)pyrene	15.498	252	57884	11.44	ng	97
92) Benzo(g,h,i)perylene	17.521	276	36733	7.44	ng	# 88

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051921\
Data File : BF123998.D
Acq On : 19 May 2021 19:30
Operator : JU/CG
Sample : M2437-05 5X
Misc :
ALS Vial : 16 Sample Multiplier: 1


Instrument :
BNA_F
ClientSampled :
TP-2

Manual Integrations
APPROVED

mohammad
5/20/2021 11:35:09 AM

Quant Time: May 20 02:26:46 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 14 19:05:57 2021
Response via : Initial Calibration

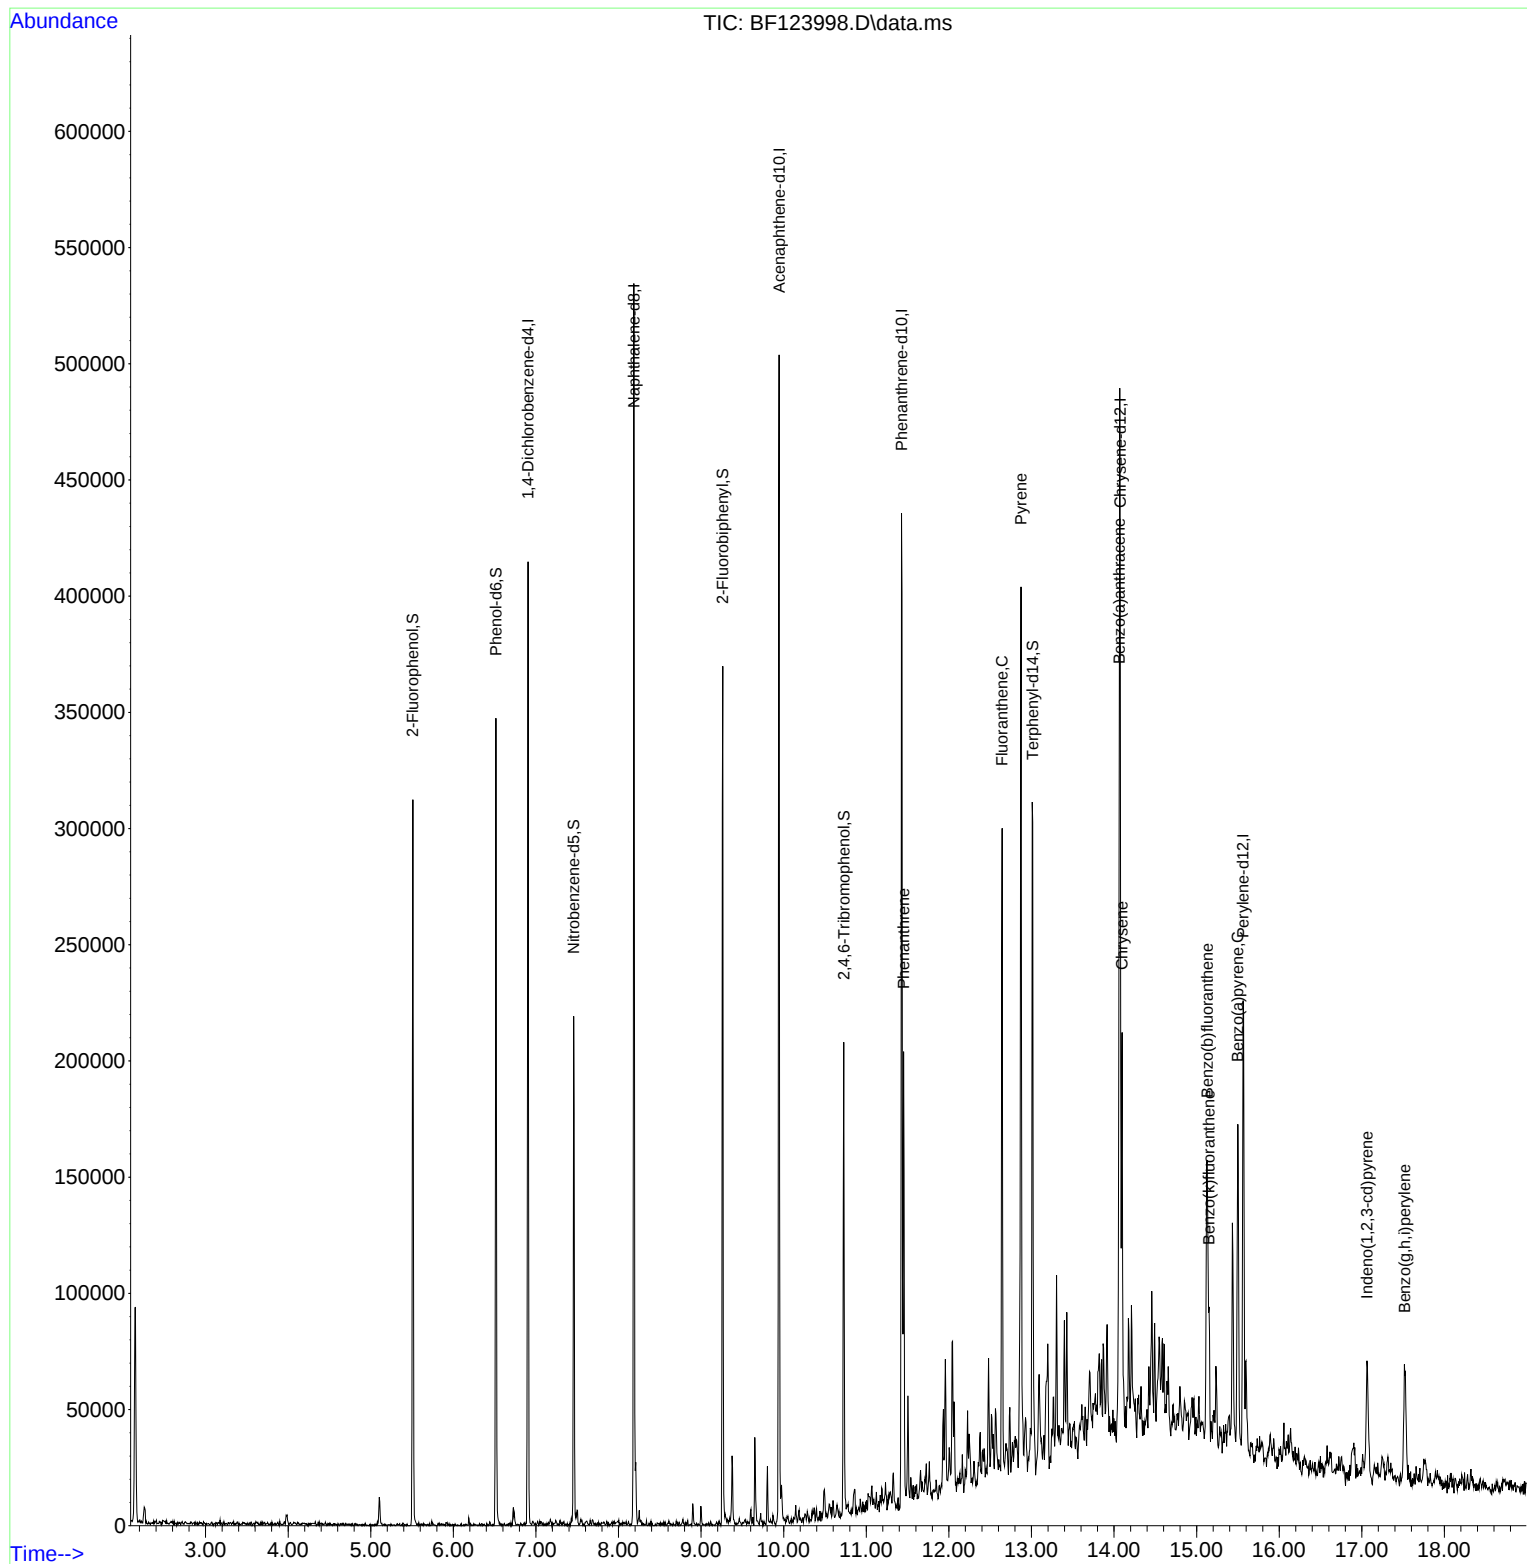

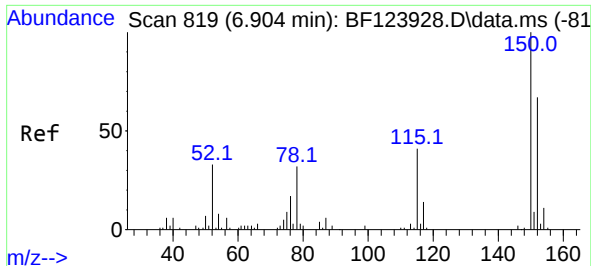





#1
1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.904 min Scan# 819
Delta R.T. 0.000 min
Lab File: BF123998.D
Acq: 19 May 2021 19:30

Tgt Ion:152 Resp: 45088
Ion Ratio Lower Upper
152 100
150 157.1 127.0 190.6
115 65.1 54.3 81.5

Instrument :
BNA_F
ClientSampleId :
TP-2




Manual Integrations
APPROVED


mohammad
5/20/2021 11:35:09 AM

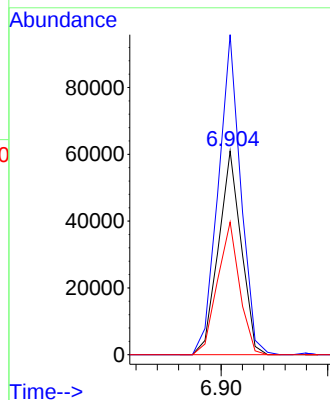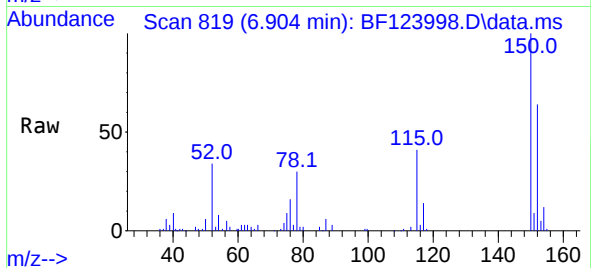

#5
2-Fluorophenol
Concen: 18.87 ng
RT: 5.510 min Scan# 582
Delta R.T. 0.000 min
Lab File: BF123998.D
Acq: 19 May 2021 19:30

Tgt Ion:112 Resp: 60603
Ion Ratio Lower Upper
112 100
64 71.5 61.4 92.0
63 43.5 33.0 49.4

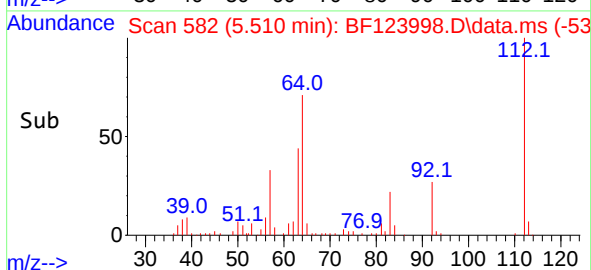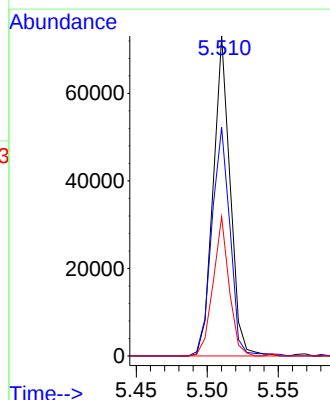

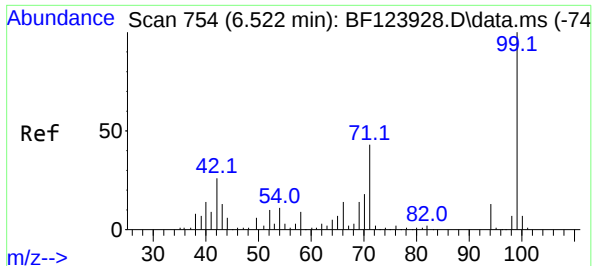





#7
Phenol-d6
Concen: 18.46 ng
RT: 6.516 min Scan# 753
Delta R.T. -0.006 min
Lab File: BF123998.D
Acq: 19 May 2021 19:30

Tgt Ion:	99	Resp:	76884
Ion	Ratio	Lower	Upper
99	100		
42	26.9	19.8	29.8
71	44.7	31.1	46.7

Instrument :
BNA_F
ClientSampled :
TP-2




Manual Integrations
APPROVED


mohammad
5/20/2021 11:35:09 AM

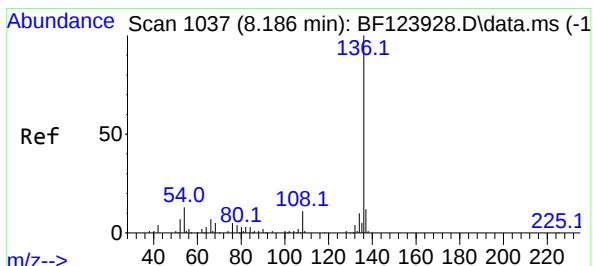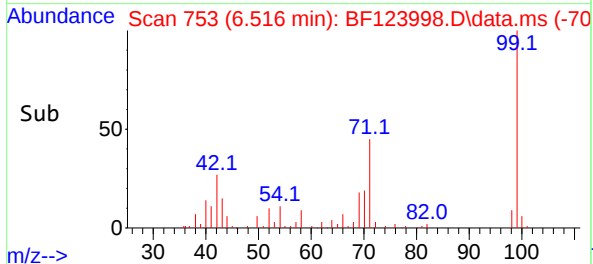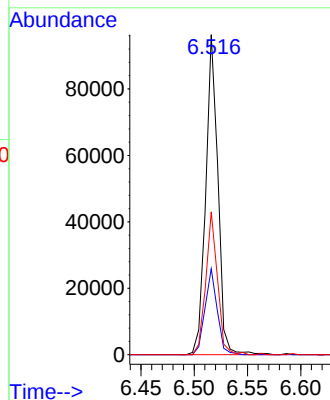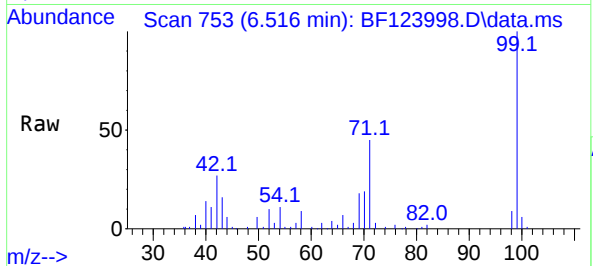


#21
Naphthalene-d8
Concen: 20.00 ng
RT: 8.186 min Scan# 1037
Delta R.T. 0.000 min
Lab File: BF123998.D
Acq: 19 May 2021 19:30

Tgt Ion:	136	Resp:	175570
Ion	Ratio	Lower	Upper
136	100		
137	11.3	8.7	13.1
54	13.7	9.8	14.6
68	6.5	4.1	6.1

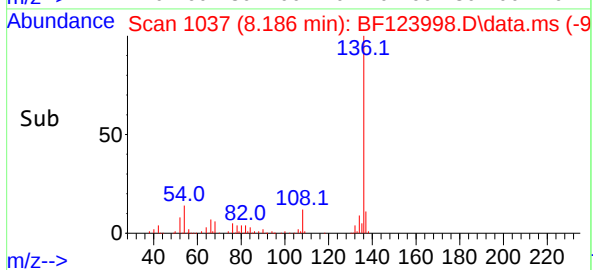
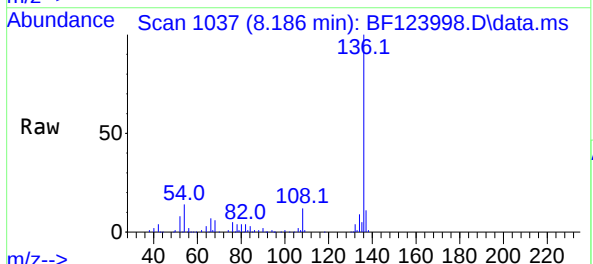
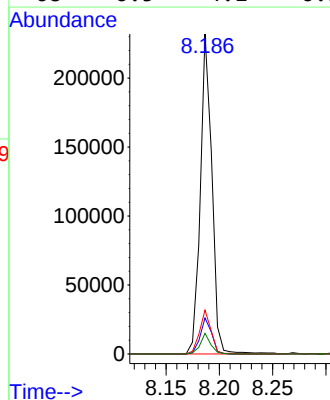


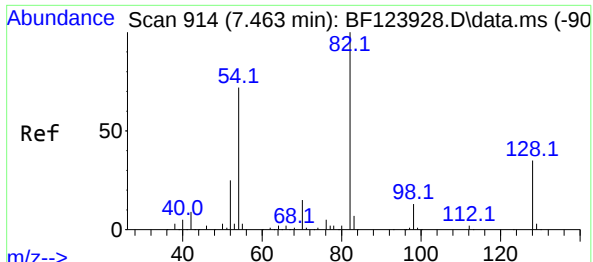


#23
Nitrobenzene-d5
Concen: 14.02 ng
RT: 7.457 min Scan# 913
Delta R.T. -0.006 min
Lab File: BF123998.D
Acq: 19 May 2021 19:30

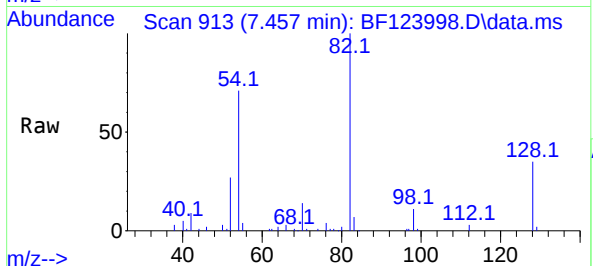



Tgt Ion: 82 Resp: 57131
Ion Ratio Lower Upper
82 100
128 34.6 29.4 44.2
54 71.0 54.1 81.1

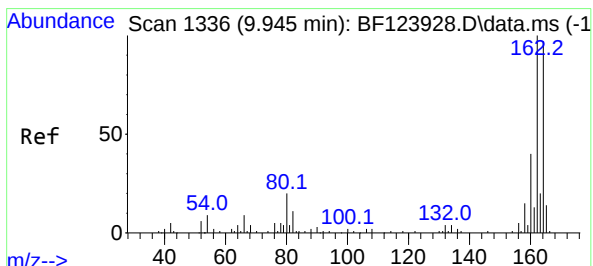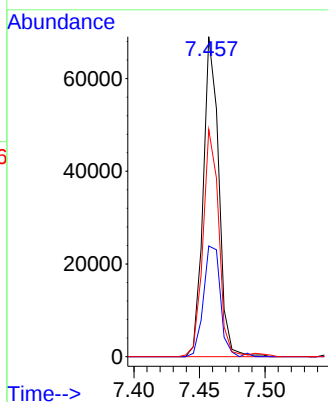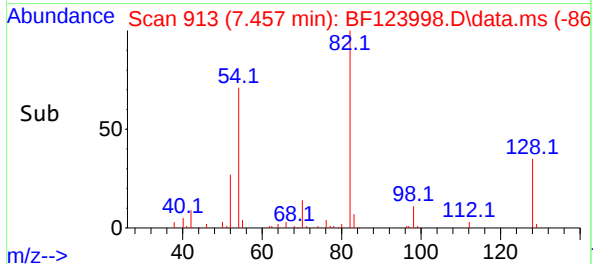

#39
Acenaphthene-d10
Concen: 20.00 ng
RT: 9.945 min Scan# 1336
Delta R.T. 0.000 min
Lab File: BF123998.D
Acq: 19 May 2021 19:30

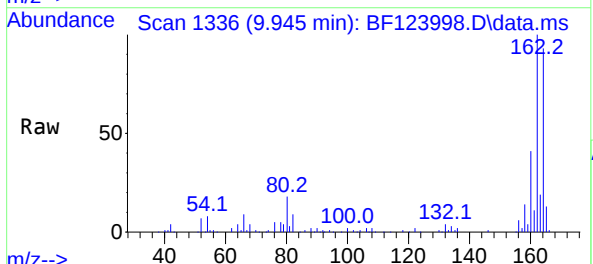


Tgt Ion: 164 Resp: 92610
Ion Ratio Lower Upper
164 100
162 107.6 80.7 121.1
160 43.9 37.3 55.9

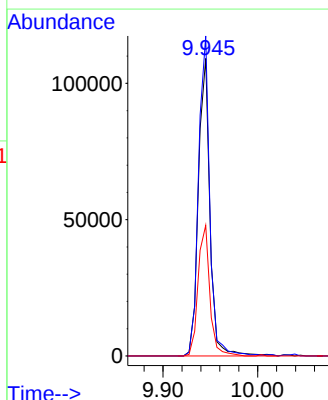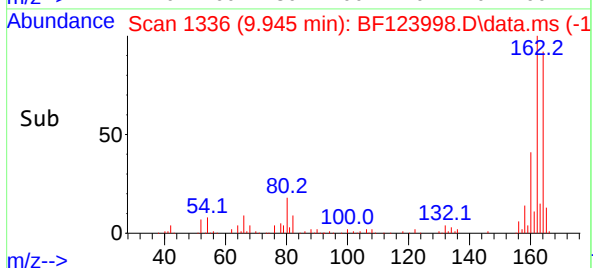

Instrument :
BNA_F
ClientSampleId :
TP-2


Manual Integrations
APPROVED

mohammad
5/20/2021 11:35:09 AM

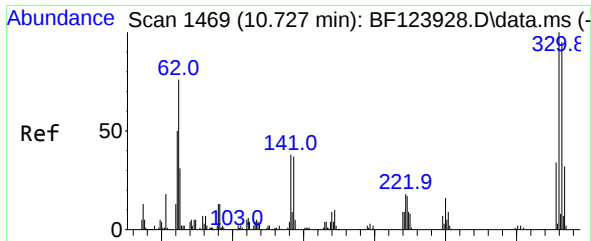

#42
2,4,6-Tribromophenol
Concen: 17.21 ng
RT: 10.727 min Scan# 1469
Delta R.T. 0.000 min
Lab File: BF123998.D
Acq: 19 May 2021 19:30




Instrument :
BNA_F
ClientSampled :
TP-2

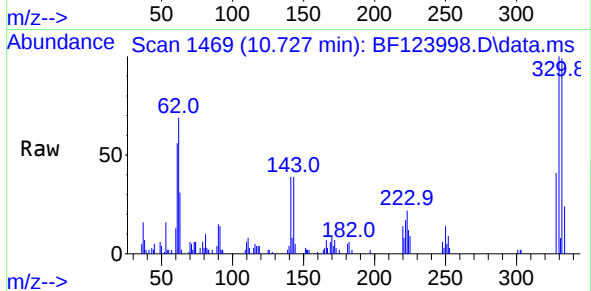


Tgt Ion: 330 Resp: 19141
Ion Ratio Lower Upper
330 100
332 95.5 77.1 115.7
141 36.4 27.9 41.9

Manual Integrations
APPROVED



mohammad
5/20/2021 11:35:09 AM

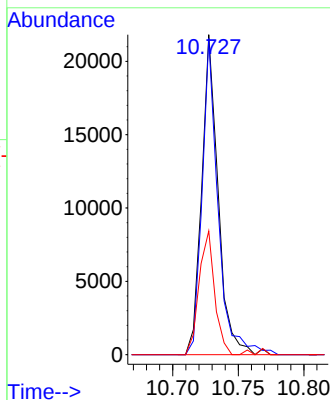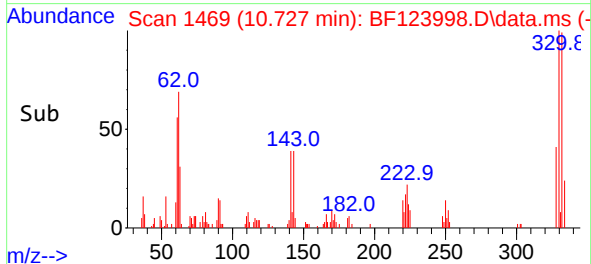


#45
2-Fluorobiphenyl
Concen: 13.57 ng
RT: 9.263 min Scan# 1220
Delta R.T. 0.000 min
Lab File: BF123998.D
Acq: 19 May 2021 19:30

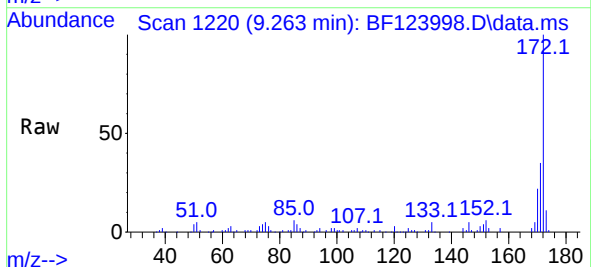


Tgt Ion: 172 Resp: 102158
Ion Ratio Lower Upper
172 100
171 34.7 28.1 42.1
170 21.8 19.2 28.8

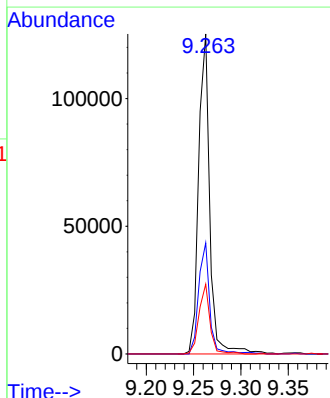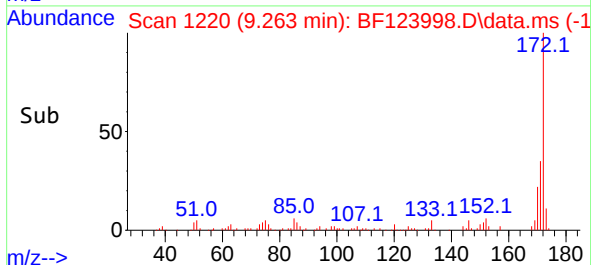



#64
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.427 min Scan# 1588
Delta R.T. 0.000 min
Lab File: BF123998.D
Acq: 19 May 2021 19:30




Instrument :
BNA_F
ClientSampled :
TP-2

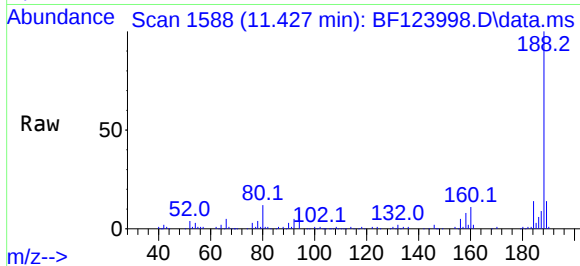


Tgt Ion:188 Resp: 145859
Ion Ratio Lower Upper
188 100
94 8.7 6.9 10.3
80 12.3 8.2 12.2#

Manual Integrations
APPROVED



mohammad
5/20/2021 11:35:09 AM

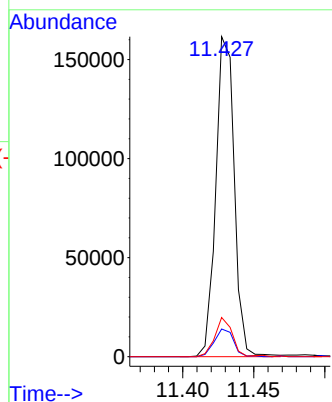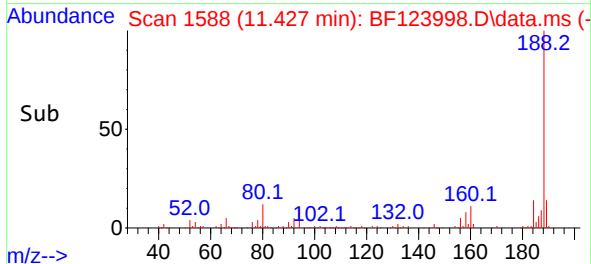


#71
Phenanthrene
Concen: 6.60 ng m
RT: 11.451 min Scan# 1592
Delta R.T. 0.000 min
Lab File: BF123998.D
Acq: 19 May 2021 19:30

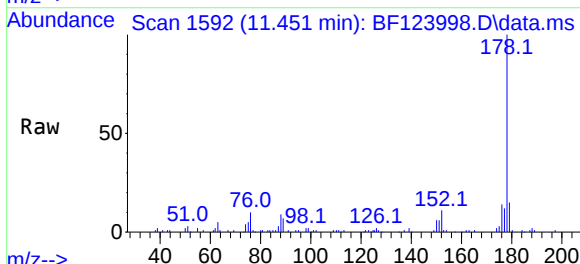


Tgt Ion:178 Resp: 60990
Ion Ratio Lower Upper
178 100
176 14.2 15.6 23.4#
179 15.1 12.5 18.7


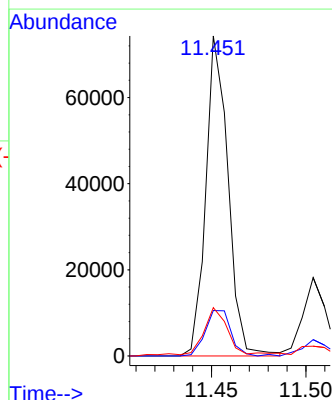
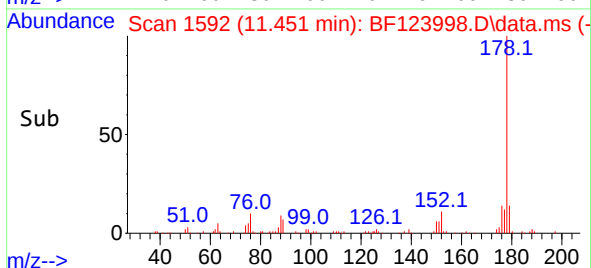





#75
Fluoranthene
Concen: 9.91 ng
RT: 12.645 min Scan# 1795
Delta R.T. 0.006 min
Lab File: BF123998.D
Acq: 19 May 2021 19:30

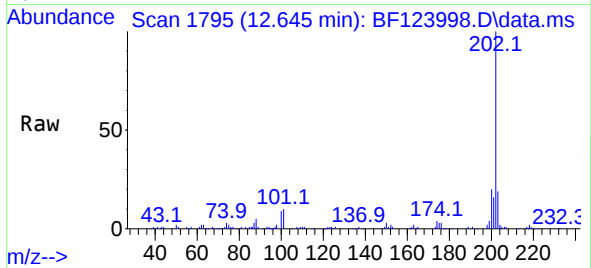



Tgt Ion:202 Resp: 94889
Ion Ratio Lower Upper
202 100
101 9.7 0.0 30.9
203 18.7 0.0 37.5

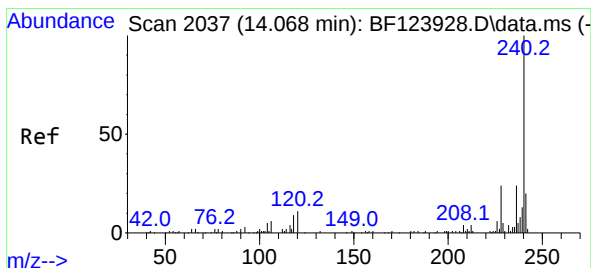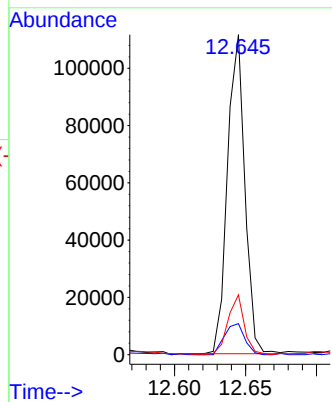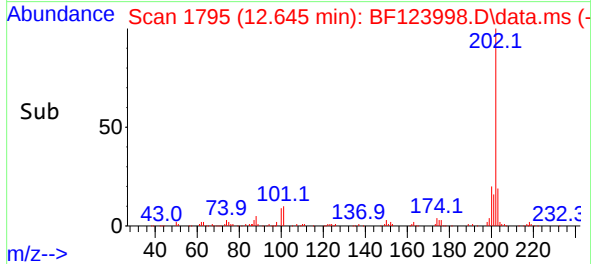

#76
Chrysene-d12
Concen: 20.00 ng
RT: 14.074 min Scan# 2038
Delta R.T. 0.006 min
Lab File: BF123998.D
Acq: 19 May 2021 19:30

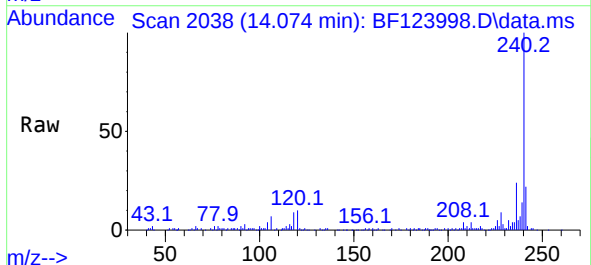


Tgt Ion:240 Resp: 104787
Ion Ratio Lower Upper
240 100
120 10.1 7.2 10.8
236 24.3 19.0 28.4

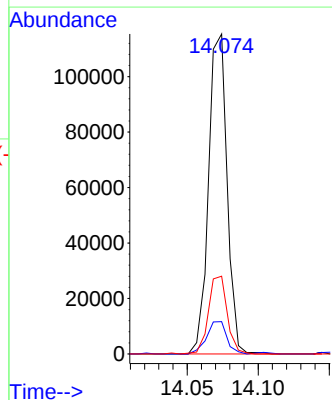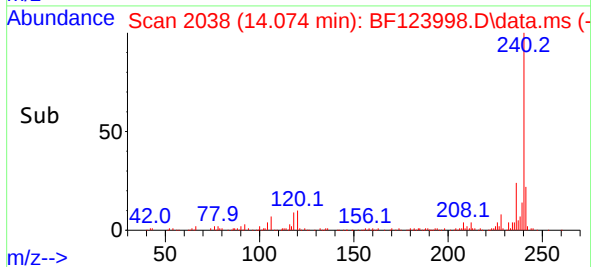


Instrument :
BNA_F
ClientSampled :
TP-2

Manual Integrations
APPROVED




mohammad
5/20/2021 11:35:09 AM




#78
Pyrene
Concen: 14.69 ng
RT: 12.874 min Scan# 1834
Delta R.T. 0.006 min
Lab File: BF123998.D
Acq: 19 May 2021 19:30





Tgt Ion:202 Resp: 136704
Ion Ratio Lower Upper
202 100
200 20.5 16.1 24.1
203 17.2 14.8 22.2

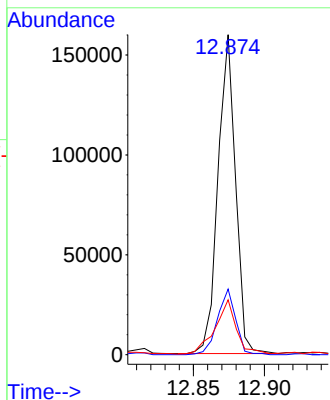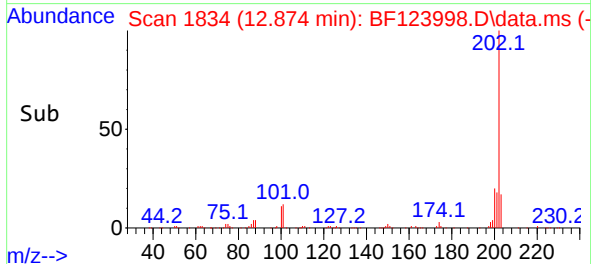

#79
Terphenyl-d14
Concen: 11.45 ng
RT: 13.016 min Scan# 1858
Delta R.T. 0.000 min
Lab File: BF123998.D
Acq: 19 May 2021 19:30

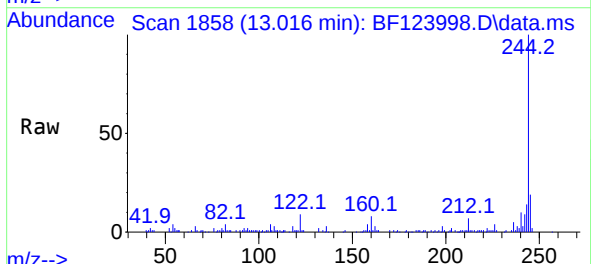


Tgt Ion:244 Resp: 79237
Ion Ratio Lower Upper
244 100
212 6.7 5.7 8.5
122 8.7 9.7 14.5#

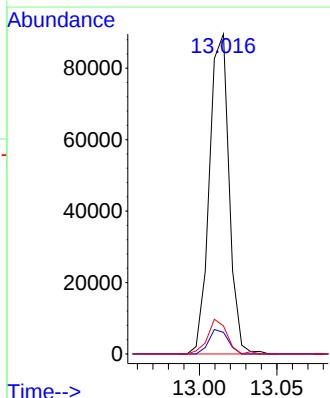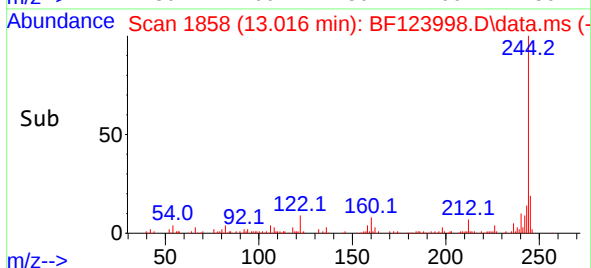

Instrument :
BNA_F
ClientSampled :
TP-2

Manual Integrations
APPROVED

mohammad
5/20/2021 11:35:09 AM







#81
Benzo(a)anthracene
Concen: 7.85 ng m
RT: 14.063 min Scan# 2036
Delta R.T. 0.006 min
Lab File: BF123998.D
Acq: 19 May 2021 19:30

Tgt Ion:228 Resp: 59471
Ion Ratio Lower Upper
228 100
226 35.8 22.4 33.6#
229 19.9 16.0 24.0

Instrument :
BNA_F
ClientSampled :
TP-2




Manual Integrations
APPROVED


mohammad
5/20/2021 11:35:09 AM

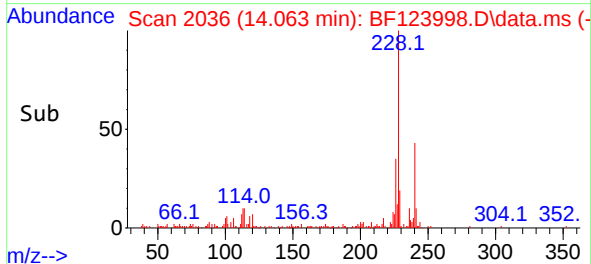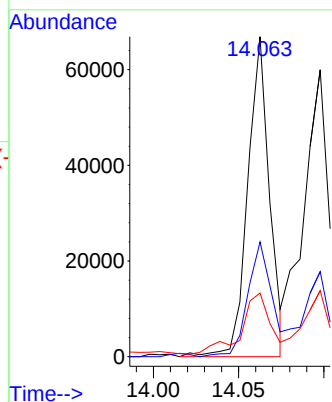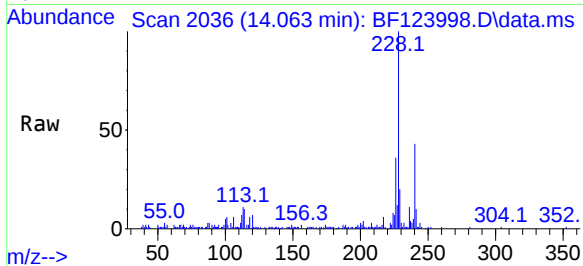

#83
Chrysene
Concen: 8.69 ng
RT: 14.098 min Scan# 2042
Delta R.T. 0.000 min
Lab File: BF123998.D
Acq: 19 May 2021 19:30

Tgt Ion:228 Resp: 63347
Ion Ratio Lower Upper
228 100
226 29.7 24.3 36.5
229 23.0 16.2 24.2

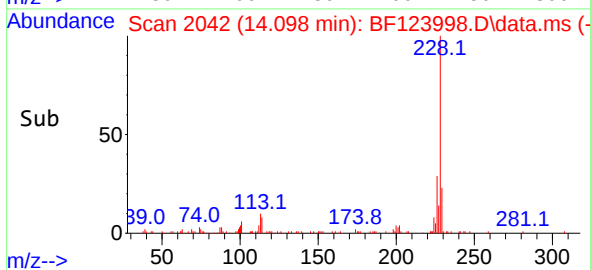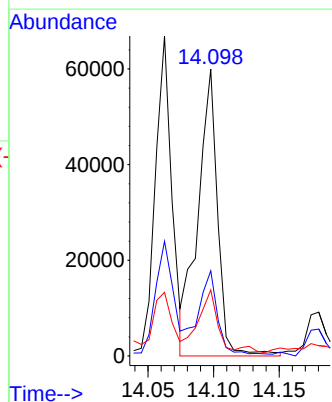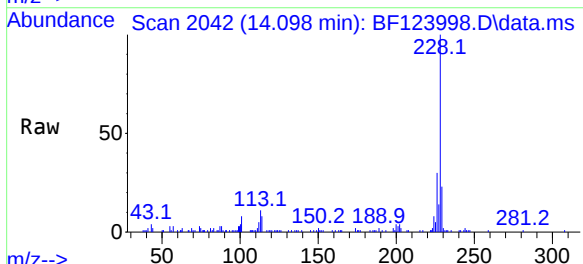

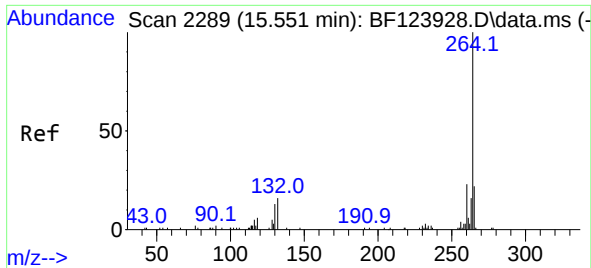





#86
Perylene-d12
Concen: 20.00 ng
RT: 15.562 min Scan# 2291
Delta R.T. 0.012 min
Lab File: BF123998.D
Acq: 19 May 2021 19:30

Tgt Ion:	264	Resp:	75656
Ion Ratio	Lower	Upper	
264	100		
260	26.8	18.7	28.1
265	21.2	17.8	26.8

Instrument :
BNA_F
ClientSampled :
TP-2




Manual Integrations
APPROVED


mohammad
5/20/2021 11:35:09 AM

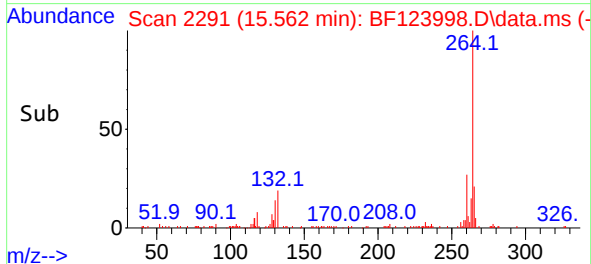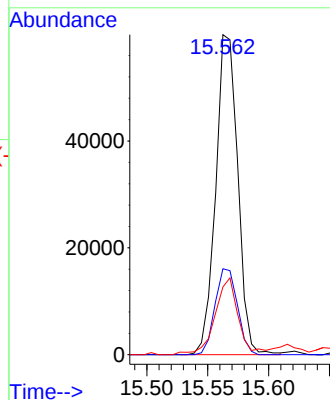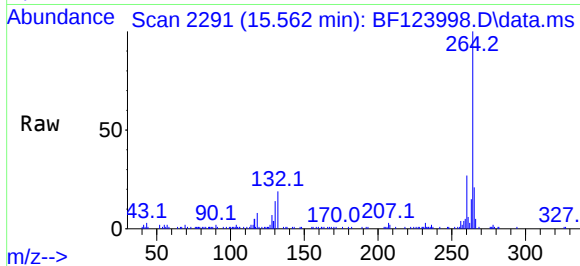


#87
Indeno(1,2,3-cd)pyrene
Concen: 4.91 ng
RT: 17.062 min Scan# 2546
Delta R.T. 0.006 min
Lab File: BF123998.D
Acq: 19 May 2021 19:30

Tgt Ion:	276	Resp:	28673
Ion Ratio	Lower	Upper	
276	100		
138	23.8	16.2	24.2
277	27.0	20.1	30.1

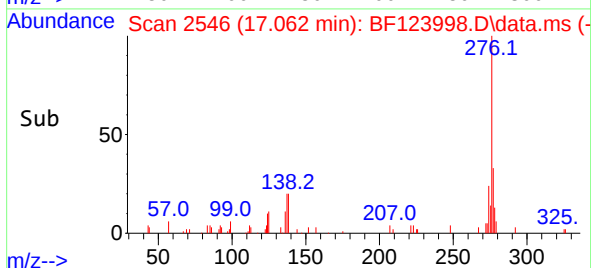
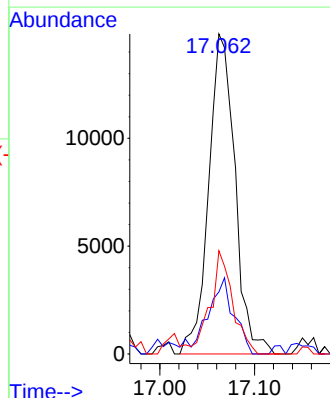
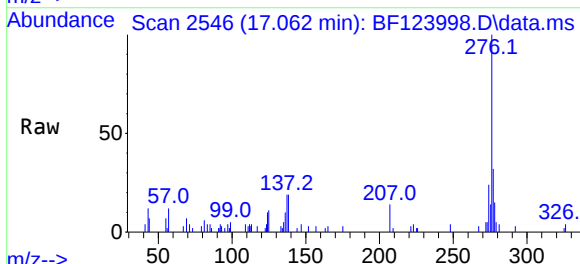





#88
Benzo(b)fluoranthene
Concen: 11.14 ng m
RT: 15.127 min Scan# 2217
Delta R.T. 0.012 min
Lab File: BF123998.D
Acq: 19 May 2021 19:30

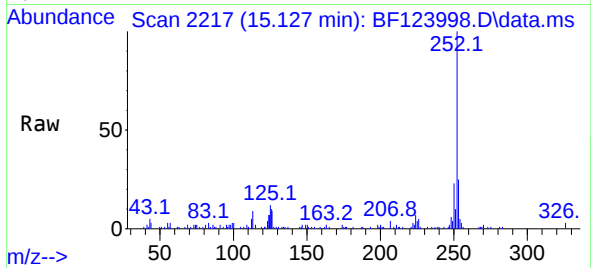



Tgt Ion:252 Resp: 65176
Ion Ratio Lower Upper
252 100
253 25.1 18.1 27.1
125 12.0 6.2 9.4#

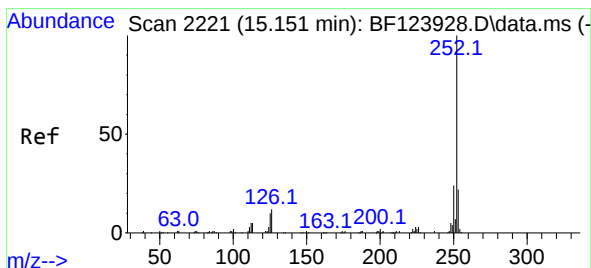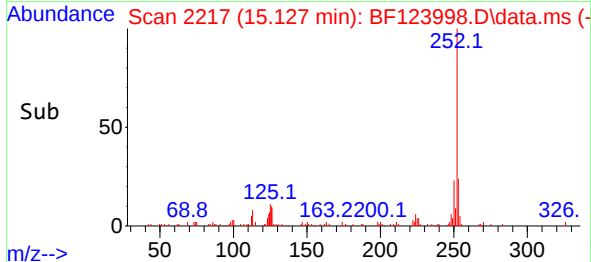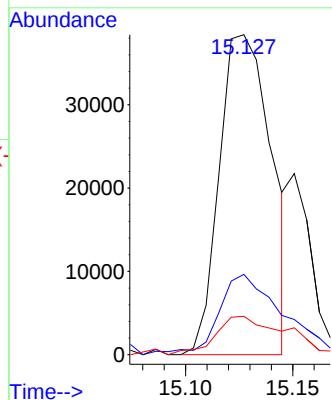

#89
Benzo(k)fluoranthene
Concen: 2.94 ng m
RT: 15.151 min Scan# 2221
Delta R.T. 0.000 min
Lab File: BF123998.D
Acq: 19 May 2021 19:30

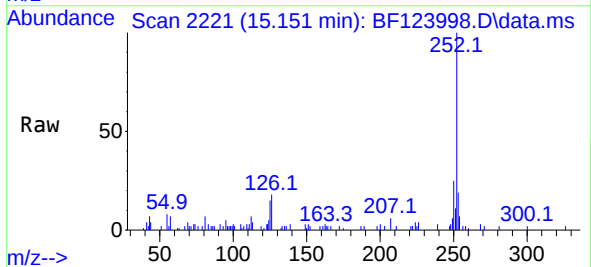


Tgt Ion:252 Resp: 15694
Ion Ratio Lower Upper
252 100
253 19.4 17.9 26.9
125 14.8 7.0 10.6#

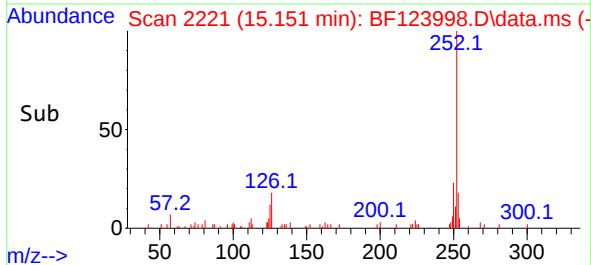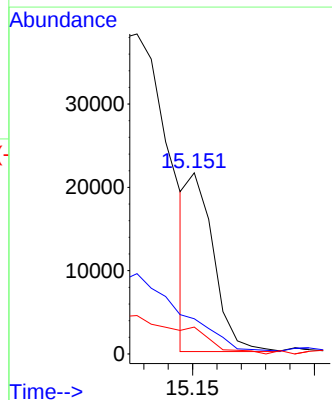

Instrument :
BNA_F
ClientSampled :
TP-2

Manual Integrations
APPROVED

mohammad
5/20/2021 11:35:09 AM







#90
Benzo(a)pyrene
Concen: 11.44 ng
RT: 15.498 min Scan# 2280
Delta R.T. 0.006 min
Lab File: BF123998.D
Acq: 19 May 2021 19:30

Tgt Ion:	252	Resp:	57884
Ion Ratio	Lower	Upper	
252	100		
253	24.5	18.4	27.6
125	9.4	8.0	12.0

Instrument :
BNA_F
ClientSampled :
TP-2

Manual Integrations
APPROVED

mohammad
5/20/2021 11:35:09 AM

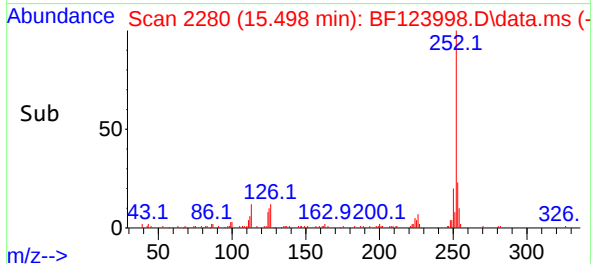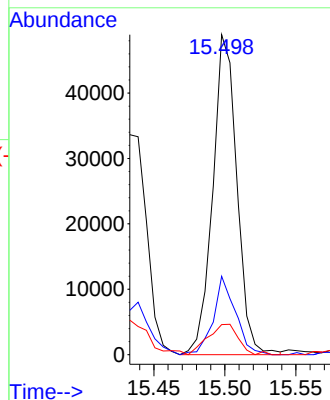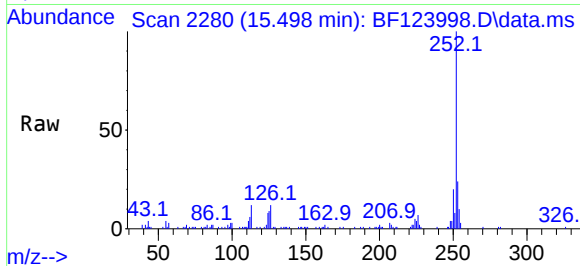

#92
Benzo(g,h,i)perylene
Concen: 7.44 ng
RT: 17.521 min Scan# 2624
Delta R.T. 0.012 min
Lab File: BF123998.D
Acq: 19 May 2021 19:30

Tgt Ion:	276	Resp:	36733
Ion Ratio	Lower	Upper	
276	100		
277	19.9	18.2	27.2
138	25.5	13.8	20.6#

