

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051921\
 Data File : BF124000.D
 Acq On : 19 May 2021 20:37
 Operator : JU/CG
 Sample : M2438-01 5X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PL-02-051821

Manual Integrations
 APPROVED

mohammad
 5/20/2021 11:35:14 AM

Quant Time: May 20 02:27:08 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 14 19:05:57 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.904	152	45407	20.00	ng	0.00
21) Naphthalene-d8	8.186	136	175657	20.00	ng	# 0.00
39) Acenaphthene-d10	9.945	164	89782	20.00	ng	0.00
64) Phenanthrene-d10	11.433	188	135431	20.00	ng	0.00
76) Chrysene-d12	14.074	240	98593	20.00	ng	0.00
86) Perylene-d12	15.568	264	70554	20.00	ng	0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.504	112	35759	11.06	ng	0.00
7) Phenol-d6	6.516	99	44957	10.72	ng	0.00
23) Nitrobenzene-d5	7.457	82	32998	8.09	ng	0.00
42) 2,4,6-Tribromophenol	10.727	330	10236	9.49	ng	0.00
45) 2-Fluorobiphenyl	9.263	172	58414	8.01	ng	0.00
79) Terphenyl-d14	13.015	244	48164	7.40	ng	0.00
Target Compounds						Qvalue
71) Phenanthrene	11.457	178	74083	8.63	ng	95
72) Anthracene	11.504	178	19360m	2.23	ng	
75) Fluoranthene	12.645	202	110255	12.41	ng	97
78) Pyrene	12.874	202	95302	10.89	ng	97
81) Benzo(a)anthracene	14.062	228	40320	5.65	ng	96
83) Chrysene	14.098	228	35880	5.23	ng	95
87) Indeno(1,2,3-cd)pyrene	17.074	276	15653	2.87	ng	# 83
88) Benzo(b)fluoranthene	15.127	252	35685m	6.54	ng	
89) Benzo(k)fluoranthene	15.156	252	13389m	2.69	ng	
90) Benzo(a)pyrene	15.504	252	25946	5.50	ng	98
92) Benzo(g,h,i)perylene	17.521	276	13805	3.00	ng	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051921\
Data File : BF124000.D
Acq On : 19 May 2021 20:37
Operator : JU/CG
Sample : M2438-01 5X
Misc :
ALS Vial : 18 Sample Multiplier: 1


Instrument :
BNA_F
ClientSampleId :
PL-02-051821

Manual Integrations
APPROVED

mohammad
5/20/2021 11:35:14 AM


Quant Time: May 20 02:27:08 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 14 19:05:57 2021
Response via : Initial Calibration

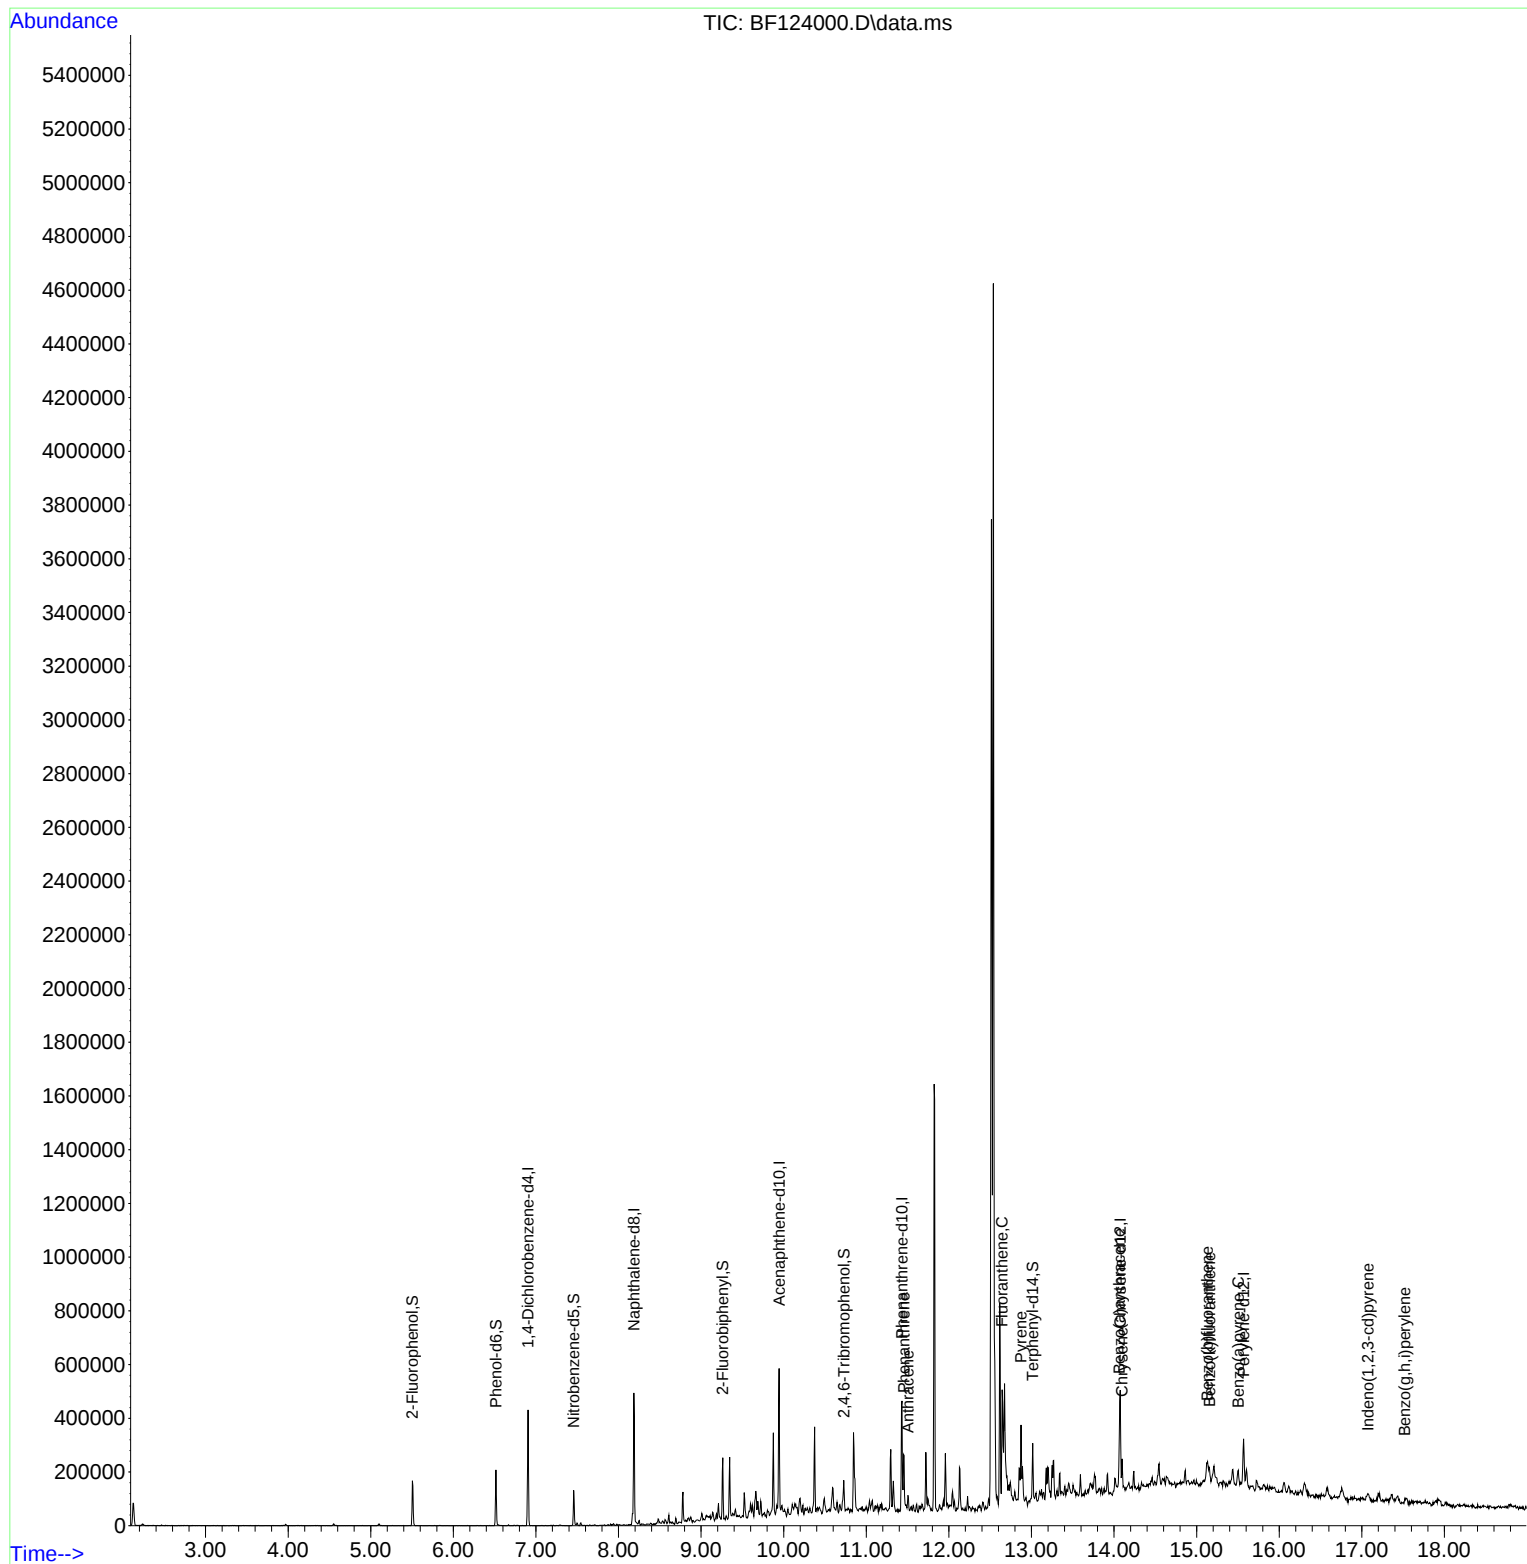



#1
1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.904 min Scan# 819
Delta R.T. 0.000 min
Lab File: BF124000.D
Acq: 19 May 2021 20:37




Instrument :
BNA_F
ClientSampled :
PL-02-051821




Tgt Ion:152 Resp: 45407
Ion Ratio Lower Upper
152 100
150 156.9 127.0 190.6
115 66.5 54.3 81.5

Manual Integrations
APPROVED



mohammad
5/20/2021 11:35:14 AM

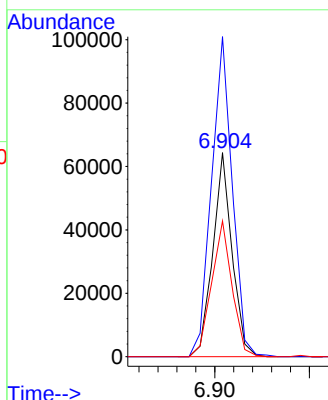


#5
2-Fluorophenol
Concen: 11.06 ng
RT: 5.504 min Scan# 581
Delta R.T. -0.006 min
Lab File: BF124000.D
Acq: 19 May 2021 20:37



Tgt Ion:112 Resp: 35759
Ion Ratio Lower Upper
112 100
64 78.8 61.4 92.0
63 45.8 33.0 49.4

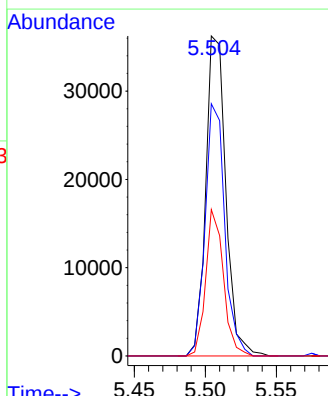

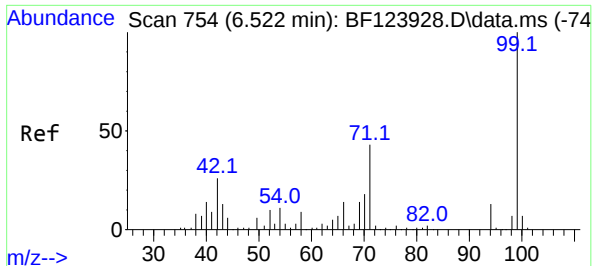





#7
Phenol-d6
Concen: 10.72 ng
RT: 6.516 min Scan# 753
Delta R.T. -0.006 min
Lab File: BF124000.D
Acq: 19 May 2021 20:37

Tgt Ion:	99	Resp:	44957
Ion	Ratio	Lower	Upper
99	100		
42	27.2	19.8	29.8
71	41.4	31.1	46.7

Instrument :
BNA_F
ClientSampleId :
PL-02-051821




Manual Integrations
APPROVED


mohammad
5/20/2021 11:35:14 AM

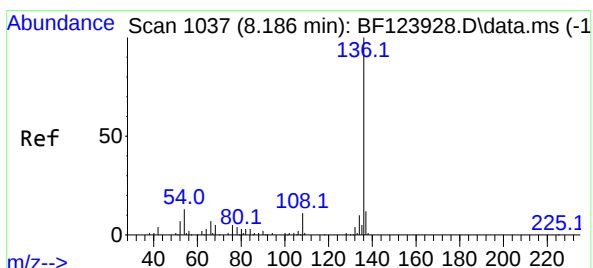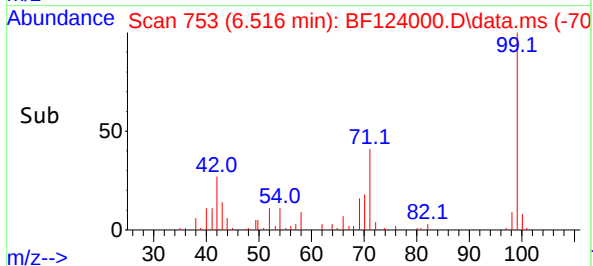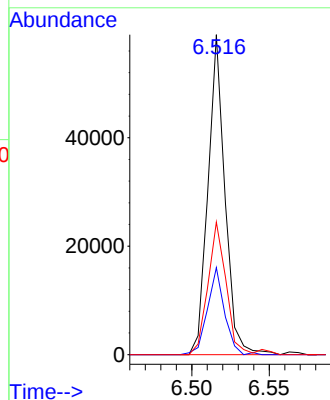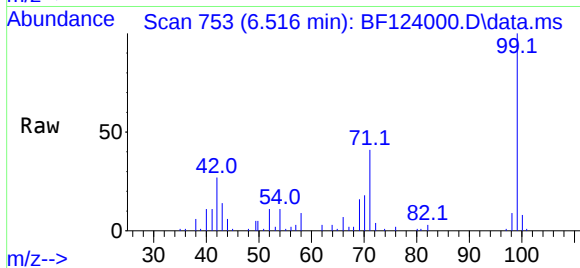


#21
Naphthalene-d8
Concen: 20.00 ng
RT: 8.186 min Scan# 1037
Delta R.T. 0.000 min
Lab File: BF124000.D
Acq: 19 May 2021 20:37

Tgt Ion:	136	Resp:	175657
Ion	Ratio	Lower	Upper
136	100		
137	11.0	8.7	13.1
54	15.3	9.8	14.6#
68	6.7	4.1	6.1#

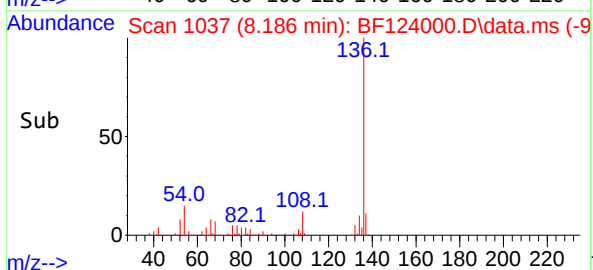
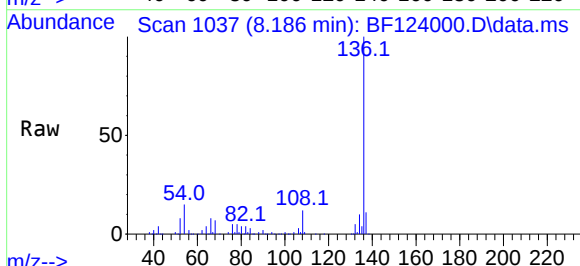
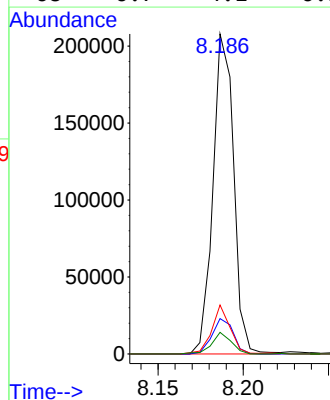


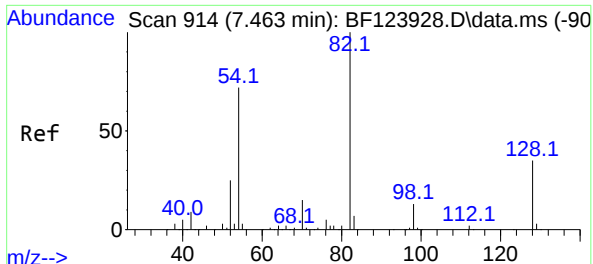


#23
Nitrobenzene-d5
Concen: 8.09 ng
RT: 7.457 min Scan# 913
Delta R.T. -0.006 min
Lab File: BF124000.D
Acq: 19 May 2021 20:37

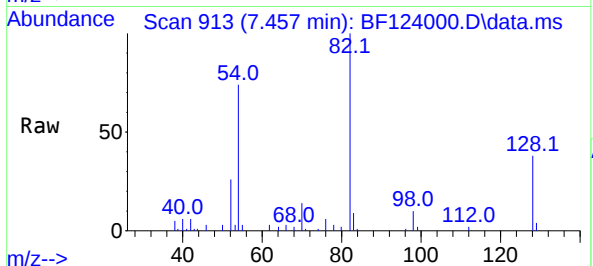



Tgt Ion: 82 Resp: 32998
Ion Ratio Lower Upper
82 100
128 38.0 29.4 44.2
54 73.8 54.1 81.1

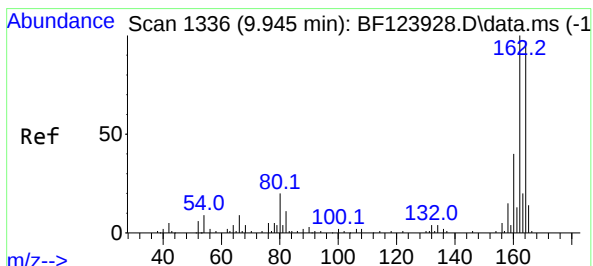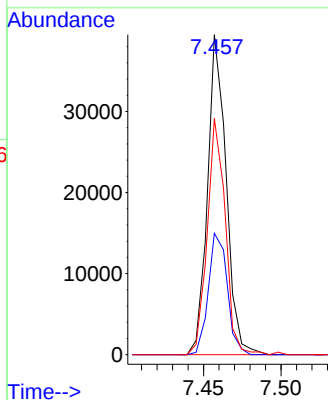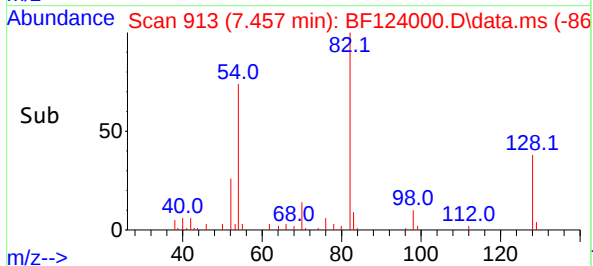

#39
Acenaphthene-d10
Concen: 20.00 ng
RT: 9.945 min Scan# 1336
Delta R.T. 0.000 min
Lab File: BF124000.D
Acq: 19 May 2021 20:37

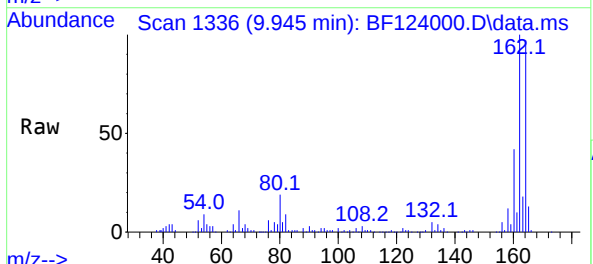


Tgt Ion: 164 Resp: 89782
Ion Ratio Lower Upper
164 100
162 103.0 80.7 121.1
160 43.7 37.3 55.9

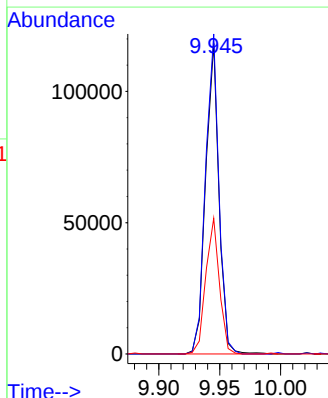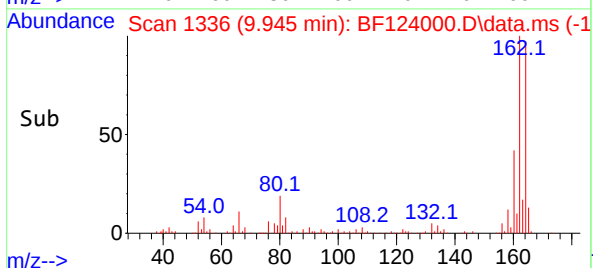


Instrument :
BNA_F
ClientSampleId :
PL-02-051821

Manual Integrations
APPROVED




mohammad
5/20/2021 11:35:14 AM

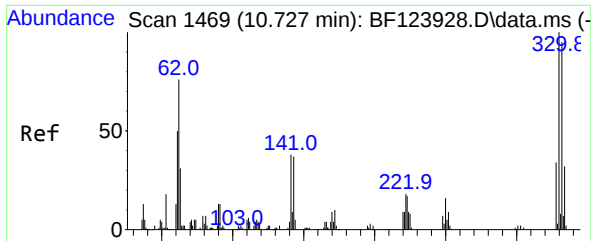


#42
2,4,6-Tribromophenol
Concen: 9.49 ng
RT: 10.727 min Scan# 1469
Delta R.T. -0.000 min
Lab File: BF124000.D
Acq: 19 May 2021 20:37

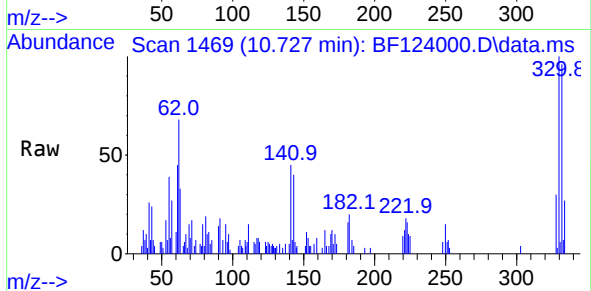



Tgt Ion: 330 Resp: 10236
Ion Ratio Lower Upper
330 100
332 84.4 77.1 115.7
141 53.0 27.9 41.9#

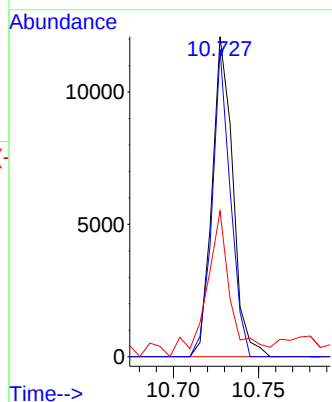

#45
2-Fluorobiphenyl
Concen: 8.01 ng
RT: 9.263 min Scan# 1220
Delta R.T. -0.000 min
Lab File: BF124000.D
Acq: 19 May 2021 20:37

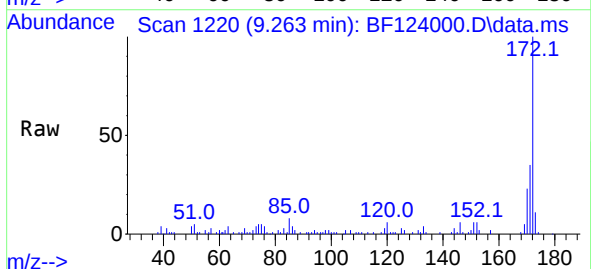


Tgt Ion: 172 Resp: 58414
Ion Ratio Lower Upper
172 100
171 35.4 28.1 42.1
170 23.1 19.2 28.8

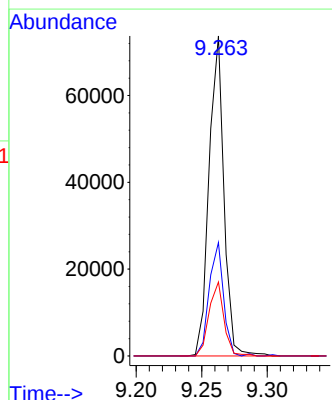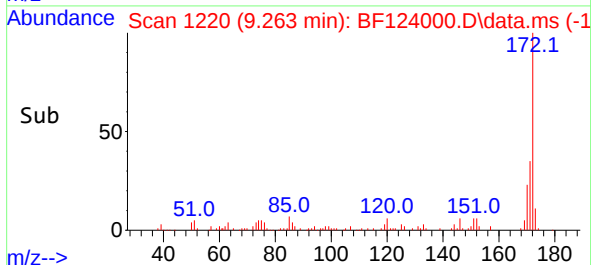

Instrument :
BNA_F
ClientSampled :
PL-02-051821


Manual Integrations
APPROVED

mohammad
5/20/2021 11:35:14 AM



#64
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.433 min Scan# 1589
Delta R.T. 0.006 min
Lab File: BF124000.D
Acq: 19 May 2021 20:37




Instrument :
BNA_F
ClientSampleId :
PL-02-051821




Tgt Ion:188 Resp: 135431
Ion Ratio Lower Upper
188 100
94 7.8 6.9 10.3
80 9.0 8.2 12.2

Manual Integrations
APPROVED



mohammad
5/20/2021 11:35:14 AM

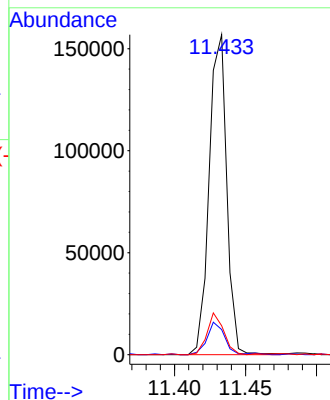


#71
Phenanthrene
Concen: 8.63 ng
RT: 11.457 min Scan# 1593
Delta R.T. 0.006 min
Lab File: BF124000.D
Acq: 19 May 2021 20:37



Tgt Ion:178 Resp: 74083
Ion Ratio Lower Upper
178 100
176 17.2 15.6 23.4
179 13.7 12.5 18.7

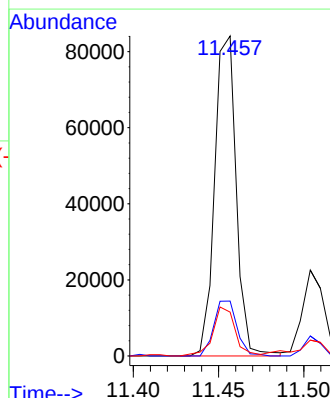







#72
 Anthracene
 Concen: 2.23 ng m
 RT: 11.504 min Scan# 1601
 Delta R.T. -0.000 min
 Lab File: BF124000.D
 Acq: 19 May 2021 20:37

Tgt Ion	Ratio	Lower	Upper
178	100		
176	23.3	15.4	23.0#
179	18.4	12.6	18.8

Instrument :
 BNA_F
 ClientSampled :
 PL-02-051821




Manual Integrations
 APPROVED


mohammad
 5/20/2021 11:35:14 AM

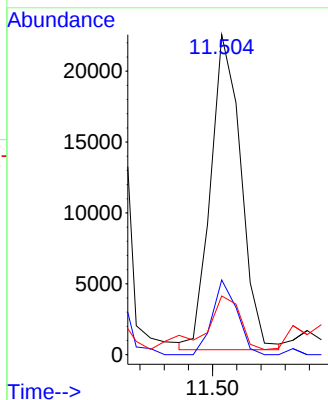


#75
 Fluoranthene
 Concen: 12.41 ng
 RT: 12.645 min Scan# 1795
 Delta R.T. 0.006 min
 Lab File: BF124000.D
 Acq: 19 May 2021 20:37

Tgt Ion	Ratio	Lower	Upper
202	100		
101	12.8	0.0	30.9
203	18.1	0.0	37.5

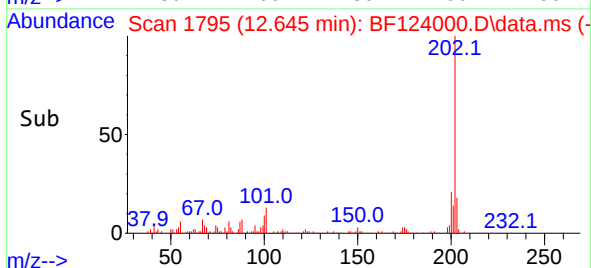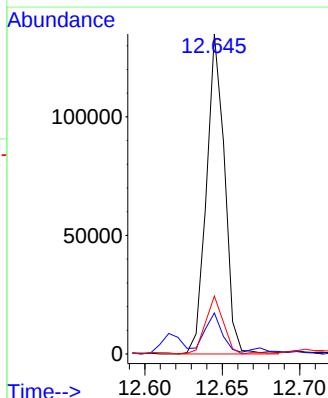



#76
Chrysene-d12
Concen: 20.00 ng
RT: 14.074 min Scan# 2038
Delta R.T. 0.006 min
Lab File: BF124000.D
Acq: 19 May 2021 20:37



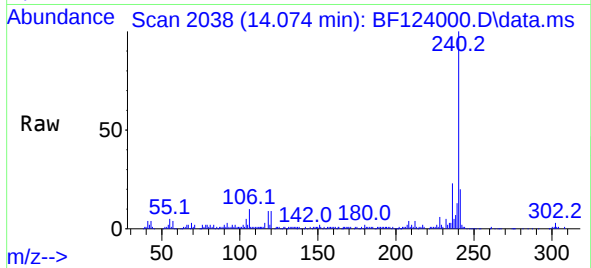


Tgt Ion:240 Resp: 98593
Ion Ratio Lower Upper
240 100
120 9.1 7.2 10.8
236 23.1 19.0 28.4


Instrument :
BNA_F
ClientSampleId :
PL-02-051821

Manual Integrations
APPROVED



mohammad
5/20/2021 11:35:14 AM

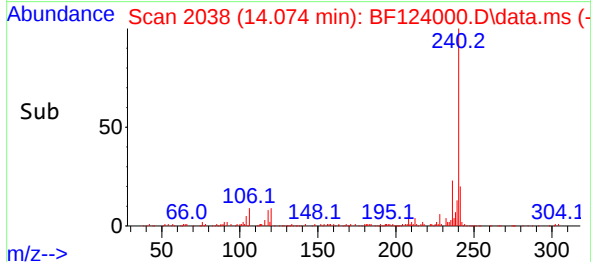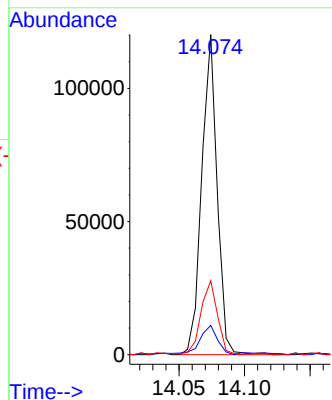


#78
Pyrene
Concen: 10.89 ng
RT: 12.874 min Scan# 1834
Delta R.T. 0.006 min
Lab File: BF124000.D
Acq: 19 May 2021 20:37



Tgt Ion:202 Resp: 95302
Ion Ratio Lower Upper
202 100
200 21.4 16.1 24.1
203 17.1 14.8 22.2

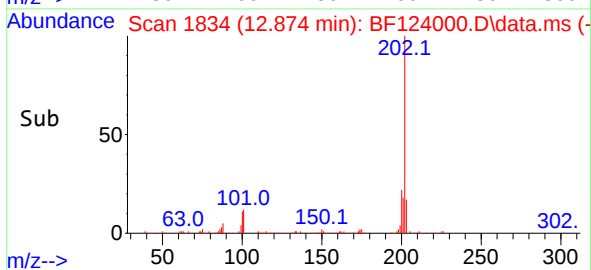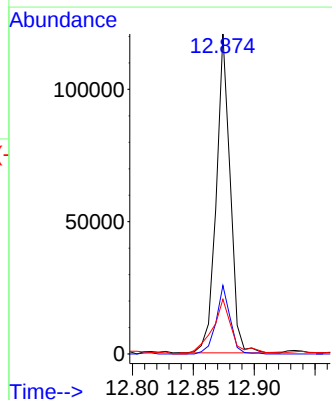







#79
Terphenyl-d14
Concen: 7.40 ng
RT: 13.015 min Scan# 1858
Delta R.T. -0.000 min
Lab File: BF124000.D
Acq: 19 May 2021 20:37

Tgt Ion:244 Resp: 48164
Ion Ratio Lower Upper
244 100
212 8.9 5.7 8.5#
122 10.4 9.7 14.5

Instrument :
BNA_F
ClientSampleId :
PL-02-051821




Manual Integrations
APPROVED


mohammad
5/20/2021 11:35:14 AM

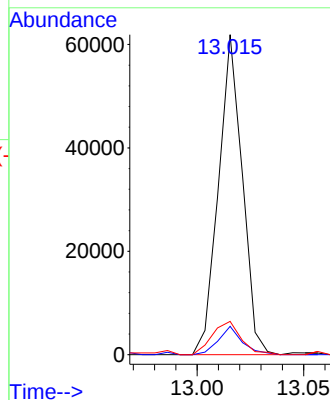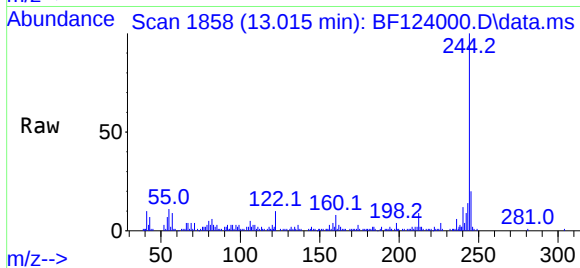


#81
Benzo(a)anthracene
Concen: 5.65 ng
RT: 14.062 min Scan# 2036
Delta R.T. 0.006 min
Lab File: BF124000.D
Acq: 19 May 2021 20:37

Tgt Ion:228 Resp: 40320
Ion Ratio Lower Upper
228 100
226 30.0 22.4 33.6
229 22.0 16.0 24.0

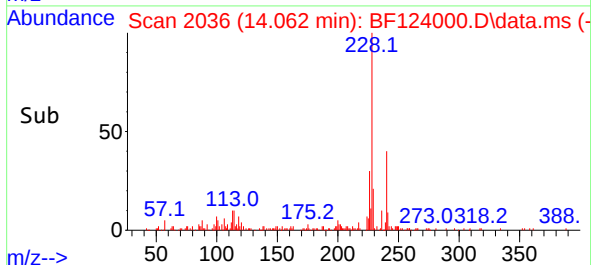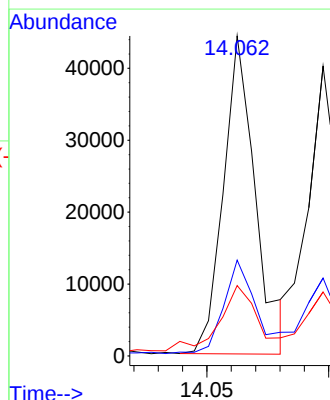
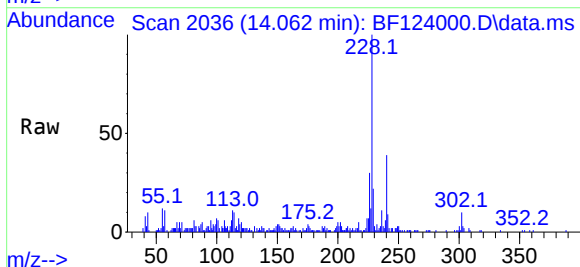




#83
Chrysene
Concen: 5.23 ng
RT: 14.098 min Scan# 2042
Delta R.T. -0.000 min
Lab File: BF124000.D
Acq: 19 May 2021 20:37

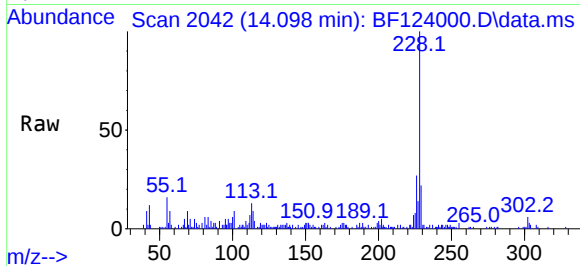


Tgt Ion:228 Resp: 35880
Ion Ratio Lower Upper
228 100
226 26.9 24.3 36.5
229 22.1 16.2 24.2

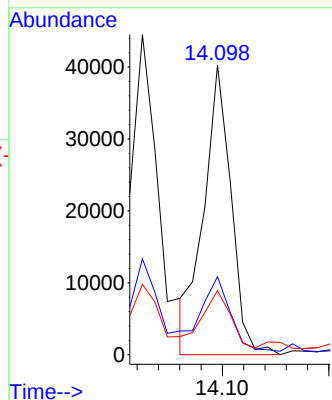


Instrument :
BNA_F
ClientSampleId :
PL-02-051821

Manual Integrations
APPROVED



mohammad
5/20/2021 11:35:14 AM




#86
Perylene-d12
Concen: 20.00 ng
RT: 15.568 min Scan# 2292
Delta R.T. 0.018 min
Lab File: BF124000.D
Acq: 19 May 2021 20:37

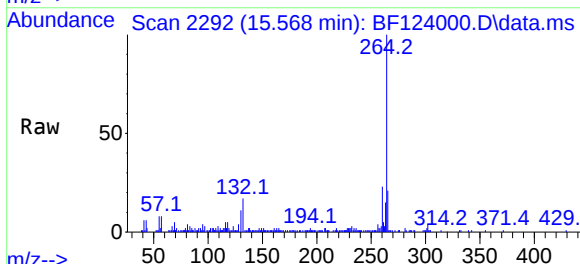

Tgt Ion:264 Resp: 70554
Ion Ratio Lower Upper
264 100
260 22.9 18.7 28.1
265 20.6 17.8 26.8

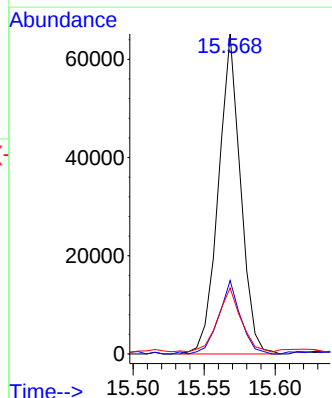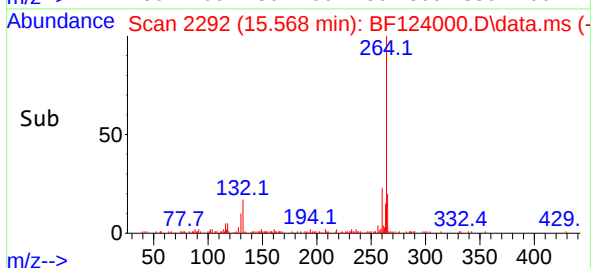







#87
Indeno(1,2,3-cd)pyrene
Concen: 2.87 ng
RT: 17.074 min Scan# 2548
Delta R.T. 0.018 min
Lab File: BF124000.D
Acq: 19 May 2021 20:37

Tgt Ion: 276 Resp: 15653
Ion Ratio Lower Upper
276 100
138 30.0 16.2 24.2#
277 32.2 20.1 30.1#

Instrument :
BNA_F
ClientSampled :
PL-02-051821




Manual Integrations
APPROVED


mohammad
5/20/2021 11:35:14 AM

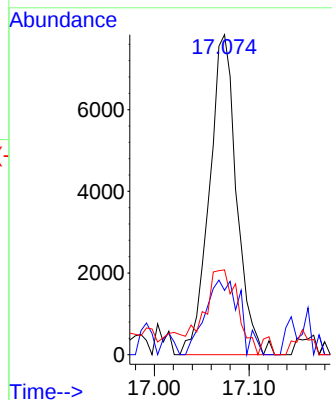

#88
Benzo(b)fluoranthene
Concen: 6.54 ng m
RT: 15.127 min Scan# 2217
Delta R.T. 0.012 min
Lab File: BF124000.D
Acq: 19 May 2021 20:37

Tgt Ion: 252 Resp: 35685
Ion Ratio Lower Upper
252 100
253 21.7 18.1 27.1
125 13.8 6.2 9.4#

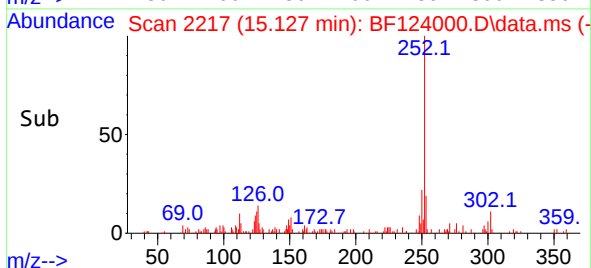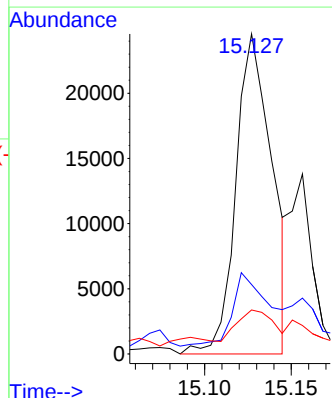



#89

Benzo(k)fluoranthene

Concen: 2.69 ng m

RT: 15.156 min Scan# 2222

Delta R.T. 0.006 min

Lab File: BF124000.D

Acq: 19 May 2021 20:37

Tgt Ion:	252	Resp:	13389
Ion Ratio	Lower	Upper	
252	100		
253	31.0	17.9	26.9#
125	15.8	7.0	10.6#

Instrument :





BNA_F

ClientSampled :

PL-02-051821

Manual Integrations
APPROVED

mohammad
5/20/2021 11:35:14 AM

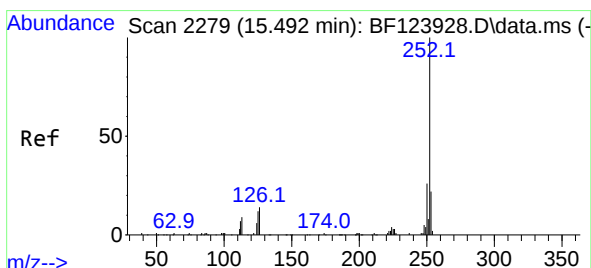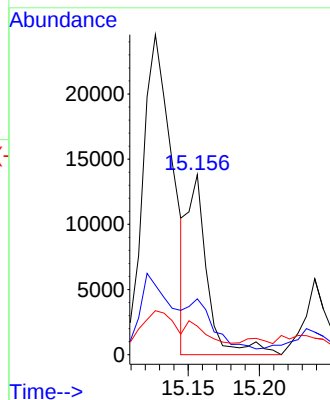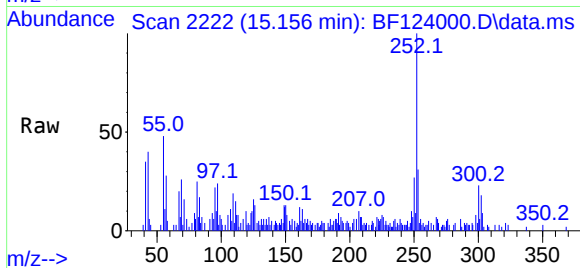

#90

Benzo(a)pyrene

Concen: 5.50 ng




RT: 15.504 min Scan# 2281


Delta R.T. 0.012 min

Lab File: BF124000.D

Acq: 19 May 2021 20:37


Tgt Ion:	252	Resp:	25946
Ion Ratio	Lower	Upper	
252	100		
253	23.6	18.4	27.6
125	10.9	8.0	12.0

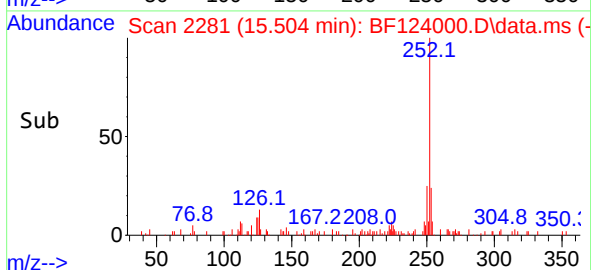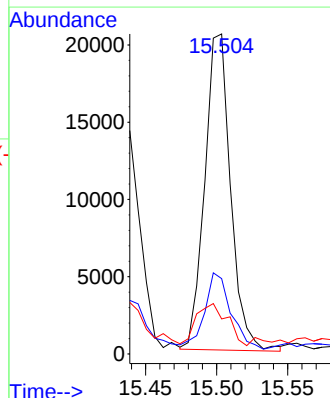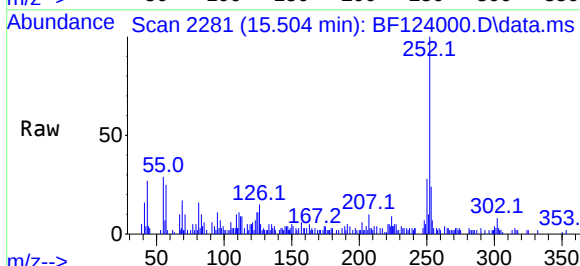



#92
Benzo(g,h,i)perylene
Concen: 3.00 ng
RT: 17.521 min Scan# 2624
Delta R.T. 0.012 min
Lab File: BF124000.D
Acq: 19 May 2021 20:37

Instrument :
BNA_F
ClientSampleId :
PL-02-051821

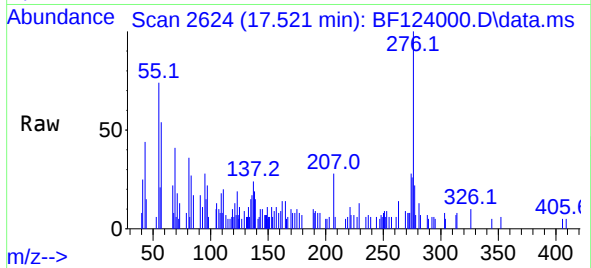

Tgt Ion:	276	Resp:	13805
Ion	Ratio	Lower	Upper
276	100		
277	22.1	18.2	27.2
138	19.2	13.8	20.6

Manual Integrations
APPROVED

mohammad
5/20/2021 11:35:14 AM

