
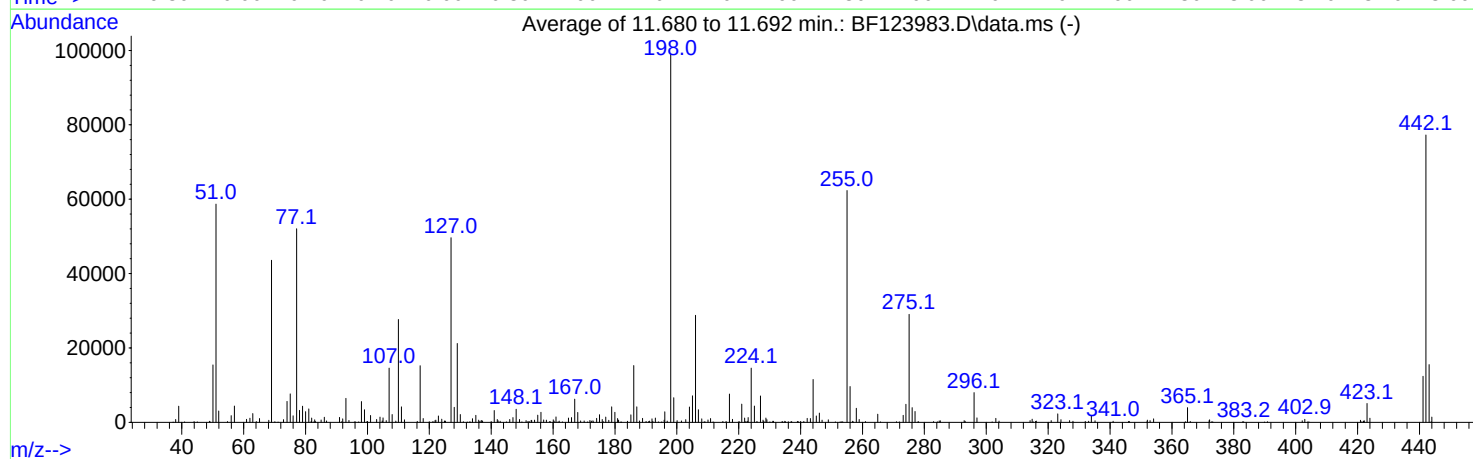


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051921\
 Data File : BF123983.D
 Acq On : 19 May 2021 10:48
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 14 19:05:57 2021

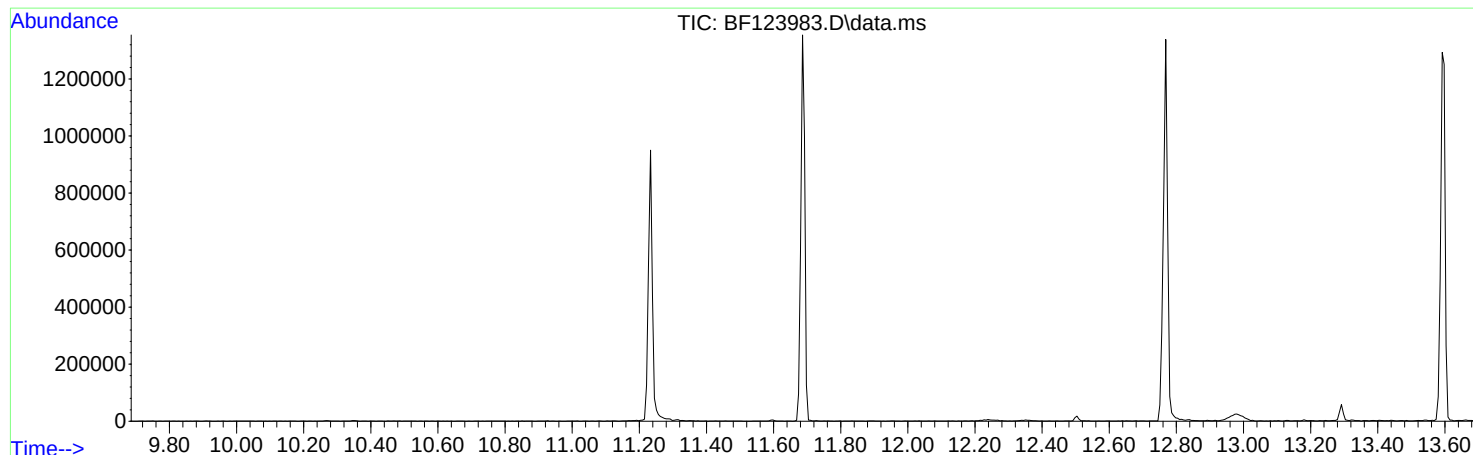




AutoFind: Scans 1631, 1632, 1633; Background Corrected with Scan 1626

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	59.3	58693	PASS
68	69	0.00	2	1.3	583	PASS
69	198	0.00	100	44.1	43579	PASS
70	69	0.00	2	0.4	165	PASS
127	198	10	80	50.2	49664	PASS
197	198	0.00	2	0.4	354	PASS
198	198	100	100	100.0	98909	PASS
199	198	5	9	6.7	6622	PASS
275	198	10	60	29.4	29051	PASS
365	198	1	100	4.0	3970	PASS
441	198	0.01	100	12.5	12374	PASS
442	442	50	100	100.0	77269	PASS
443	442	15	24	20.1	15515	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051921\
Data File : BF123983.D
Acq On : 19 May 2021 10:48
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 19 12:49:55 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 14 19:05:57 2021
Response via : Initial Calibration

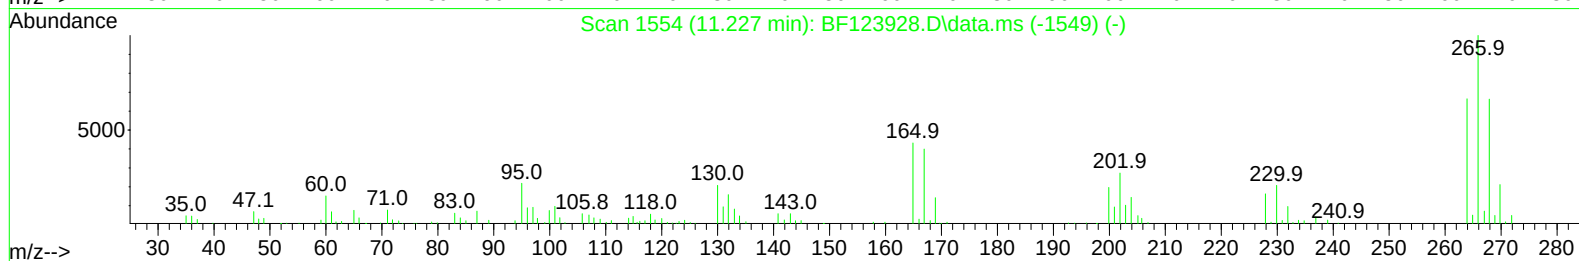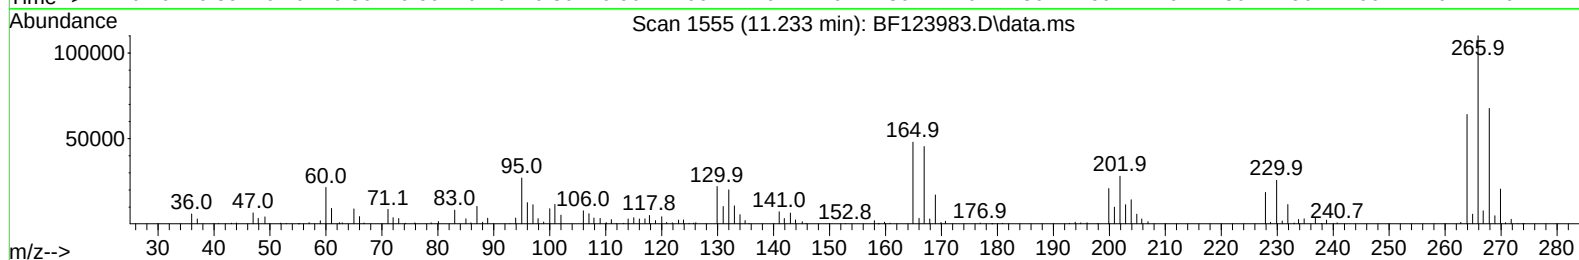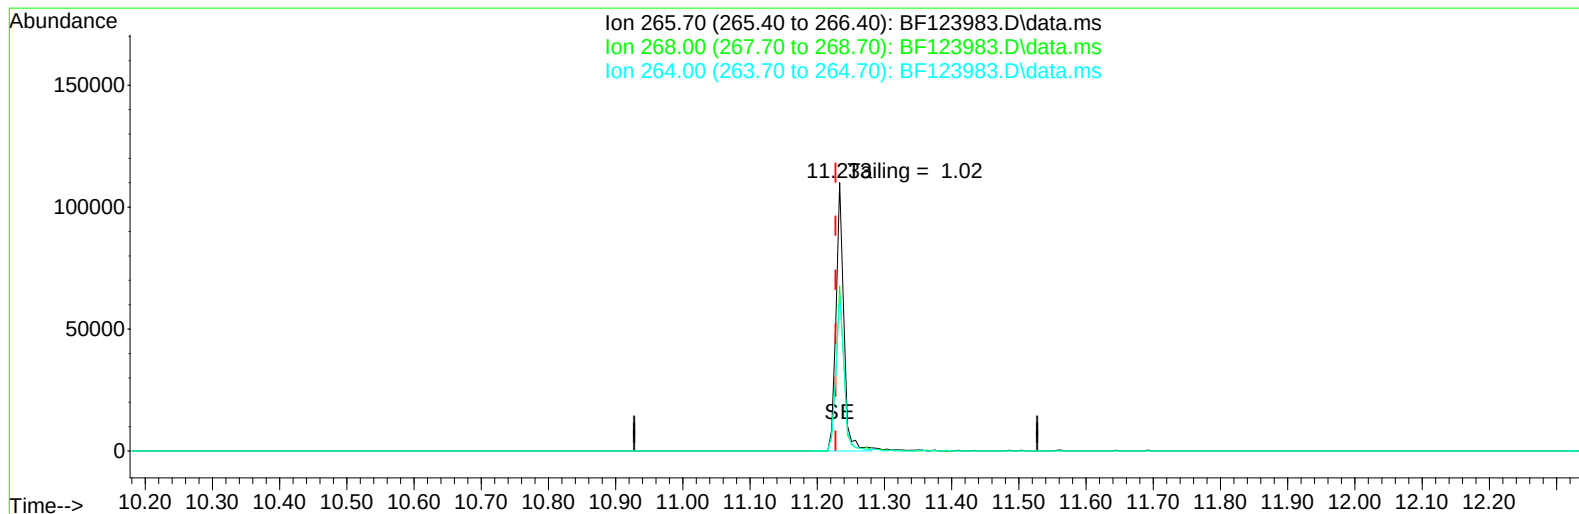

TIC: BF123983.D\data.ms

(70) Pentachlorophenol (C)

11.233min (+ 0.006) 25558.29 ng




response 91145

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	61.49
264.00	65.70	58.25
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051921\
 Data File : BF123983.D
 Acq On : 19 May 2021 10:48
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: May 19 12:49:55 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 14 19:05:57 2021
 Response via : Initial Calibration

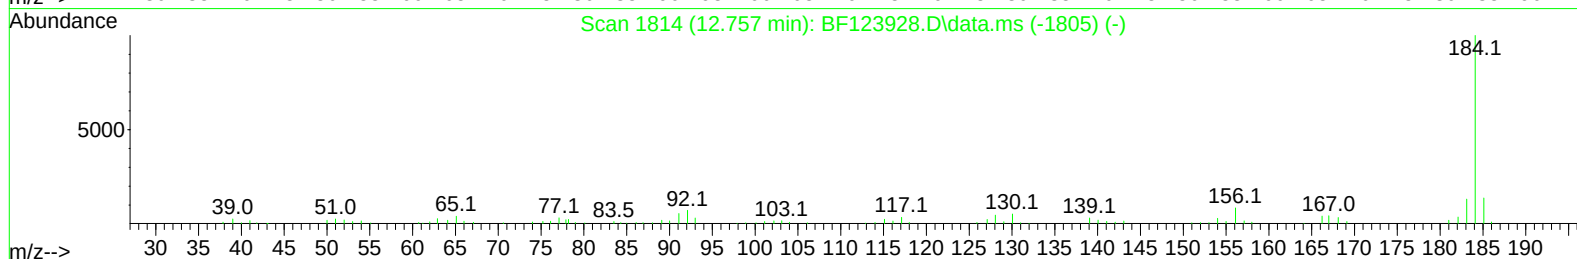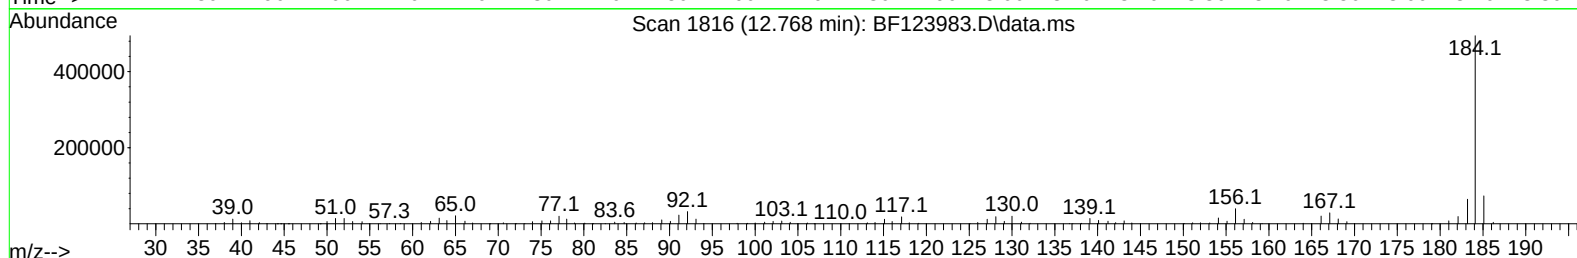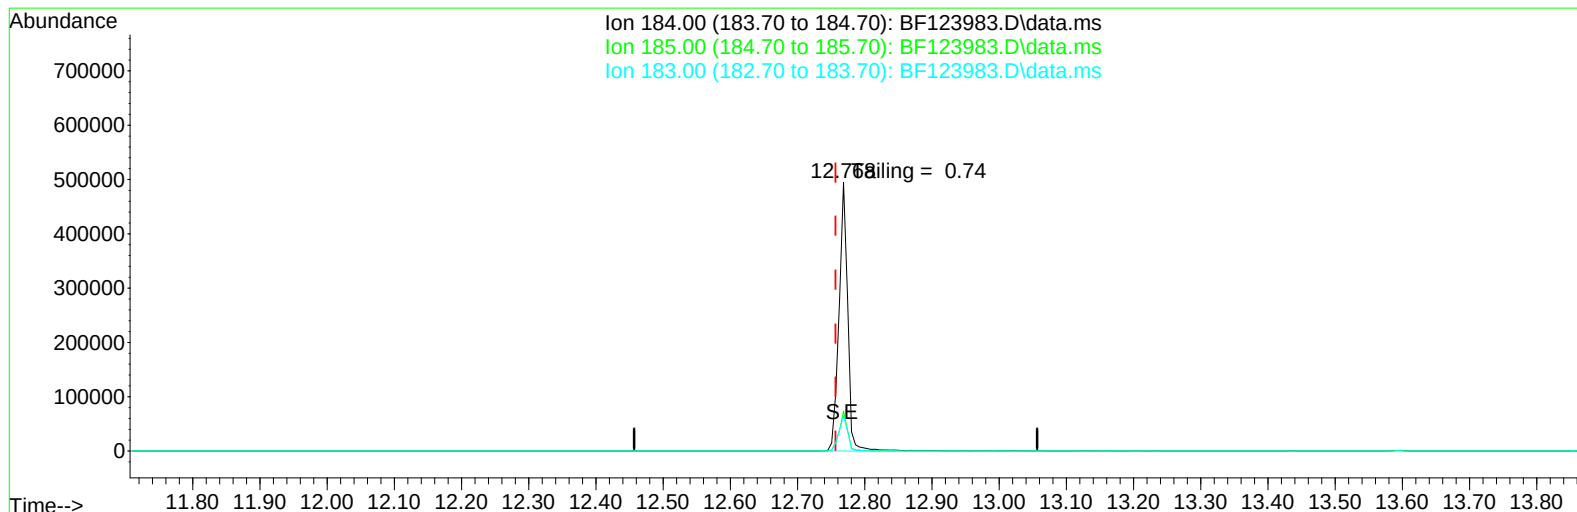

TIC: BF123983.D\data.ms

(77) Benzidine

12.768min (+ 0.012) 0.00 ng

response 446390

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.89
183.00	9.80	13.08#
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/19/2021	BNA_F	<u>BF123983.D</u>
Compound Name	Response	Retention Time
DDT	219755	13.59
DDD	9001	13.29
DDE	438	12.96
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9439	229194	4.12