
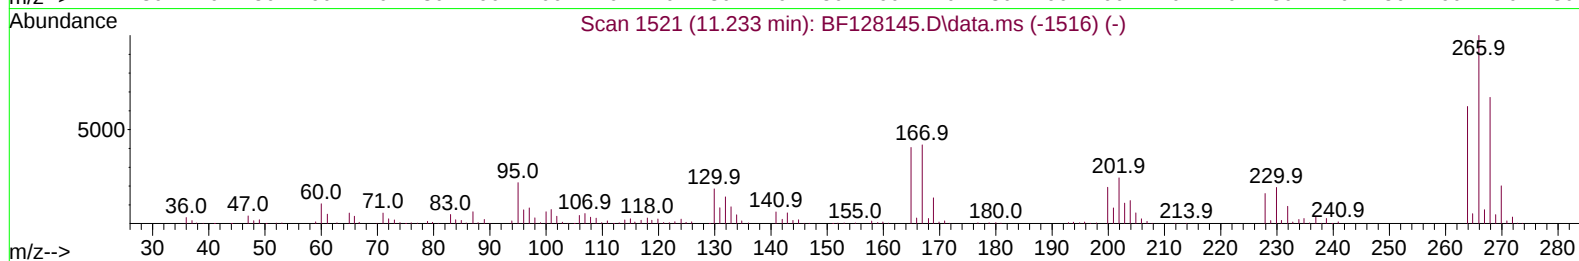
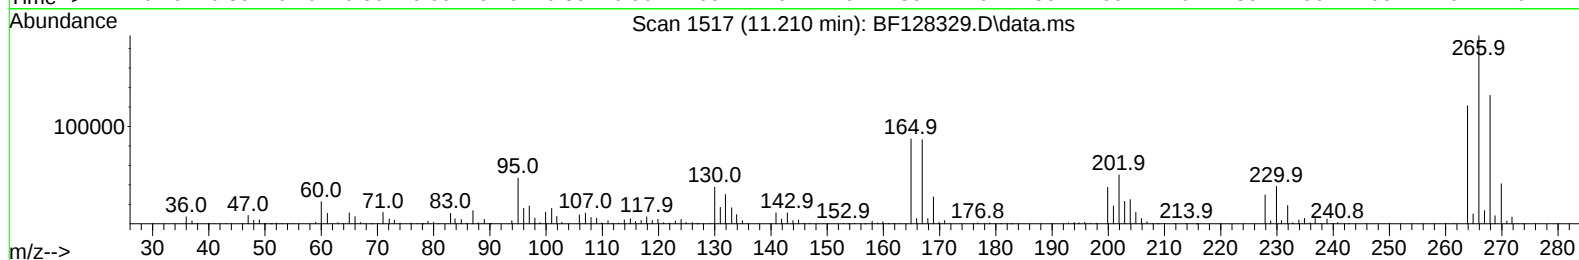


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF051922\  
 Data File : BF128329.D  
 Acq On : 19 May 2022 11:35  
 Operator : CG\JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 19 17:10:33 2022  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF050922.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu May 19 06:47:51 2022  
 Response via : Initial Calibration

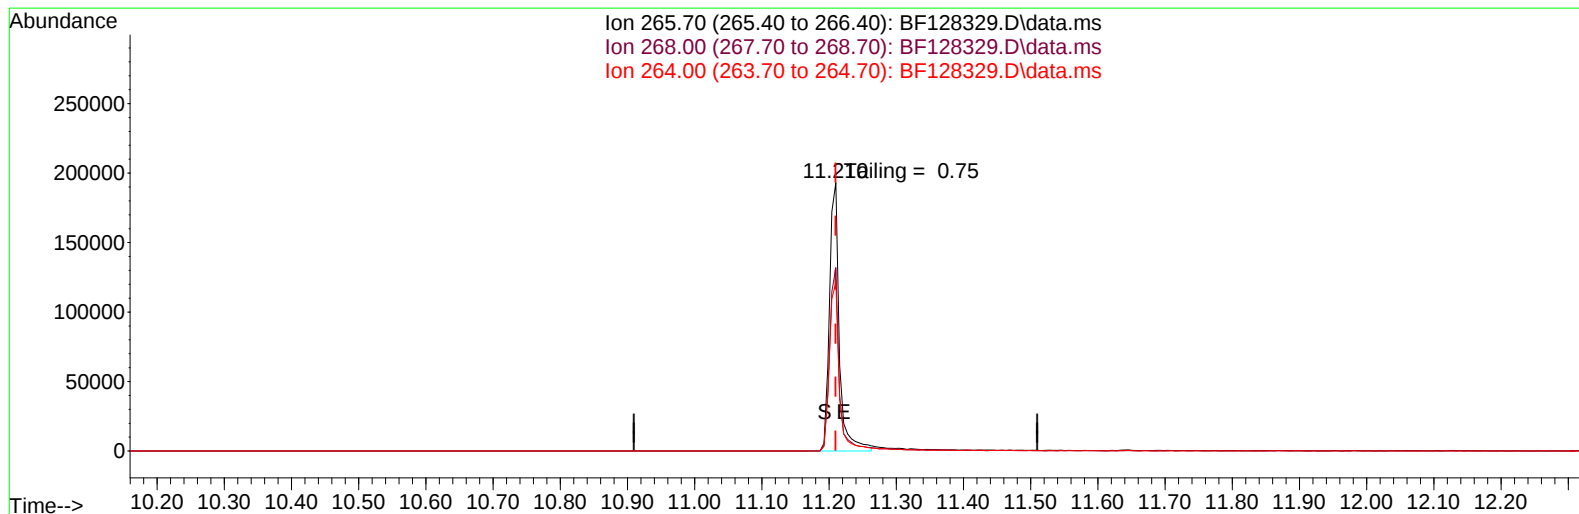

TIC: BF128329.D\data.ms

**(70) Pentachlorophenol (C)**




11.210min (+ 0.000) 279486.14 ng

response 204330

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 66.30  | 68.32  |
| 264.00 | 66.40  | 62.79  |
| 0.00   | 0.00   | 0.00   |

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051922\  
Data File : BF128329.D  
Acq On    : 19 May 2022  11:35  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: May 19 17:10:33 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF050922.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu May 19 06:47:51 2022  
Response via : Initial Calibration

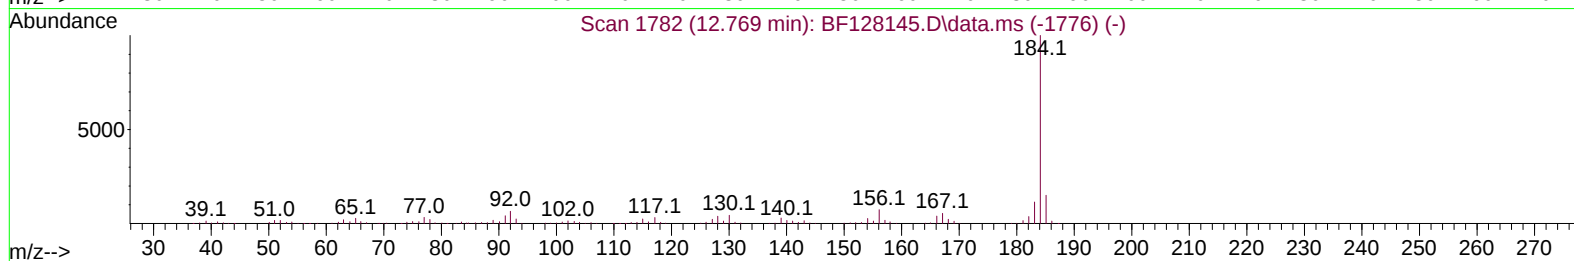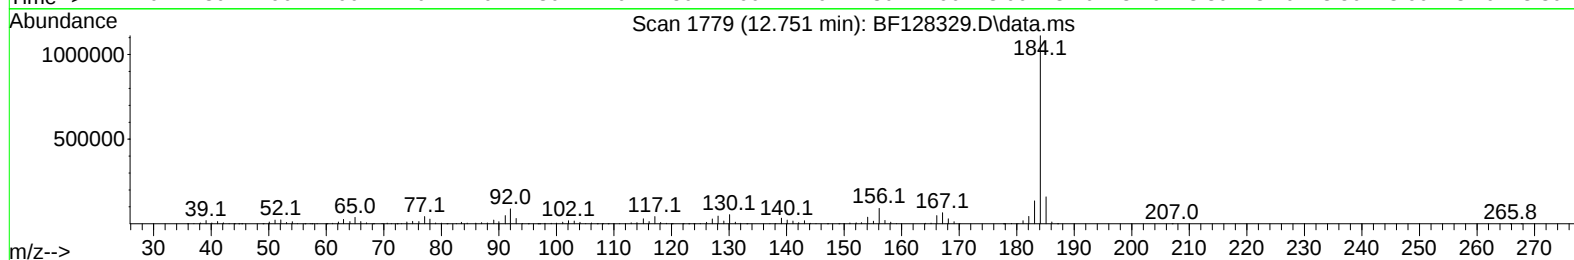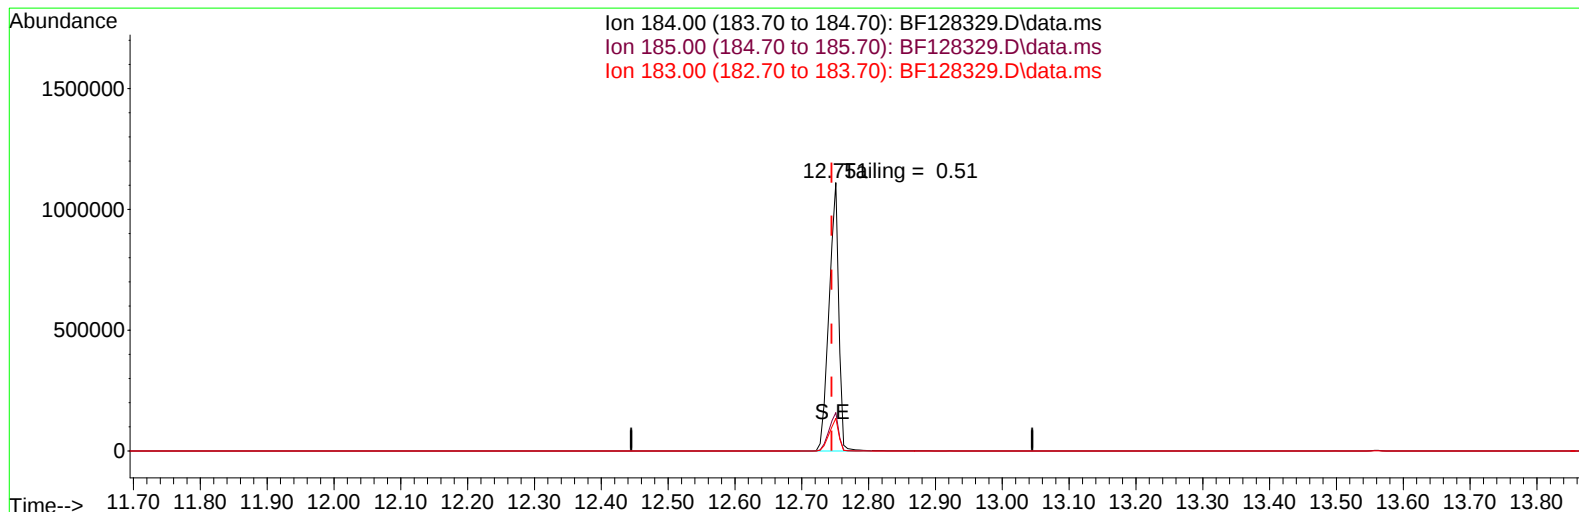

TIC: BF128329.D\data.ms

(77) Benzidine

**12.751min (+ 0.006) 51730.25 ng**

response 1123751

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.10  | 14.33  |
| 183.00 | 11.20  | 12.16  |
| 0.00   | 0.00   | 0.00   |