

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051922\
 Data File : BF128336.D
 Acq On : 19 May 2022 14:58
 Operator : CG\JU
 Sample : PB144922TB
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB144922TB

Quant Time: May 19 16:52:13 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 19 06:47:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.863	152	90365	20.000	ng	0.00
21) Naphthalene-d8	8.145	136	353109	20.000	ng	-0.01
39) Acenaphthene-d10	9.904	164	197580	20.000	ng	-0.01
64) Phenanthrene-d10	11.398	188	371510	20.000	ng	0.00
76) Chrysene-d12	14.045	240	264828	20.000	ng	-0.01
86) Perylene-d12	15.533	264	196336	20.000	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.498	112	656807	115.868	ng	0.00
7) Phenol-d6	6.498	99	901619	120.254	ng	-0.01
23) Nitrobenzene-d5	7.428	82	661130	84.248	ng	-0.02
42) 2,4,6-Tribromophenol	10.698	330	252586	111.468	ng	-0.01
45) 2-Fluorobiphenyl	9.222	172	1067974	84.576	ng	-0.01
79) Terphenyl-d14	12.986	244	1229304	87.101	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051922\
Data File : BF128336.D
Acq On : 19 May 2022 14:58
Operator : CG\JU
Sample : PB144922TB
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB144922TB

Quant Time: May 19 16:52:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 19 06:47:51 2022
Response via : Initial Calibration




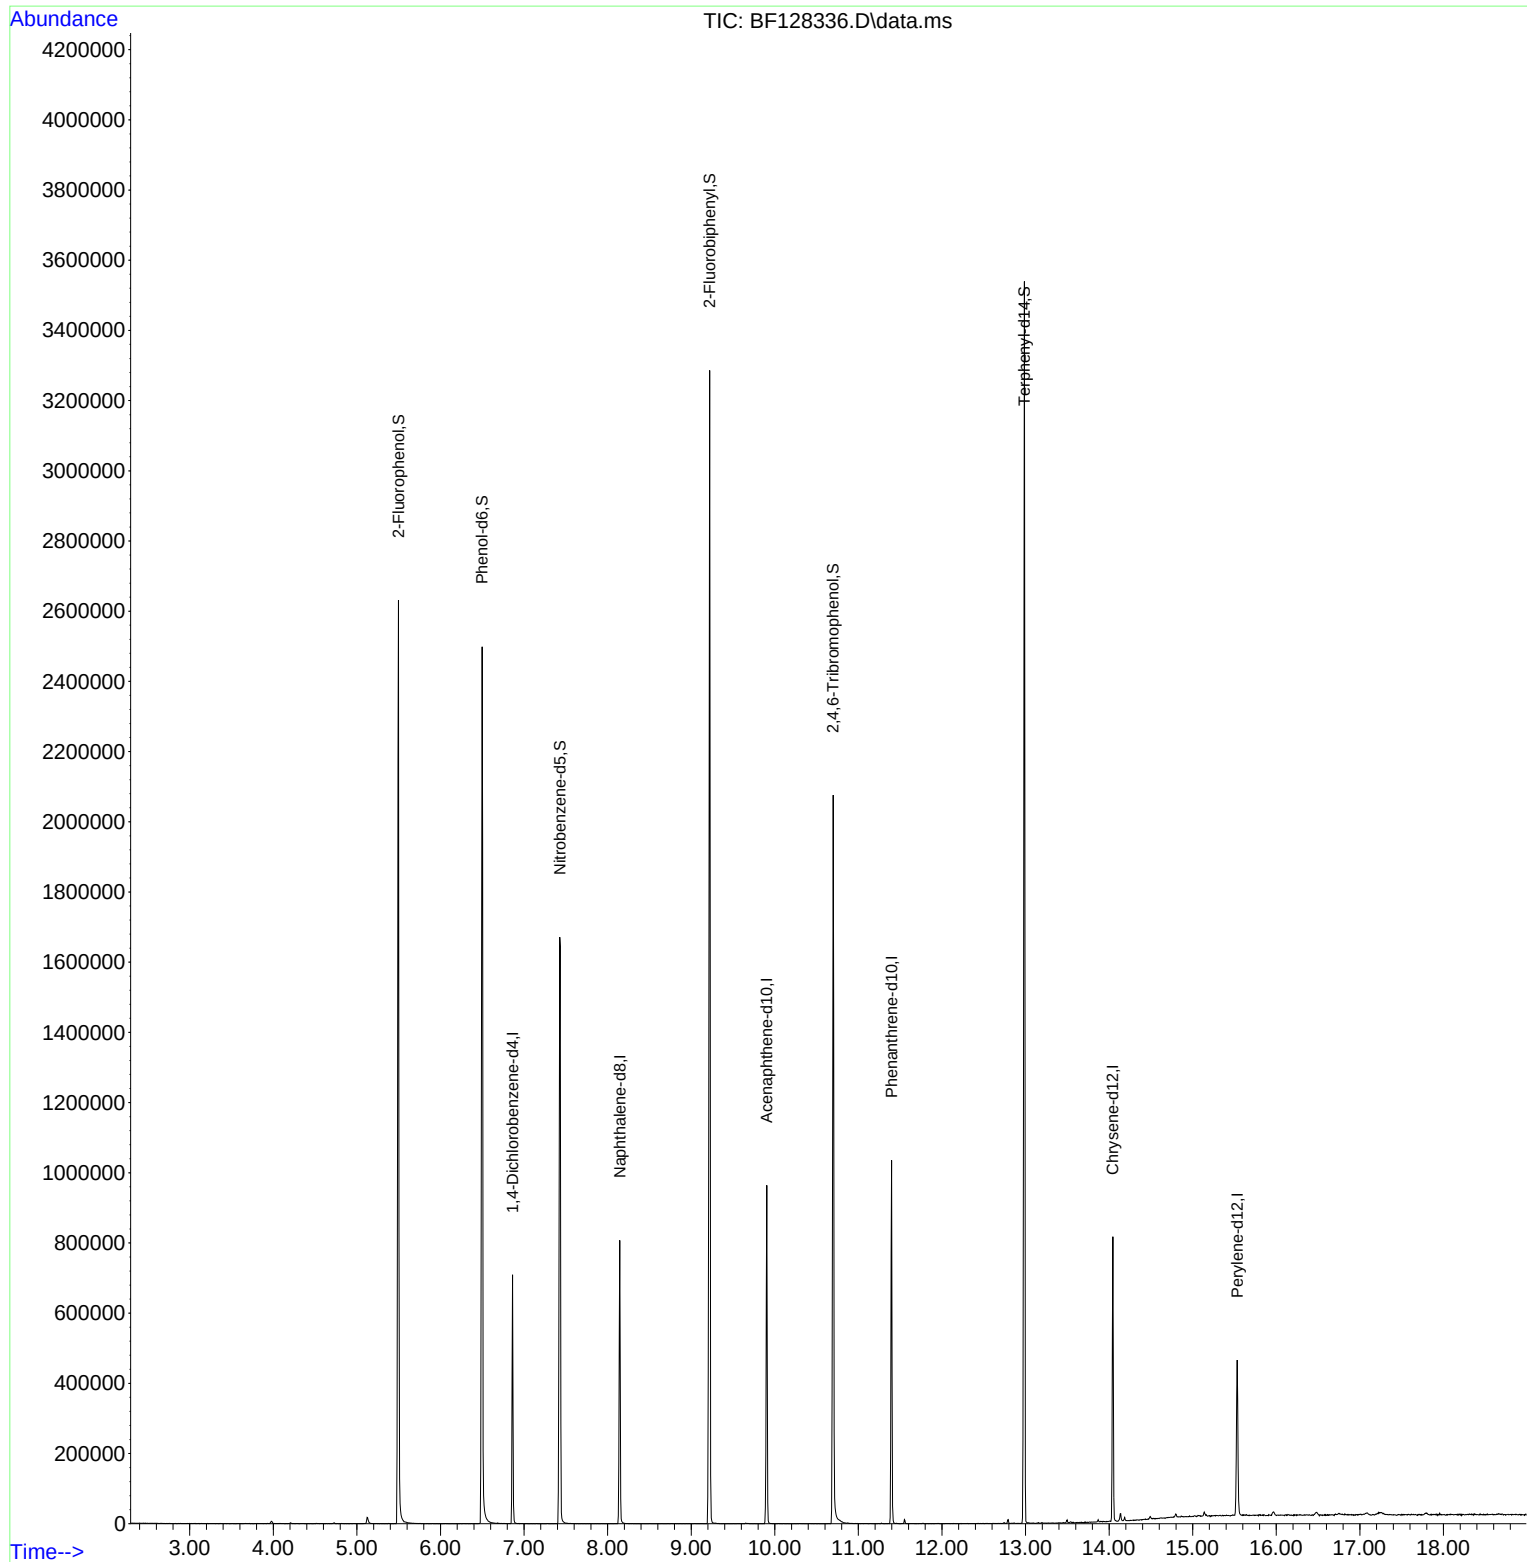




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.863 min Scan# 71
Delta R.T. -0.006 min
Lab File: BF128336.D
Acq: 19 May 2022 14:58




Instrument :
BNA_F
ClientSampleId :
PB144922TB


Tgt Ion:152 Resp: 90365
Ion Ratio Lower Upper
152 100
150 153.7 125.3 187.9
115 65.1 48.8 73.2

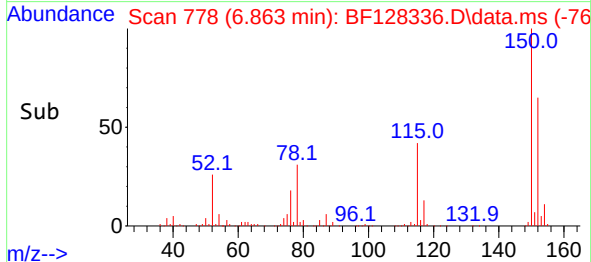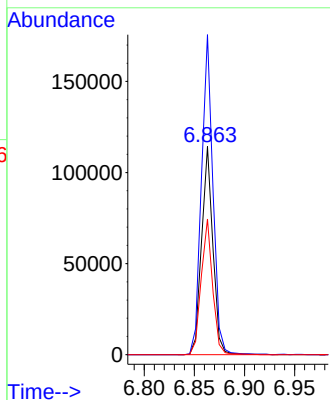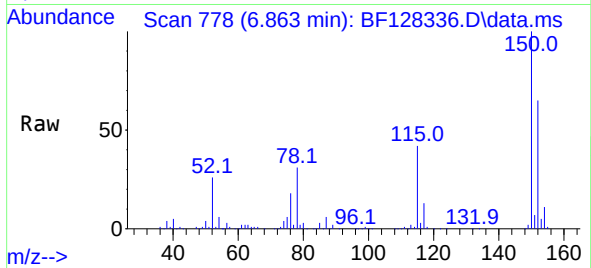

#5
2-Fluorophenol
Concen: 115.868 ng
RT: 5.498 min Scan# 546
Delta R.T. 0.006 min
Lab File: BF128336.D
Acq: 19 May 2022 14:58

Tgt Ion:112 Resp: 656807
Ion Ratio Lower Upper
112 100
64 67.3 49.5 74.3
63 37.6 26.3 39.5


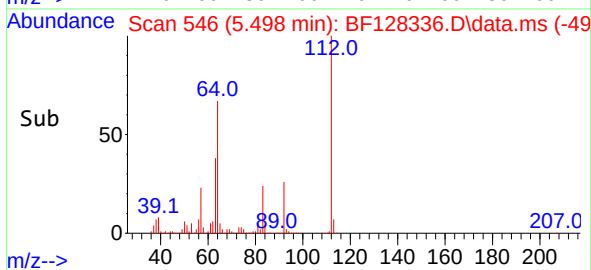
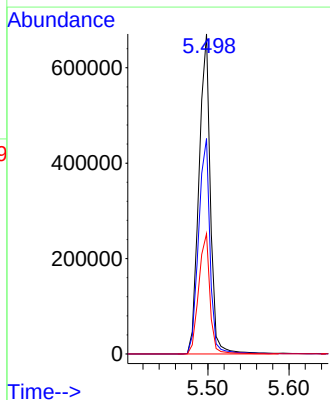





#7
Phenol-d6
Concen: 120.254 ng
RT: 6.498 min Scan# 71
Delta R.T. -0.012 min
Lab File: BF128336.D
Acq: 19 May 2022 14:58




Instrument :
BNA_F
ClientSampleId :
PB144922TB


Tgt Ion: 99 Resp: 901619
Ion Ratio Lower Upper
99 100
42 22.7 16.6 24.8
71 40.9 30.0 45.0

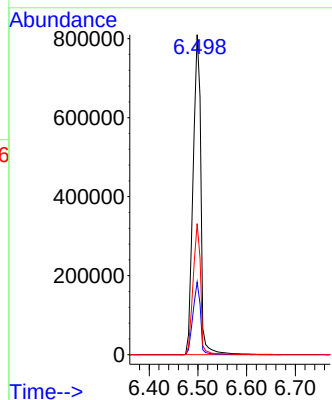

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.145 min Scan# 996
Delta R.T. -0.012 min
Lab File: BF128336.D
Acq: 19 May 2022 14:58

Tgt Ion: 136 Resp: 353109
Ion Ratio Lower Upper
136 100
137 10.9 8.6 13.0
54 8.6 6.8 10.2
68 6.4 5.1 7.7


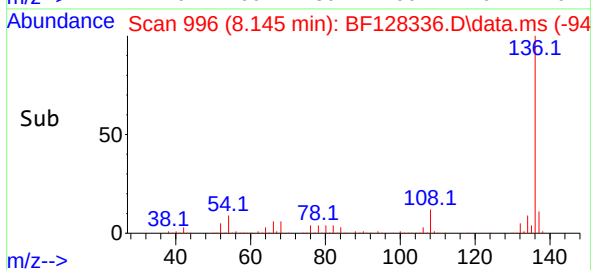
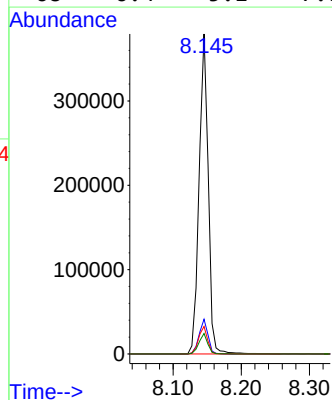





#23
Nitrobenzene-d5
Concen: 84.248 ng
RT: 7.428 min Scan# 81
Delta R.T. -0.018 min
Lab File: BF128336.D
Acq: 19 May 2022 14:58




Instrument :
BNA_F
ClientSampleId :
PB144922TB


Tgt Ion: 82 Resp: 661130
Ion Ratio Lower Upper
82 100
128 35.8 30.0 45.0
54 52.5 41.3 61.9

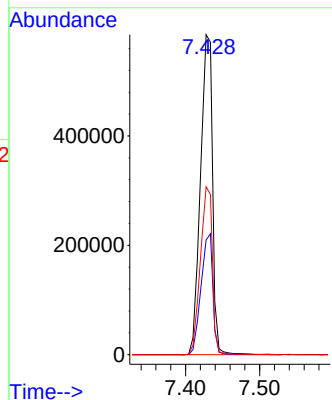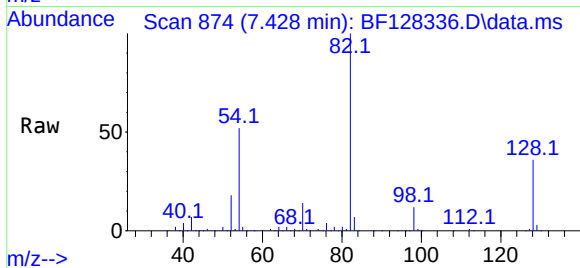

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.904 min Scan# 1295
Delta R.T. -0.012 min
Lab File: BF128336.D
Acq: 19 May 2022 14:58

Tgt Ion:164 Resp: 197580
Ion Ratio Lower Upper
164 100
162 96.6 76.0 114.0
160 45.2 34.8 52.2


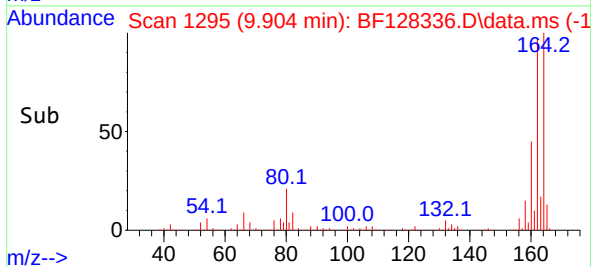
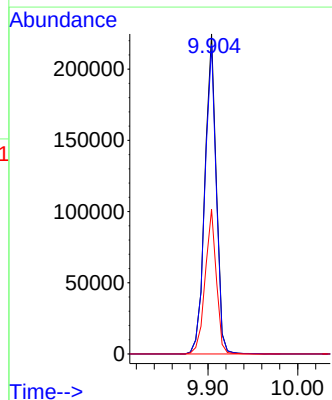
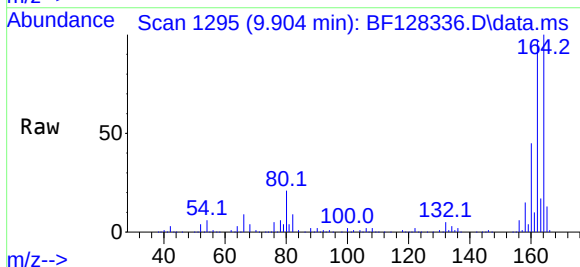




#42
2,4,6-Tribromophenol
Concen: 111.468 ng
RT: 10.698 min Scan# 1436
Delta R.T. -0.012 min
Lab File: BF128336.D
Acq: 19 May 2022 14:58




Instrument :
BNA_F
ClientSampleId :
PB144922TB


Tgt Ion:330 Resp: 252586
Ion Ratio Lower Upper
330 100
332 96.2 79.0 118.4
141 34.0 28.9 43.3

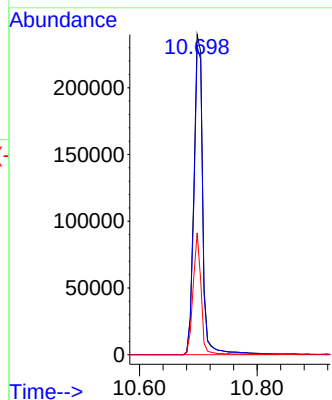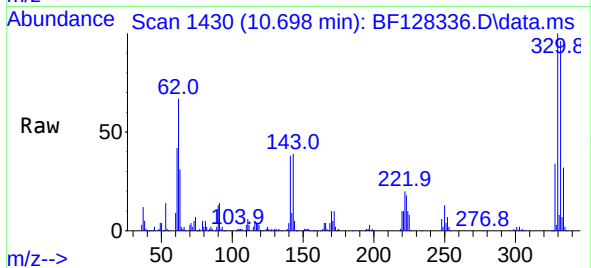

#45
2-Fluorobiphenyl
Concen: 84.576 ng
RT: 9.222 min Scan# 1179
Delta R.T. -0.012 min
Lab File: BF128336.D
Acq: 19 May 2022 14:58

Tgt Ion:172 Resp: 1067974
Ion Ratio Lower Upper
172 100
171 35.1 28.6 42.8
170 23.6 19.1 28.7


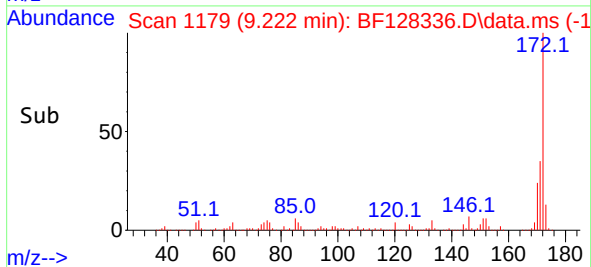
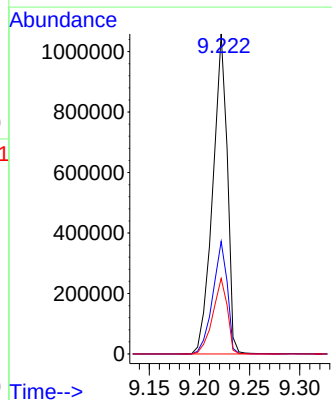
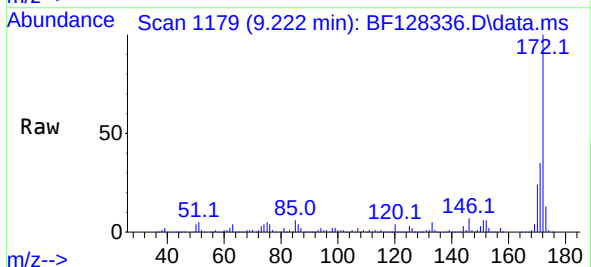




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.398 min Scan# 11
Delta R.T. -0.006 min
Lab File: BF128336.D
Acq: 19 May 2022 14:58




Instrument :
BNA_F
ClientSampleId :
PB144922TB


Tgt Ion:188 Resp: 371510
Ion Ratio Lower Upper
188 100
94 8.5 8.0 12.0
80 9.8 8.9 13.3

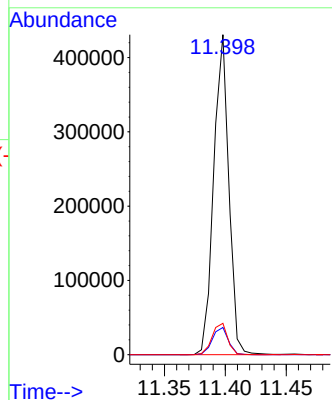

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.045 min Scan# 1999
Delta R.T. -0.012 min
Lab File: BF128336.D
Acq: 19 May 2022 14:58

Tgt Ion:240 Resp: 264828
Ion Ratio Lower Upper
240 100
120 9.3 7.0 10.6
236 24.9 20.3 30.5


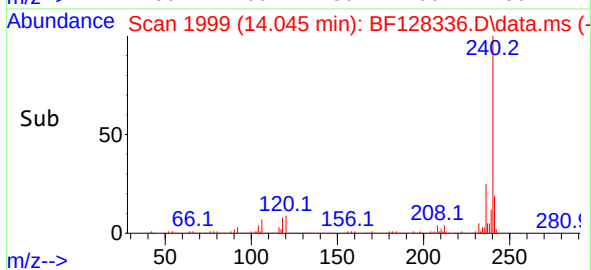
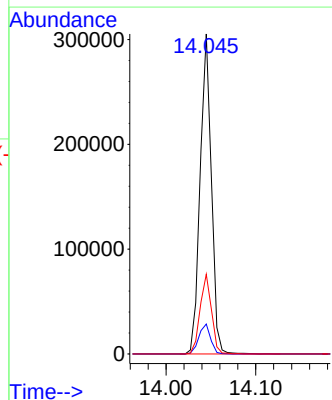





#79
 Terphenyl-d14
 Concen: 87.101 ng
 RT: 12.986 min Scan# 11
 Delta R.T. -0.006 min
 Lab File: BF128336.D
 Acq: 19 May 2022 14:58

Instrument :
 BNA_F
 ClientSampleId :
 PB144922TB

Tgt Ion:244 Resp: 1229304
 Ion Ratio Lower Upper
 244 100
 212 7.8 6.2 9.4
 122 10.1 8.6 12.8

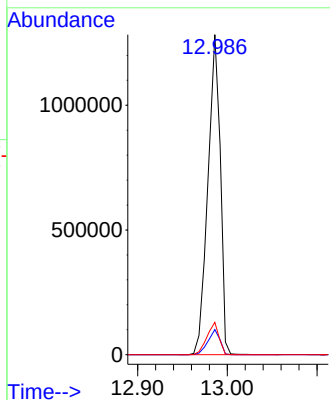

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.533 min Scan# 2252
 Delta R.T. -0.012 min
 Lab File: BF128336.D
 Acq: 19 May 2022 14:58

Tgt Ion:264 Resp: 196336
 Ion Ratio Lower Upper
 264 100
 260 24.1 20.1 30.1
 265 21.3 17.5 26.3

