

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051922\
 Data File : BF128334.D
 Acq On : 19 May 2022 14:00
 Operator : CG\JU
 Sample : PB144922BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB144922BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128334.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.499	541	546	549	rBV	2616525	2538389	79.45%	13.179%
2	6.498	711	716	719	rBV	2411499	2585114	80.91%	13.422%
3	6.863	774	778	782	rBV	679872	542275	16.97%	2.815%
4	7.434	869	875	878	rBV	1613861	1735914	54.33%	9.013%
5	8.145	992	996	1004	rBV	795671	713146	22.32%	3.703%
6	9.222	1173	1179	1182	rBV	3173419	3123467	97.76%	16.217%
7	9.904	1290	1295	1299	rBV	972846	820617	25.68%	4.261%
8	10.698	1426	1430	1452	rBV	2015423	1965777	61.53%	10.206%
9	11.398	1545	1549	1552	rBV	1049795	853343	26.71%	4.431%
10	12.986	1814	1819	1822	rBV	3327630	3194973	100.00%	16.588%
11	14.045	1995	1999	2003	rBV	759952	667727	20.90%	3.467%
12	15.533	2247	2252	2263	rBV2	396673	519774	16.27%	2.699%




Sum of corrected areas: 19260516

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051922\
Data File : BF128334.D
Acq On : 19 May 2022 14:00
Operator : CG\JU
Sample : PB144922BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB144922BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

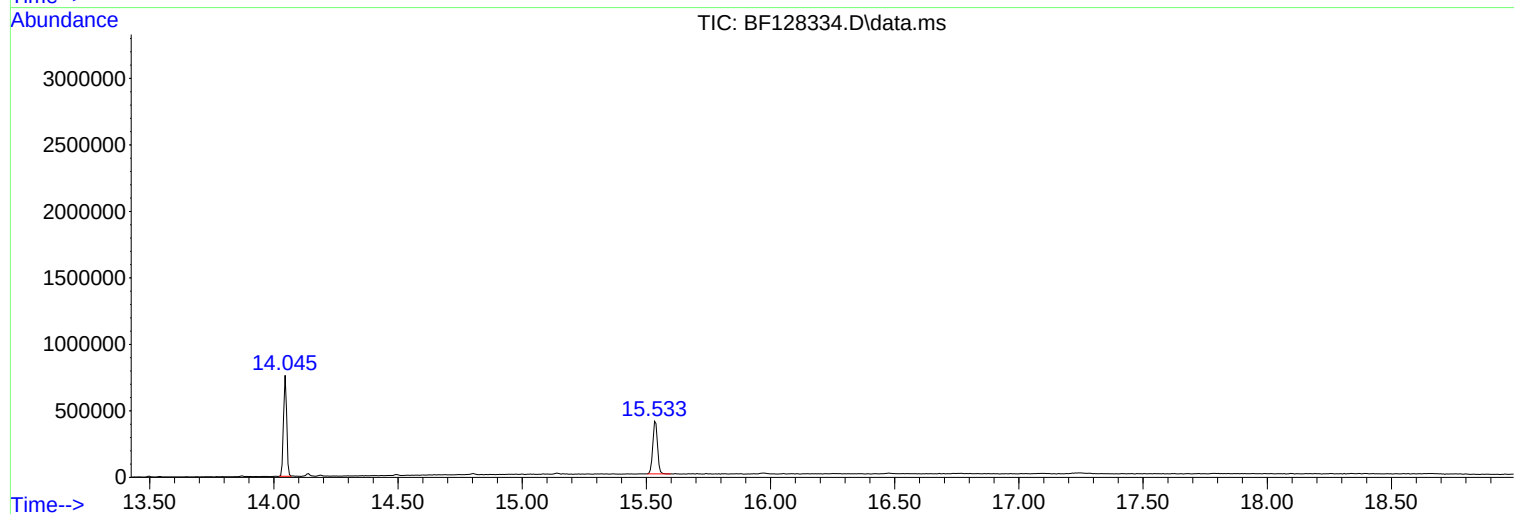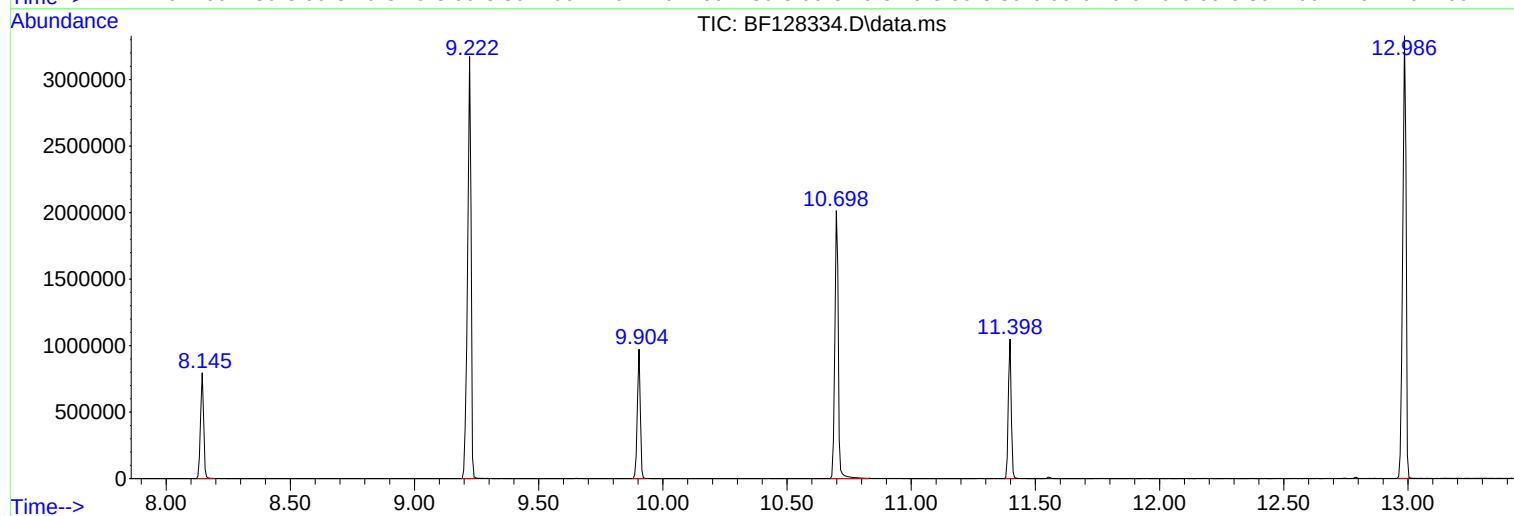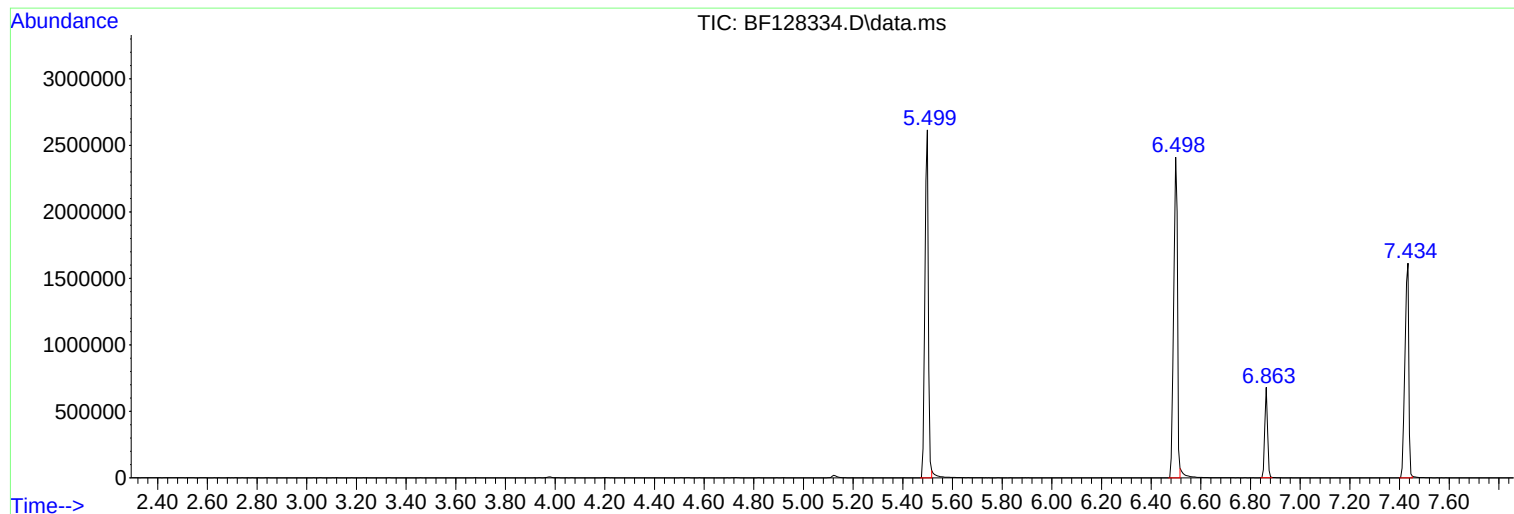

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051922\
Data File : BF128334.D
Acq On : 19 May 2022 14:00
Operator : CG\JU
Sample : PB144922BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB144922BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051922\
Data File : BF128334.D
Acq On : 19 May 2022 14:00
Operator : CG\JU
Sample : PB144922BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB144922BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------