

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051922\
 Data File : BF128344.D
 Acq On : 19 May 2022 18:57
 Operator : CG\JU
 Sample : N2864-07
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 P011-SS003-1824-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128344.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.487	540	544	557	rBV	1884609	1723099	90.05%	12.864%
2	6.498	711	716	727	rBV	1784453	1751987	91.56%	13.080%
3	6.863	774	778	785	rBV	629335	499606	26.11%	3.730%
4	7.428	870	874	877	rBV	1361637	1168717	61.08%	8.725%
5	8.145	992	996	999	rBV	797450	649359	33.94%	4.848%
6	9.222	1174	1179	1182	rBV	2154900	1913516	100.00%	14.286%
7	9.904	1291	1295	1298	rBV	837889	717609	37.50%	5.357%
8	10.698	1426	1430	1443	rBV	1367489	1279051	66.84%	9.549%
9	11.392	1545	1548	1552	rBV	790307	723658	37.82%	5.403%
10	12.980	1814	1818	1821	rBV	2018425	1711298	89.43%	12.776%
11	13.892	1966	1973	1988	rBV4	42948	147313	7.70%	1.100%
12	14.045	1995	1999	2002	rBV	591162	545368	28.50%	4.072%
13	14.133	2010	2014	2018	rBV	31256	30702	1.60%	0.229%
14	15.533	2247	2252	2260	rBV	427810	533373	27.87%	3.982%




Sum of corrected areas: 13394656

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051922\
Data File : BF128344.D
Acq On : 19 May 2022 18:57
Operator : CG\JU
Sample : N2864-07
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P011-SS003-1824-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

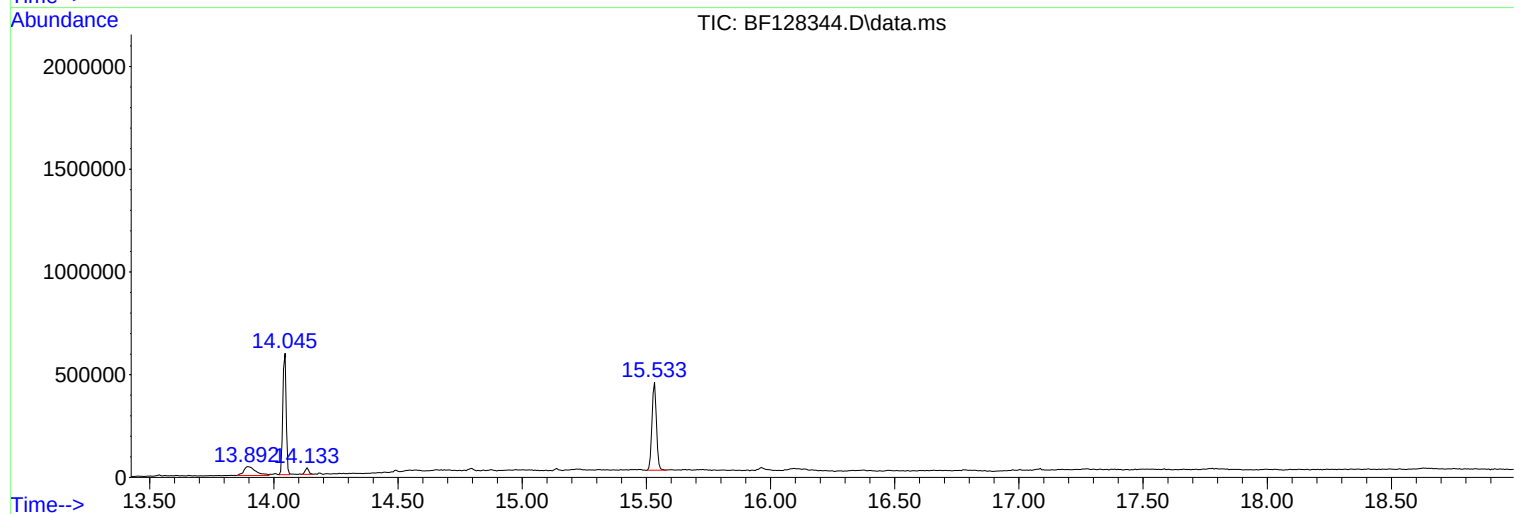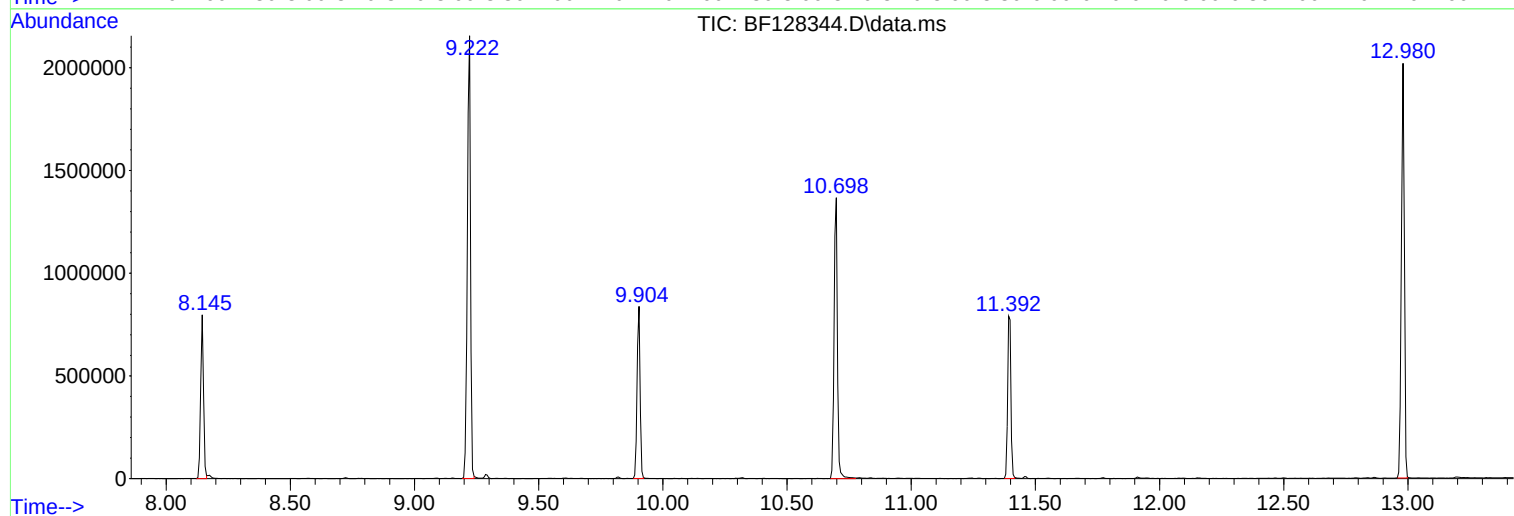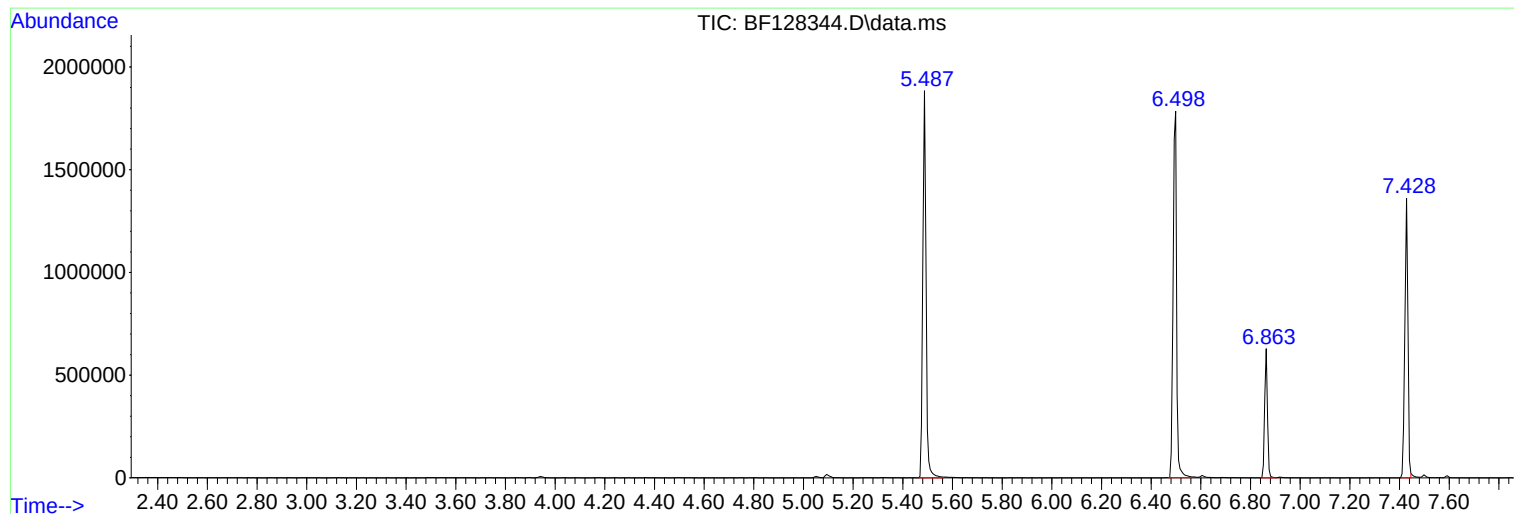

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051922\
Data File : BF128344.D
Acq On : 19 May 2022 18:57
Operator : CG\JU
Sample : N2864-07
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P011-SS003-1824-01










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 n-Nonadecanol-1 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.892	5.40 ng	147313	Chrysene-d12	14.045

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			n-Nonadecanol-1	284	C19H40O	001454-84-8	95
2			Trifluoroacetoxy hexadecane	338	C18H33F3O2	006222-03-3	94
3			Bromoacetic acid, hexadecyl ester	362	C18H35BrO2	005454-48-8	94
4			Behenic alcohol	326	C22H46O	000661-19-8	94
5			1-Tricosene	322	C23H46	018835-32-0	94

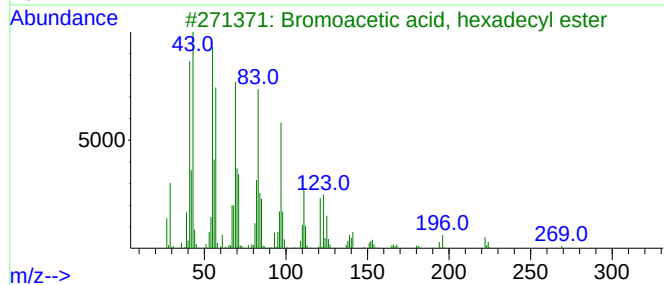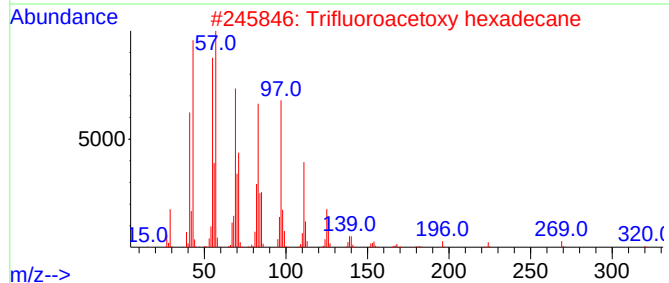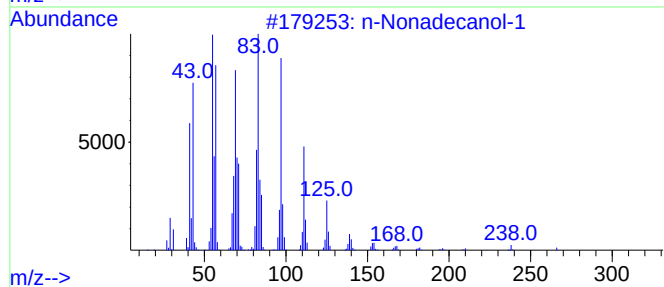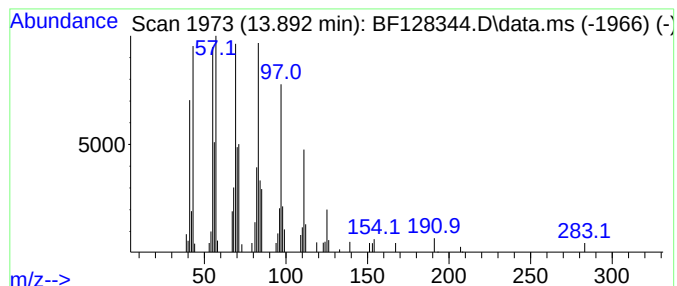

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051922\
Data File : BF128344.D
Acq On : 19 May 2022 18:57
Operator : CG\JU
Sample : N2864-07
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P011-SS003-1824-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
n-Nonadecanol-1	13.892	5.4	ng	147313	5	14.045	545368	20.0