

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051922\
 Data File : BF128346.D
 Acq On : 19 May 2022 19:56
 Operator : CG\JU
 Sample : N2934-08
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 RB-220513

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128346.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.093	474	477	490	rVB	96824	114663	3.32%	0.654%
2	5.487	541	544	563	rBV	1468120	1512820	43.80%	8.626%
3	6.493	711	715	727	rBV	1389973	1249526	36.18%	7.124%
4	6.863	774	778	785	rBV	646068	523915	15.17%	2.987%
5	7.434	869	875	878	rBV	2115825	2187984	63.35%	12.475%
6	8.145	992	996	1004	rVB	782313	678027	19.63%	3.866%
7	8.704	1088	1091	1099	rBV	37693	41386	1.20%	0.236%
8	9.222	1173	1179	1182	rBV	3603140	3453941	100.00%	19.693%
9	9.904	1288	1295	1298	rBV	876627	744108	21.54%	4.243%
10	10.698	1426	1430	1445	rBV	1553977	1456663	42.17%	8.305%
11	11.398	1545	1549	1552	rBV	823041	746914	21.62%	4.259%
12	11.769	1609	1612	1616	rVB	132309	100394	2.91%	0.572%
13	12.986	1814	1819	1822	rBV	3328952	3103805	89.86%	17.697%
14	14.045	1995	1999	2002	rBV	495025	449283	13.01%	2.562%
15	14.786	2121	2125	2134	rBV	623881	646846	18.73%	3.688%
16	15.533	2247	2252	2260	rVB	422738	528455	15.30%	3.013%




Sum of corrected areas: 17538730

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051922\
Data File : BF128346.D
Acq On : 19 May 2022 19:56
Operator : CG\JU
Sample : N2934-08
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
RB-220513

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

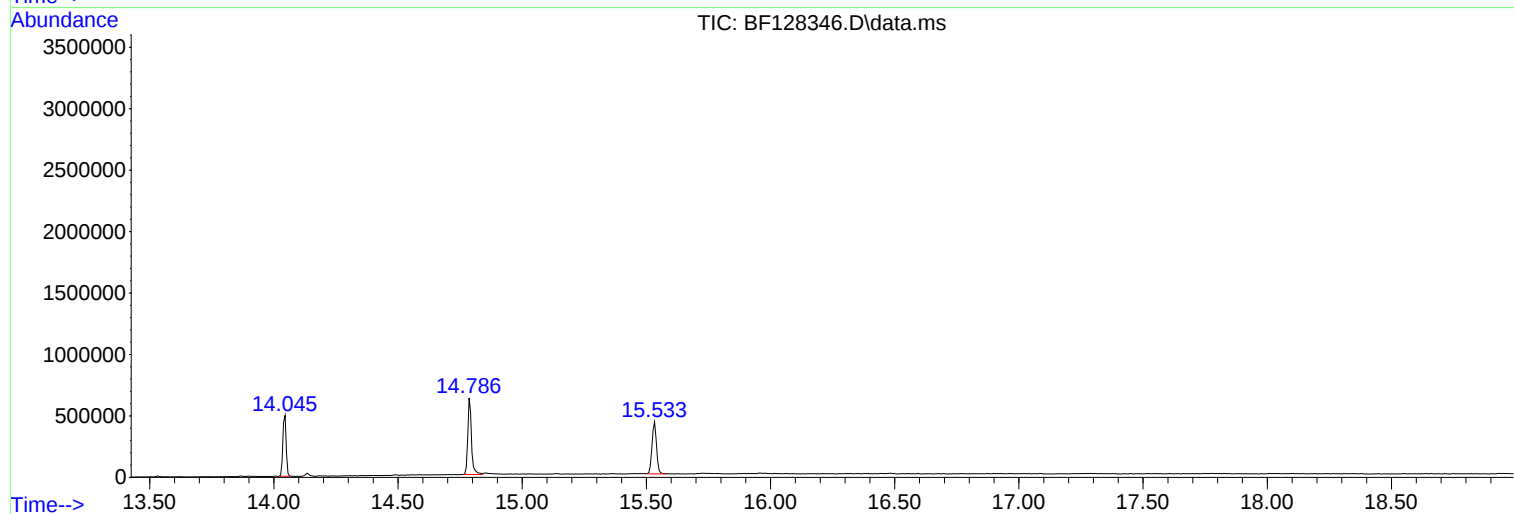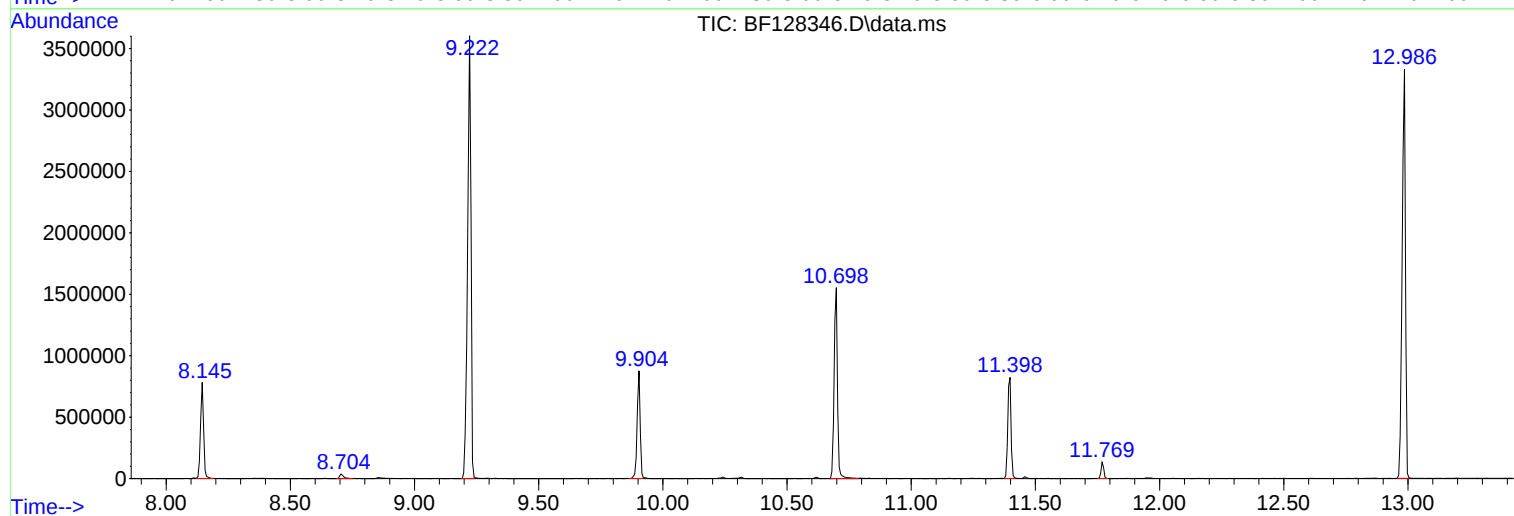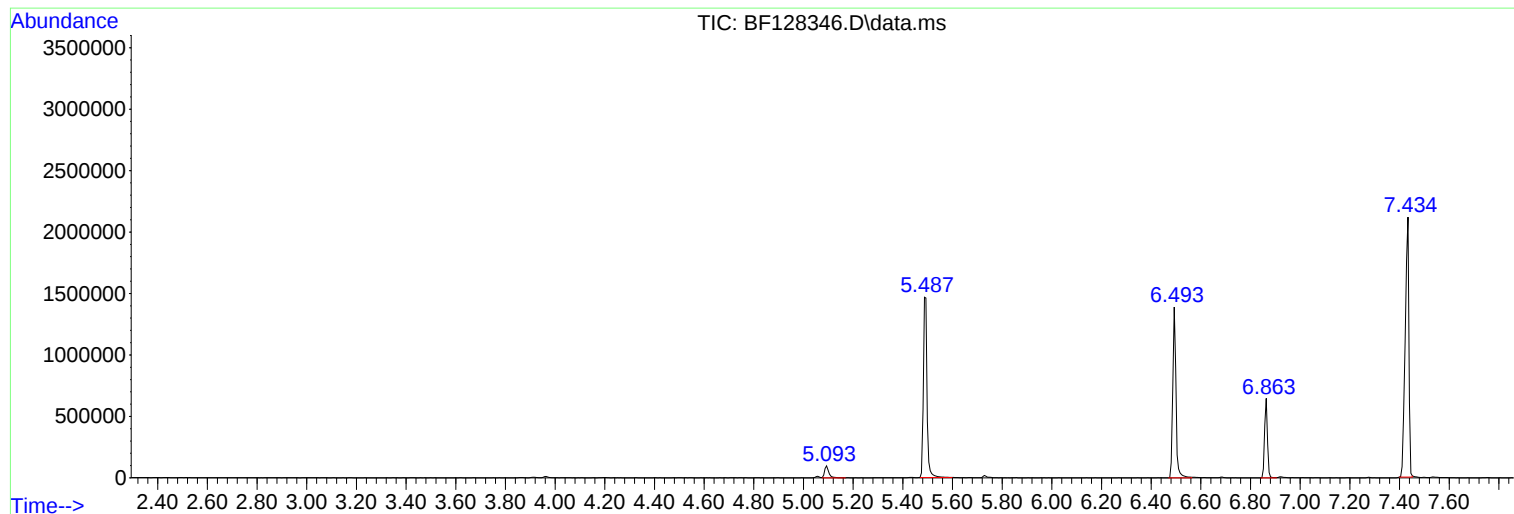

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051922\
Data File : BF128346.D
Acq On : 19 May 2022 19:56
Operator : CG\JU
Sample : N2934-08
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
RB-220513

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051922\
Data File : BF128346.D
Acq On : 19 May 2022 19:56
Operator : CG\JU
Sample : N2934-08
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
RB-220513

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc