

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051922\
 Data File : BF128348.D
 Acq On : 19 May 2022 20:55
 Operator : CG\JU
 Sample : N2864-06
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 P011-SS003-1218-01

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128348.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.087	473	476	487	rVB	28445	37576	2.03%	0.301%
2	5.487	540	544	564	rBV	1718703	1652260	89.15%	13.237%
3	6.492	711	715	732	rBV	1647095	1664760	89.82%	13.337%
4	6.863	774	778	786	rBV	640954	509247	27.48%	4.080%
5	7.428	870	874	877	rBV	1328881	1136188	61.30%	9.103%
6	8.145	992	996	1000	rBV	780891	639440	34.50%	5.123%
7	9.222	1174	1179	1182	rBV	2072891	1853435	100.00%	14.849%
8	9.904	1291	1295	1298	rBV	854489	701124	37.83%	5.617%
9	10.698	1426	1430	1442	rBV	1194849	1134707	61.22%	9.091%
10	11.392	1545	1548	1552	rBV	718179	670166	36.16%	5.369%
11	12.980	1814	1818	1821	rBV	1676082	1398916	75.48%	11.207%
12	13.915	1971	1977	1984	rBV7	13030	37030	2.00%	0.297%
13	14.045	1995	1999	2007	rBV	450775	435431	23.49%	3.488%
14	14.133	2011	2014	2019	rVB	22484	23520	1.27%	0.188%
15	14.786	2122	2125	2132	rVB2	39090	43293	2.34%	0.347%
16	15.533	2247	2252	2259	rVB	396439	504120	27.20%	4.039%
17	15.956	2321	2324	2328	rBV4	13371	20435	1.10%	0.164%
18	17.074	2509	2514	2524	rVB9	9489	20353	1.10%	0.163%




Sum of corrected areas: 12482001

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051922\
Data File : BF128348.D
Acq On : 19 May 2022 20:55
Operator : CG\JU
Sample : N2864-06
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P011-SS003-1218-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

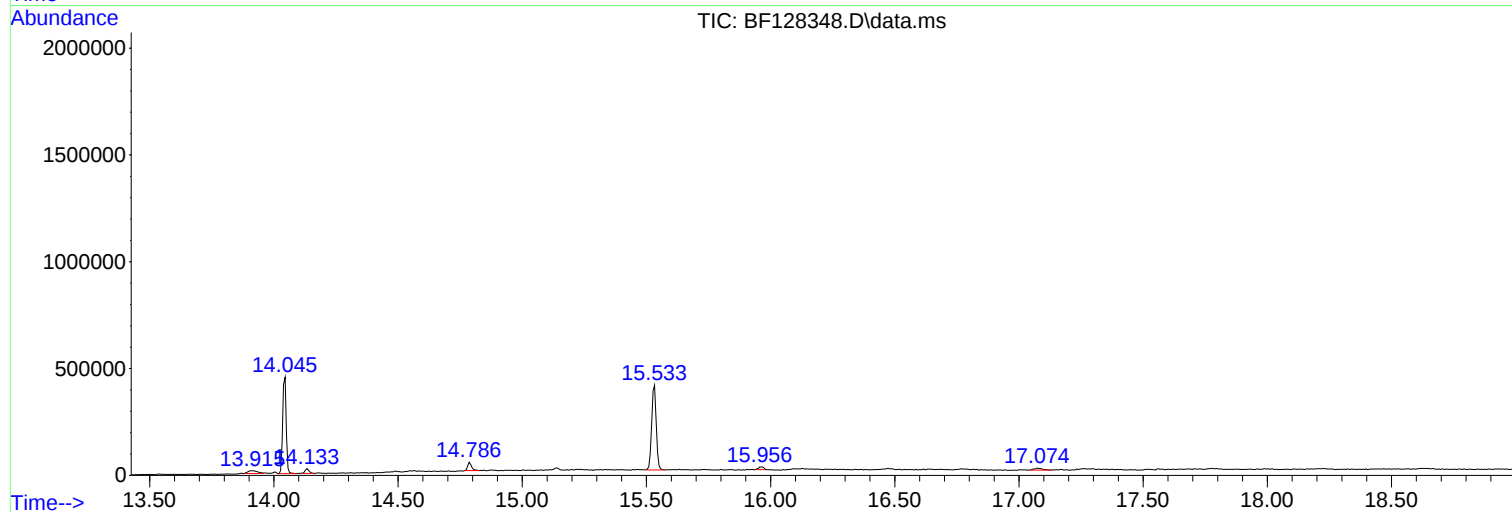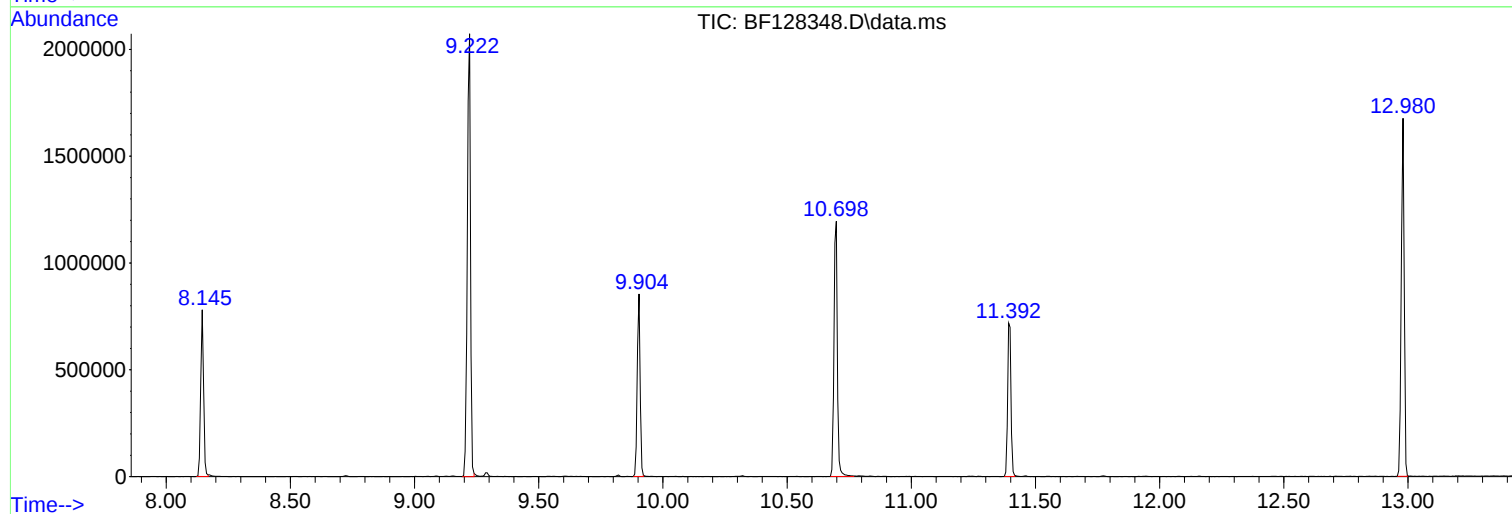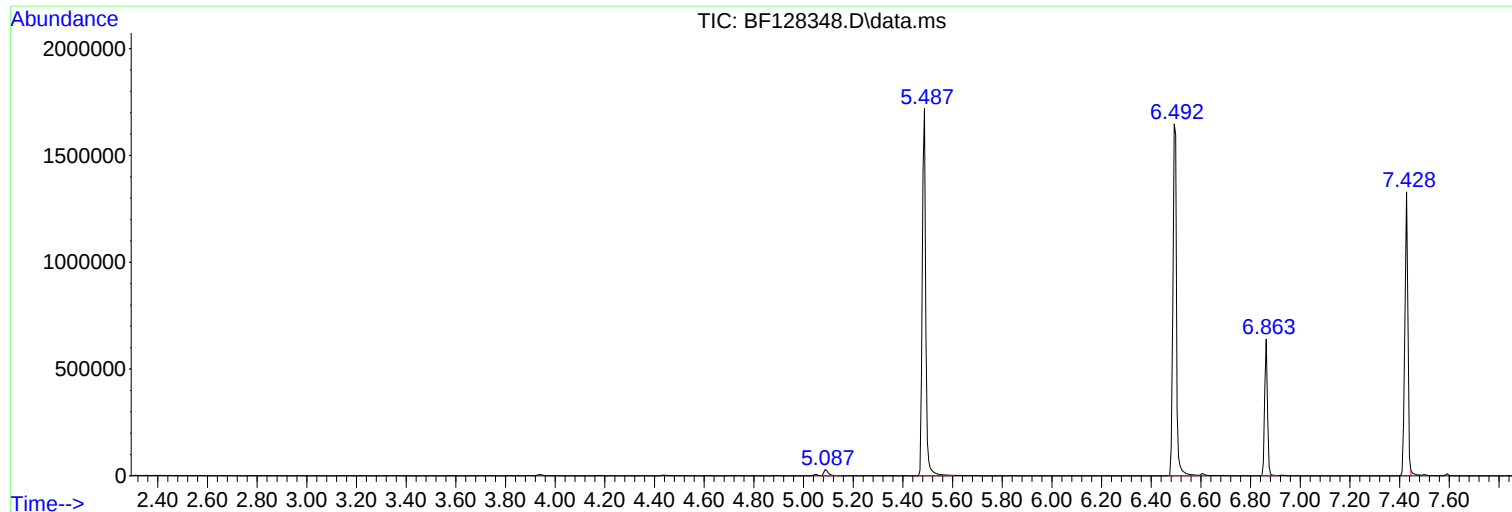

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051922\
Data File : BF128348.D
Acq On : 19 May 2022 20:55
Operator : CG\JU
Sample : N2864-06
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P011-SS003-1218-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051922\
Data File : BF128348.D
Acq On : 19 May 2022 20:55
Operator : CG\JU
Sample : N2864-06
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P011-SS003-1218-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------