

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051922\
 Data File : BF128349.D
 Acq On : 19 May 2022 21:25
 Operator : CG\JU
 Sample : N2864-08
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 P011-SS003-2430-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128349.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.093	474	477	486	rVB	24483	31681	1.68%	0.235%
2	5.487	540	544	565	rBV	1845598	1828672	96.73%	13.542%
3	6.498	711	716	732	rBV	1780736	1877349	99.31%	13.903%
4	6.863	774	778	782	rBV	633141	517297	27.36%	3.831%
5	7.428	870	874	877	rBV	1389709	1235579	65.36%	9.150%
6	8.145	992	996	1004	rBV	784590	650863	34.43%	4.820%
7	9.222	1174	1179	1182	rBV	2070544	1890473	100.00%	14.000%
8	9.904	1291	1295	1298	rBV	823969	694274	36.72%	5.142%
9	10.698	1426	1430	1444	rBV	1262626	1236798	65.42%	9.159%
10	11.392	1545	1548	1552	rBV	808747	707210	37.41%	5.237%
11	12.980	1814	1818	1821	rBV	1805493	1524056	80.62%	11.287%
12	13.898	1966	1974	1989	rBV4	57665	206298	10.91%	1.528%
13	14.045	1995	1999	2002	rBV	496954	473777	25.06%	3.509%
14	14.133	2010	2014	2018	rBV	24815	25240	1.34%	0.187%
15	14.786	2121	2125	2132	rBV2	55207	61496	3.25%	0.455%
16	15.533	2246	2252	2258	rBV2	415274	542181	28.68%	4.015%

Sum of corrected areas: 13503244

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051922\
Data File : BF128349.D
Acq On : 19 May 2022 21:25
Operator : CG\JU
Sample : N2864-08
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P011-SS003-2430-01










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Dichloroacetic acid, heptad... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.898	8.71 ng	206298	Chrysene-d12	14.045

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Dichloroacetic acid, heptadecyl ...	366	C19H36Cl2O2	1000282-98-2	95
2			Trichloroacetic acid, pentadecyl...	372	C17H31Cl3O2	074339-53-0	95
3			Heptafluorobutyric acid, n-tetra...	410	C18H29F7O2	007365-36-8	94
4			2- Chloropropionic acid, octadec...	360	C21H41ClO2	088104-31-8	94
5			Heptafluorobutyric acid, pentade...	424	C19H31F7O2	959261-23-5	93

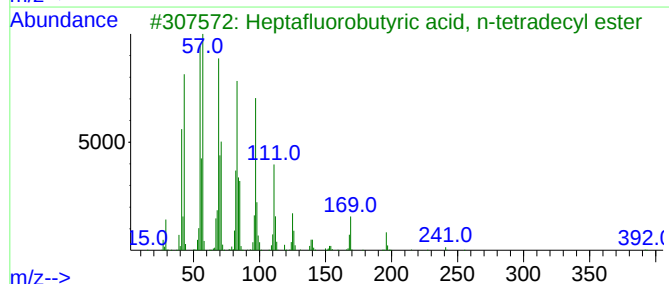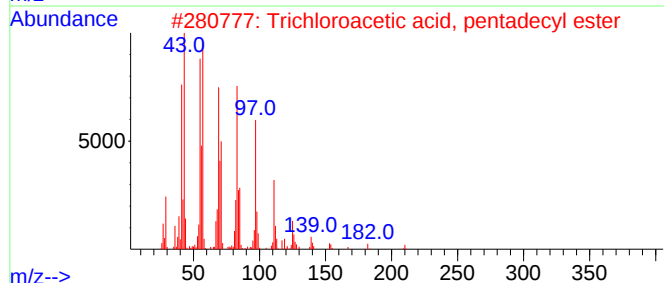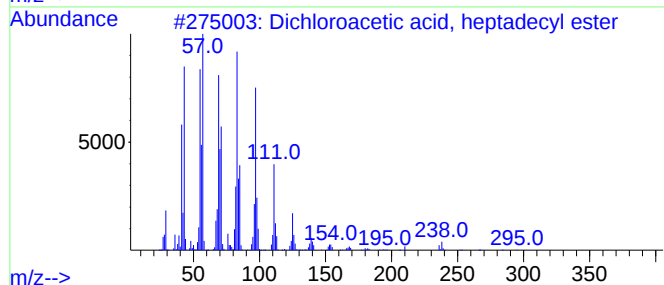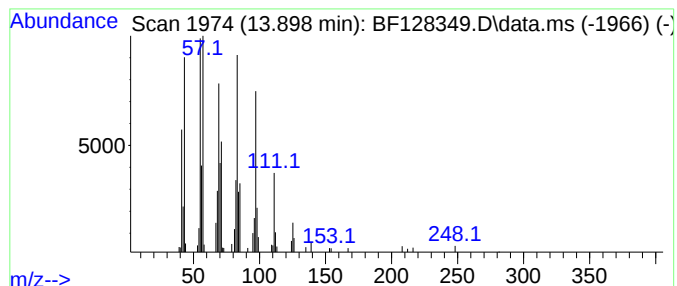

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051922\
Data File : BF128349.D
Acq On : 19 May 2022 21:25
Operator : CG\JU
Sample : N2864-08
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P011-SS003-2430-01










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 9-Octadecenamide, (Z)- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.786	2.60 ng	61496	Chrysene-d12	14.045

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		9-Octadecenamide, (Z)-	281	C18H35NO	000301-02-0	95
2		13-Docosenamide, (Z)-	337	C22H43NO	000112-84-5	76
3		Hexadecanamide	255	C16H33NO	000629-54-9	59
4		Octadecanamide	283	C18H37NO	000124-26-5	59
5		Palmitoleamide	253	C16H31NO	106010-22-4	58

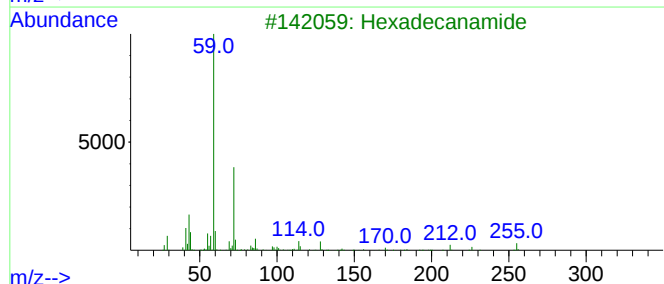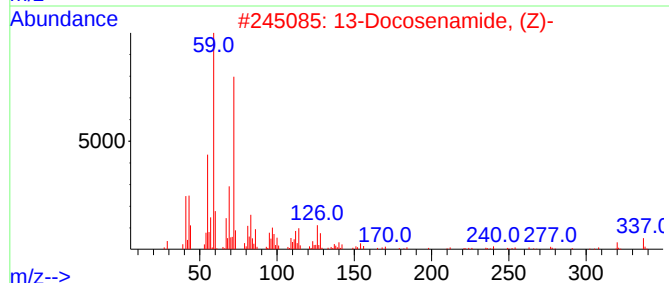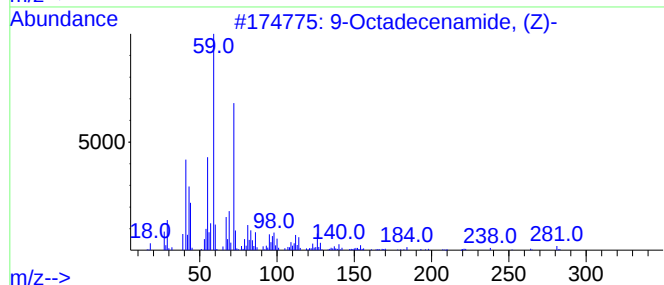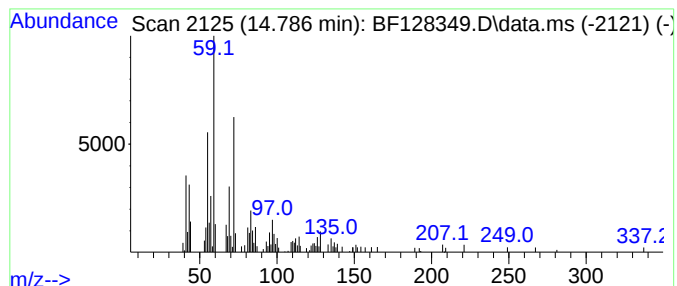

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051922\
Data File : BF128349.D
Acq On : 19 May 2022 21:25
Operator : CG\JU
Sample : N2864-08
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P011-SS003-2430-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Dichloroacetic ...	13.898	8.7	ng	206298	5	14.045	473777	20.0
9-Octadecenamid...	14.786	2.6	ng	61496	5	14.045	473777	20.0