
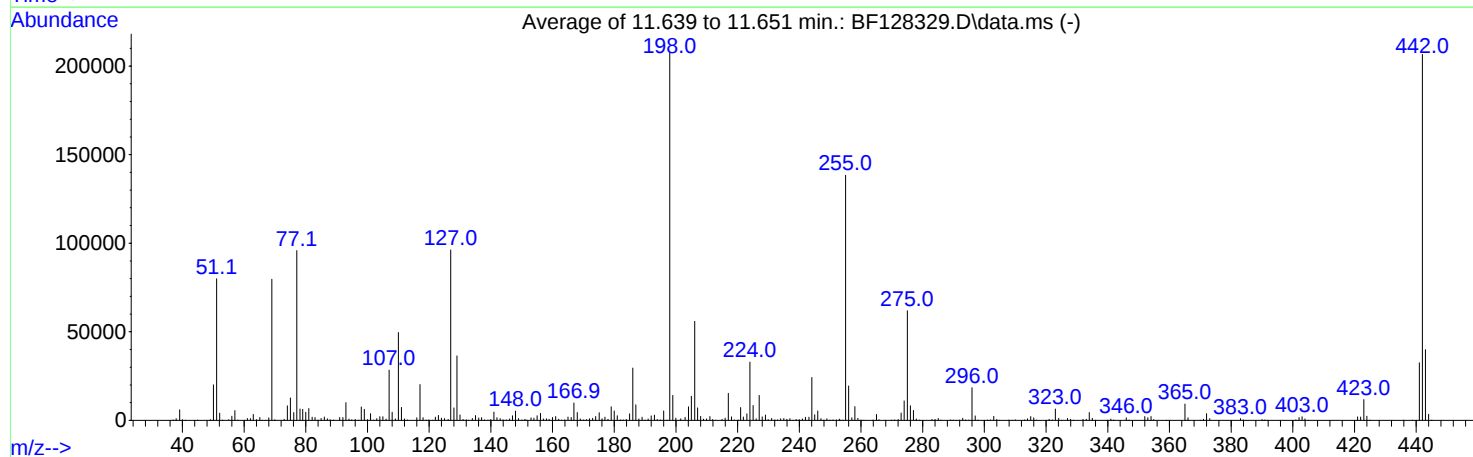


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051922\
 Data File : BF128329.D
 Acq On : 19 May 2022 11:35
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 19 06:47:51 2022

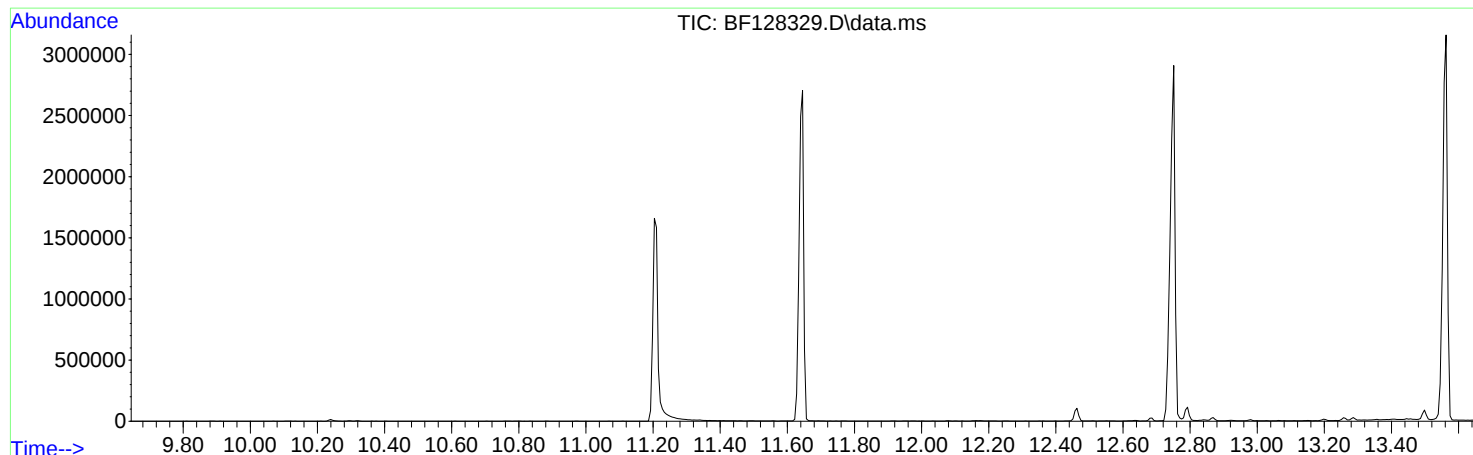




AutoFind: Scans 1590, 1591, 1592; Background Corrected with Scan 1584

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.5	79938	PASS
68	69	0.00	2	1.8	1430	PASS
69	198	0.00	100	38.4	79636	PASS
70	69	0.00	2	0.5	406	PASS
127	198	10	80	46.3	96195	PASS
197	198	0.00	2	0.1	161	PASS
198	198	100	100	100.0	207651	PASS
199	198	5	9	6.8	14124	PASS
275	198	10	60	29.8	61837	PASS
365	198	1	100	4.5	9254	PASS
441	198	0.01	100	15.7	32509	PASS
442	442	50	100	100.0	206592	PASS
443	442	15	24	19.3	39928	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051922\
Data File : BF128329.D
Acq On : 19 May 2022 11:35
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 19 17:10:33 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 19 06:47:51 2022
Response via : Initial Calibration

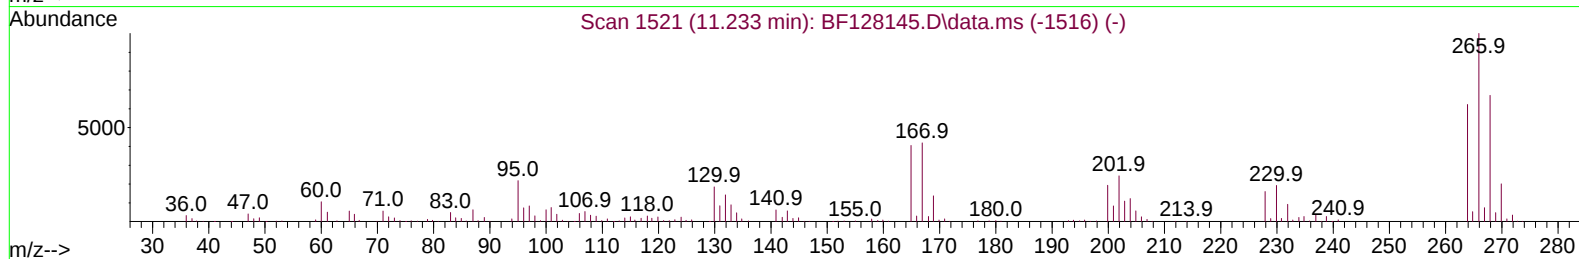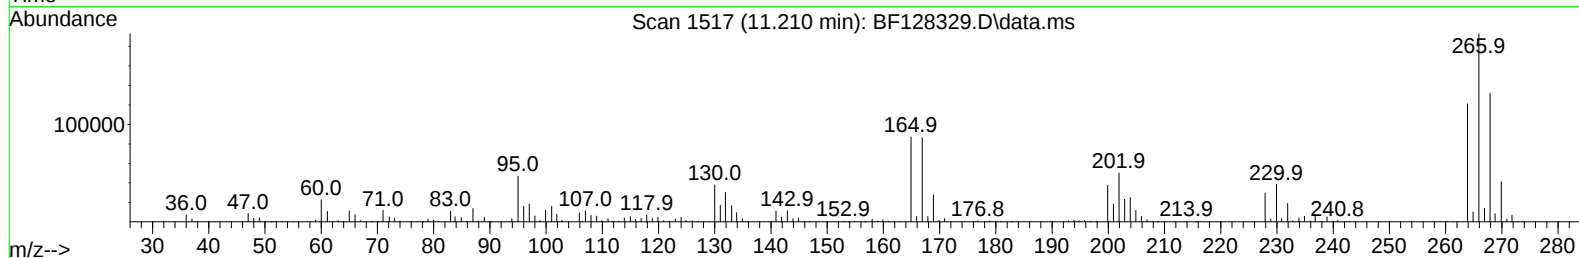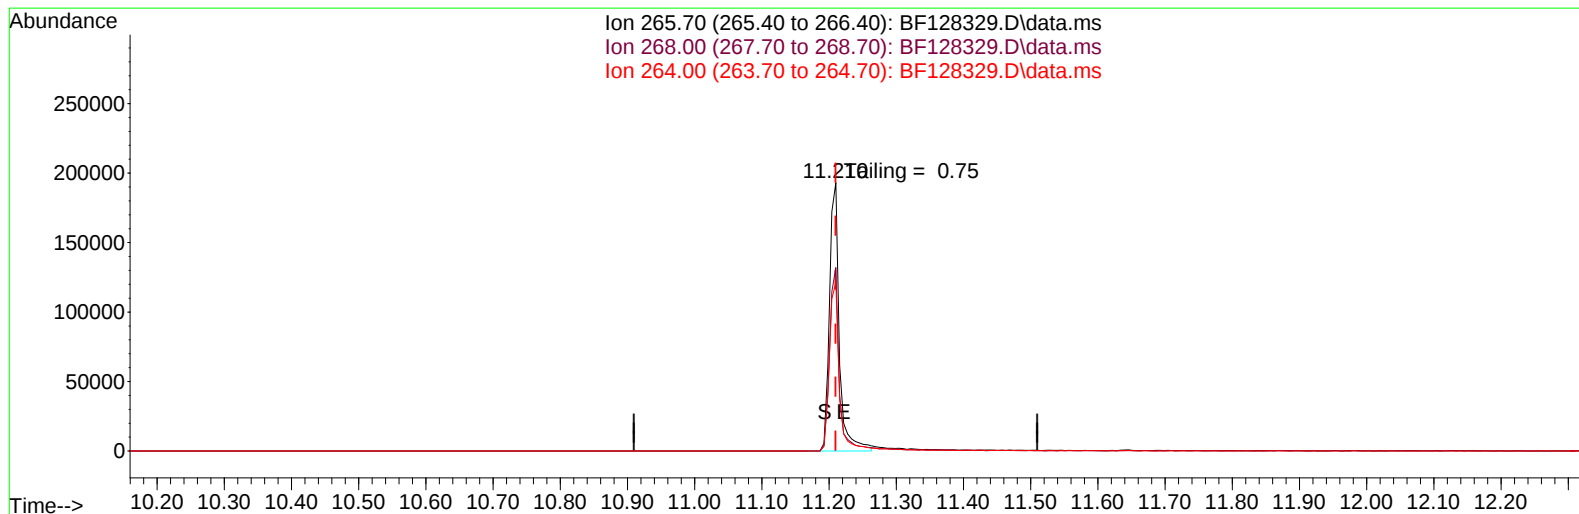

TIC: BF128329.D\data.ms

(70) Pentachlorophenol (C)

11.210min (+ 0.000) 279486.14 ng




response 204330

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.30	68.32
264.00	66.40	62.79
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051922\  
Data File : BF128329.D  
Acq On    : 19 May 2022  11:35  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 19 17:10:33 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 19 06:47:51 2022
Response via : Initial Calibration

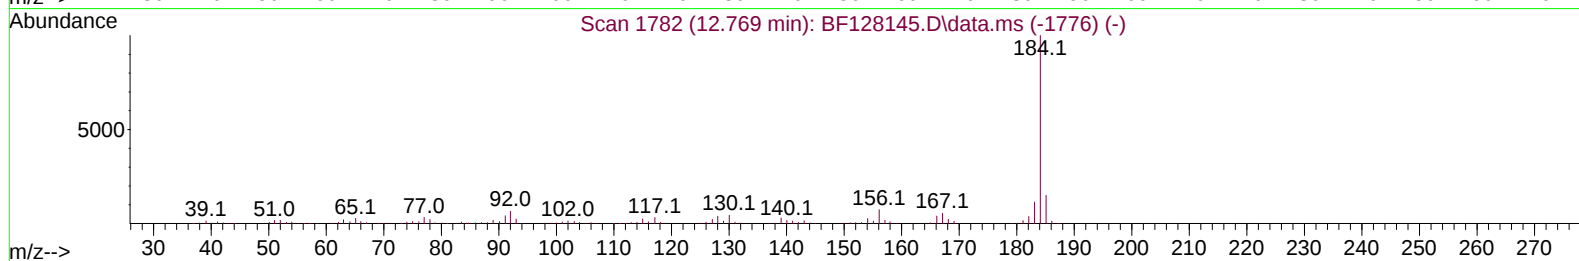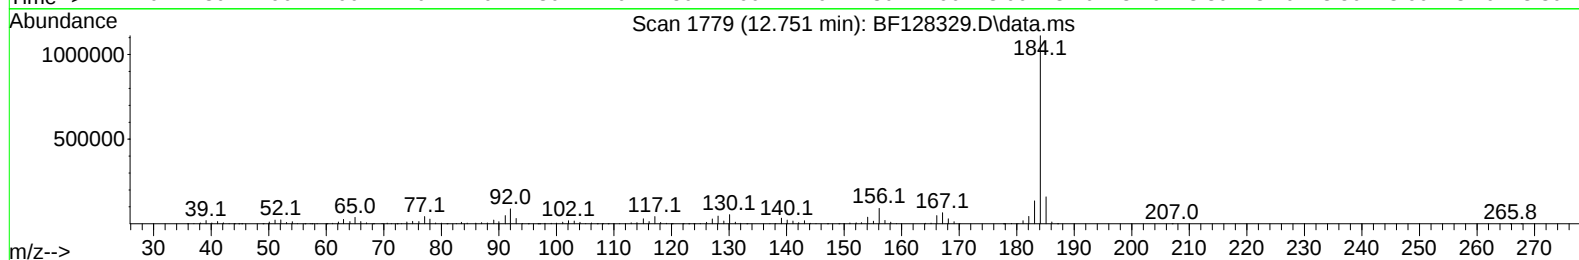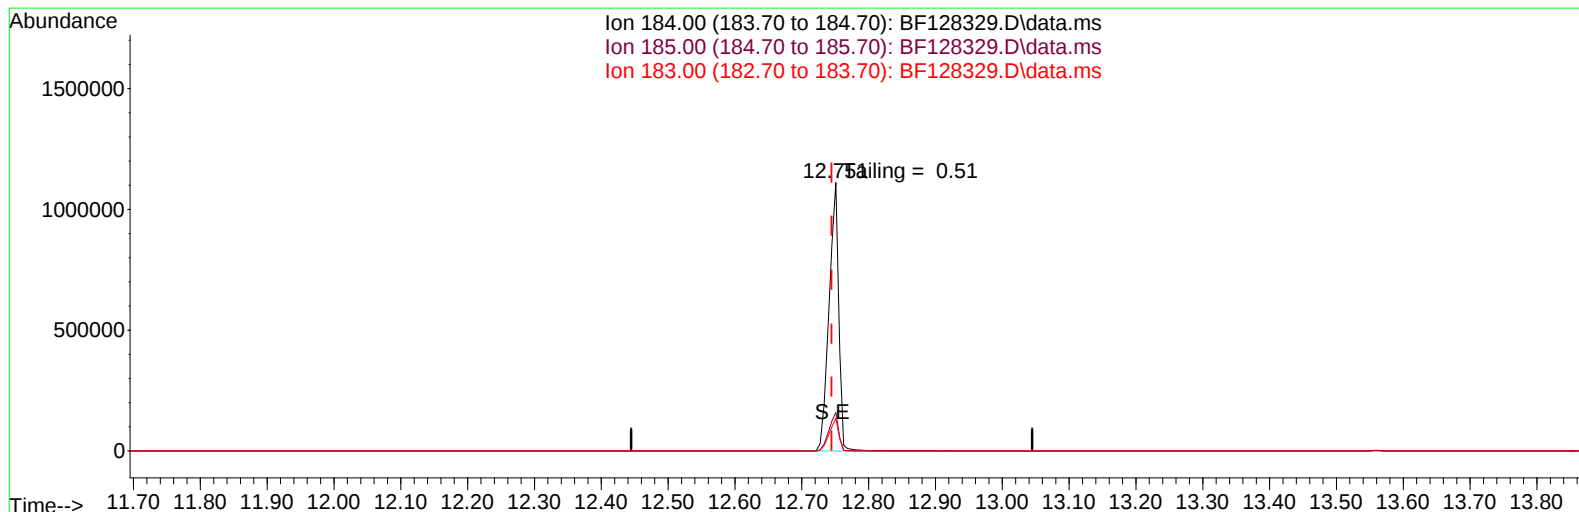

TIC: BF128329.D\data.ms

(77) Benzidine

12.751min (+ 0.006) 51730.25 ng

response 1123751

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.33
183.00	11.20	12.16
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/19/2022	BNA_F	<u>BF128329.D</u>
Compound Name	Response	Retention Time
DDT	560326	13.56
DDD	4964	13.26
DDE	1002	12.92
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5966	566292	1.05

Instrument :
BNA_F
ClientSampleId :
DFTPP