

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051925\
 Data File : BF142461.D
 Acq On : 19 May 2025 19:54
 Operator : RC/JU
 Sample : Q1984-09
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU4-TS-25-050725

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050525.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF142461.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.387	198	203	224	rBV	30672	91501	4.97%	0.545%
2	5.110	488	496	504	rBV	109077	164945	8.97%	0.982%
3	5.516	559	565	570	rBV	1126866	1485194	80.73%	8.845%
4	6.522	730	736	748	rVB	1144407	1535601	83.47%	9.145%
5	6.728	764	771	777	rBV	26180	34254	1.86%	0.204%
6	6.904	796	801	806	rBV	427496	519449	28.24%	3.093%
7	7.463	890	896	901	rBV	775663	972697	52.87%	5.793%
8	8.186	1013	1019	1034	rVB	553070	691183	37.57%	4.116%
9	8.492	1066	1071	1082	rBV	64984	88455	4.81%	0.527%
10	9.257	1195	1201	1206	rBV	1507910	1839618	100.00%	10.956%
11	9.528	1239	1247	1252	rBV2	30106	44487	2.42%	0.265%
12	9.598	1252	1259	1264	rBV5	10302	19627	1.07%	0.117%
13	9.939	1311	1317	1326	rBV	648245	818481	44.49%	4.874%
14	10.028	1326	1332	1342	rVV	329283	523104	28.44%	3.115%
15	10.727	1445	1451	1466	rBV	899067	1187938	64.58%	7.075%
16	11.310	1543	1550	1554	rBV7	6409	18543	1.01%	0.110%
17	11.427	1564	1570	1576	rBV	603769	790759	42.98%	4.709%
18	11.474	1576	1578	1584	rVB3	14051	18822	1.02%	0.112%
19	11.645	1603	1607	1612	rBV5	13307	23801	1.29%	0.142%
20	11.910	1649	1652	1654	rBV	21471	24423	1.33%	0.145%
21	11.945	1654	1658	1671	rVB2	132407	212468	11.55%	1.265%
22	12.121	1684	1688	1698	rBV3	61366	97047	5.28%	0.578%
23	12.204	1699	1702	1705	rBV2	17364	21217	1.15%	0.126%
24	12.639	1772	1776	1779	rBV	44576	65296	3.55%	0.389%
25	12.733	1788	1792	1797	rBV3	28087	45319	2.46%	0.270%
26	12.868	1812	1815	1824	rVB2	23270	36734	2.00%	0.219%
27	13.010	1834	1839	1847	rBV	1153851	1466115	79.70%	8.731%
28	13.445	1909	1913	1917	rBV2	63318	87342	4.75%	0.520%
29	13.904	1988	1991	2002	rVB	87969	143017	7.77%	0.852%
30	14.068	2014	2019	2027	rBV	437405	624201	33.93%	3.717%
31	14.533	2094	2098	2116	rVB2	105421	246530	13.40%	1.468%
32	15.198	2206	2211	2222	rVB	242914	407870	22.17%	2.429%
33	15.557	2267	2272	2282	rVB	311296	518423	28.18%	3.087%
34	16.039	2349	2354	2360	rBV	163149	276955	15.06%	1.649%
35	17.686	2628	2634	2636	rBV2	131450	274571	14.93%	1.635%
36	17.727	2638	2641	2659	rVB3	244553	639715	34.77%	3.810%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051925\
Data File : BF142461.D
Acq On : 19 May 2025 19:54
Operator : RC/JU
Sample : Q1984-09
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-25-050725

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	18.162	2709	2715	2726	rBV	138212	360394	19.59%	2.146%
38	18.527	2769	2777	2781	rBV5	124747	375604	20.42%	2.237%




Sum of corrected areas: 16791700

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051925\
Data File : BF142461.D
Acq On : 19 May 2025 19:54
Operator : RC/JU
Sample : Q1984-09
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-25-050725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

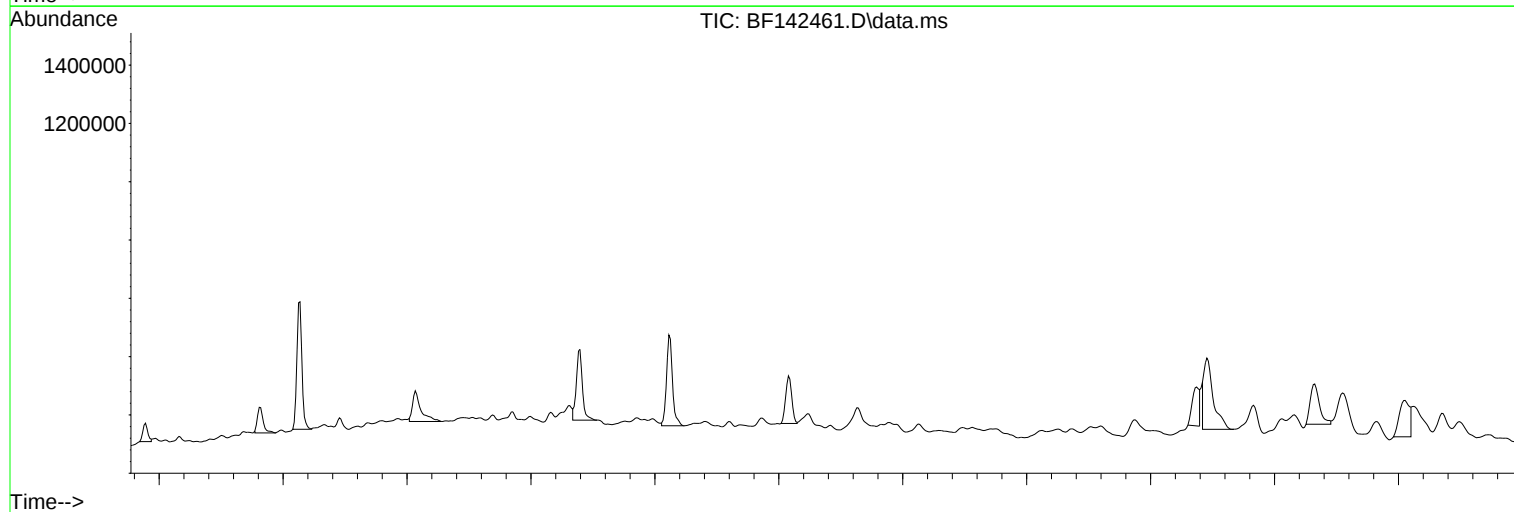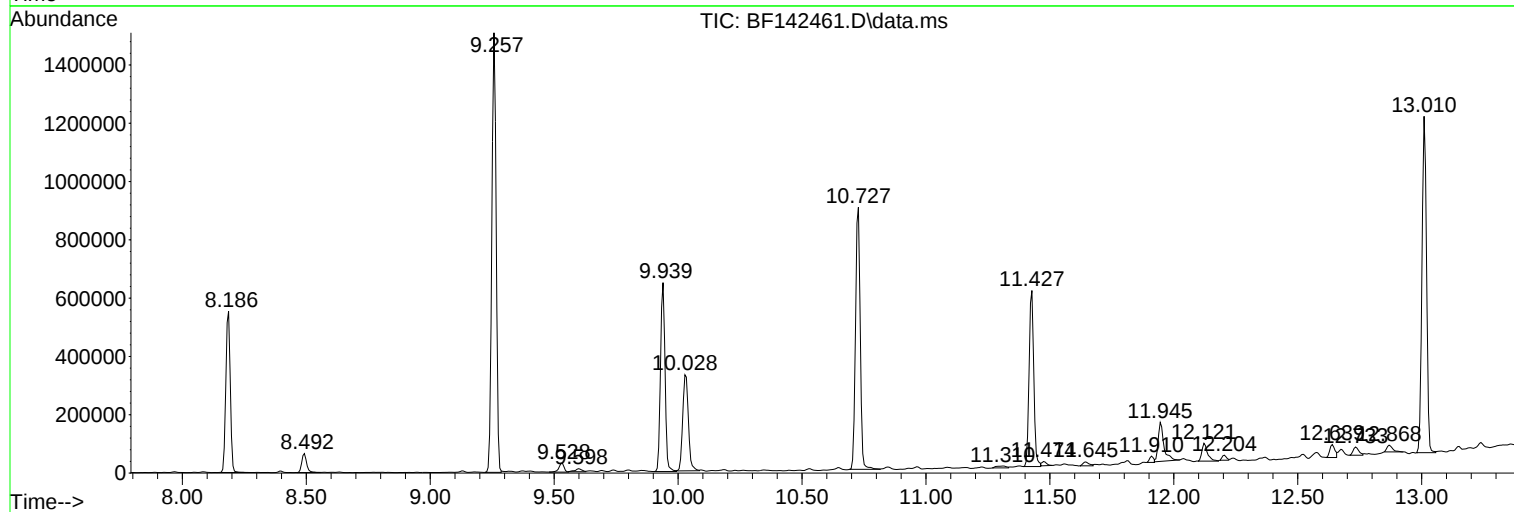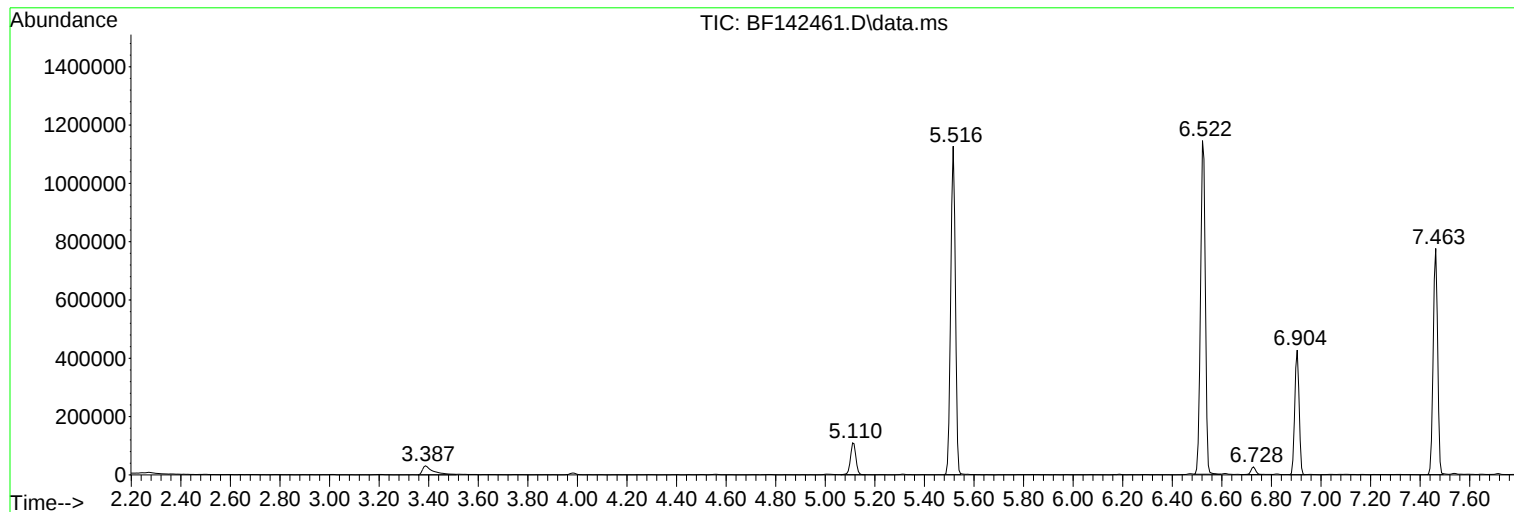

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051925\
Data File : BF142461.D
Acq On : 19 May 2025 19:54
Operator : RC/JU
Sample : Q1984-09
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-25-050725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051925\
Data File : BF142461.D
Acq On : 19 May 2025 19:54
Operator : RC/JU
Sample : Q1984-09
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-25-050725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------