

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051925\
 Data File : BF142462.D
 Acq On : 19 May 2025 20:23
 Operator : RC/JU
 Sample : Q1984-13
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU4-TS-27-050725

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050525.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF142462.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.387	197	203	226	rBV	32235	86390	5.20%	0.497%
2	5.110	488	496	505	rVB	100382	146651	8.82%	0.844%
3	5.516	559	565	570	rBV	1042104	1352103	81.35%	7.783%
4	6.522	730	736	747	rBV	1055930	1387775	83.50%	7.988%
5	6.728	765	771	781	rBV	24531	32267	1.94%	0.186%
6	6.904	796	801	806	rBV	414303	500511	30.11%	2.881%
7	7.463	890	896	901	rBV	700210	876737	52.75%	5.047%
8	8.186	1014	1019	1026	rBV	534466	658946	39.65%	3.793%
9	8.492	1066	1071	1083	rBV	62069	86796	5.22%	0.500%
10	9.257	1196	1201	1206	rBV	1371024	1662093	100.00%	9.567%
11	9.528	1240	1247	1252	rBV2	25677	35040	2.11%	0.202%
12	9.939	1312	1317	1326	rBV	627099	779391	46.89%	4.486%
13	10.033	1326	1333	1342	rBV	823465	1268888	76.34%	7.304%
14	10.651	1434	1438	1445	rVB	20775	26417	1.59%	0.152%
15	10.727	1445	1451	1458	rBV	797214	1070733	64.42%	6.163%
16	11.427	1564	1570	1576	rBV	579107	763549	45.94%	4.395%
17	11.474	1576	1578	1585	rVB4	11720	16624	1.00%	0.096%
18	11.645	1602	1607	1612	rBV4	11201	21988	1.32%	0.127%
19	11.810	1629	1635	1641	rVB4	10878	22567	1.36%	0.130%
20	11.910	1649	1652	1654	rBV	18455	20971	1.26%	0.121%
21	11.945	1654	1658	1668	rVB2	128607	195908	11.79%	1.128%
22	12.122	1684	1688	1697	rVB3	57603	86217	5.19%	0.496%
23	12.204	1698	1702	1706	rBV4	18771	28661	1.72%	0.165%
24	12.574	1760	1765	1769	rBV5	16194	29112	1.75%	0.168%
25	12.639	1772	1776	1779	rBV	57360	78224	4.71%	0.450%
26	12.733	1788	1792	1797	rBV	26393	38528	2.32%	0.222%
27	12.869	1811	1815	1820	rBV	33550	45872	2.76%	0.264%
28	13.010	1834	1839	1849	rVB	1111447	1392821	83.80%	8.017%
29	13.445	1909	1913	1924	rVB3	68017	133105	8.01%	0.766%
30	13.904	1987	1991	2002	rVB	85055	142969	8.60%	0.823%
31	14.063	2013	2018	2027	rVB	453580	665914	40.06%	3.833%
32	14.533	2095	2098	2105	rVB2	66956	94838	5.71%	0.546%
33	15.192	2206	2210	2222	rVB	201986	339703	20.44%	1.955%
34	15.557	2267	2272	2282	rVB	305874	494350	29.74%	2.846%
35	16.039	2349	2354	2359	rBV	137552	228534	13.75%	1.315%
36	17.680	2627	2633	2635	rBV3	119868	242825	14.61%	1.398%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051925\
Data File : BF142462.D
Acq On : 19 May 2025 20:23
Operator : RC/JU
Sample : Q1984-13
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-27-050725

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	17.727	2637	2641	2659	rVB3	217999	617746	37.17%	3.556%
38	18.156	2708	2714	2726	rBV2	143167	436243	26.25%	2.511%
39	18.274	2728	2734	2745	rVB4	184650	545302	32.81%	3.139%
40	18.521	2768	2776	2795	rBV6	142131	719604	43.30%	4.142%

Sum of corrected areas: 17372913




Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051925\
Data File : BF142462.D
Acq On : 19 May 2025 20:23
Operator : RC/JU
Sample : Q1984-13
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-27-050725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

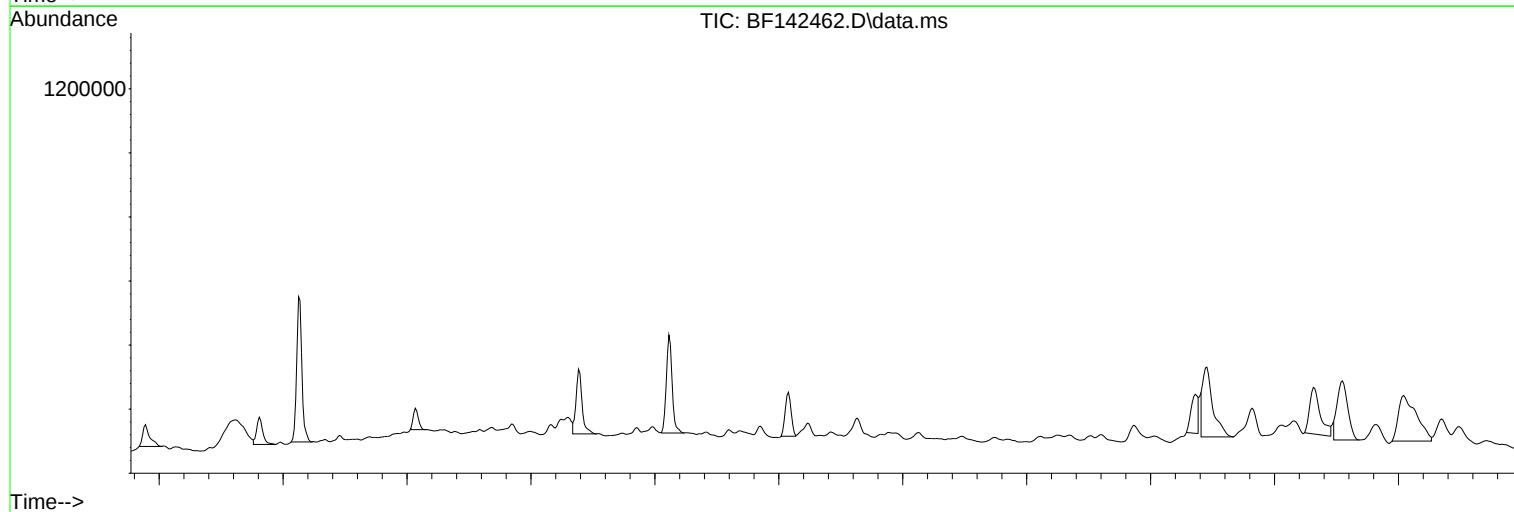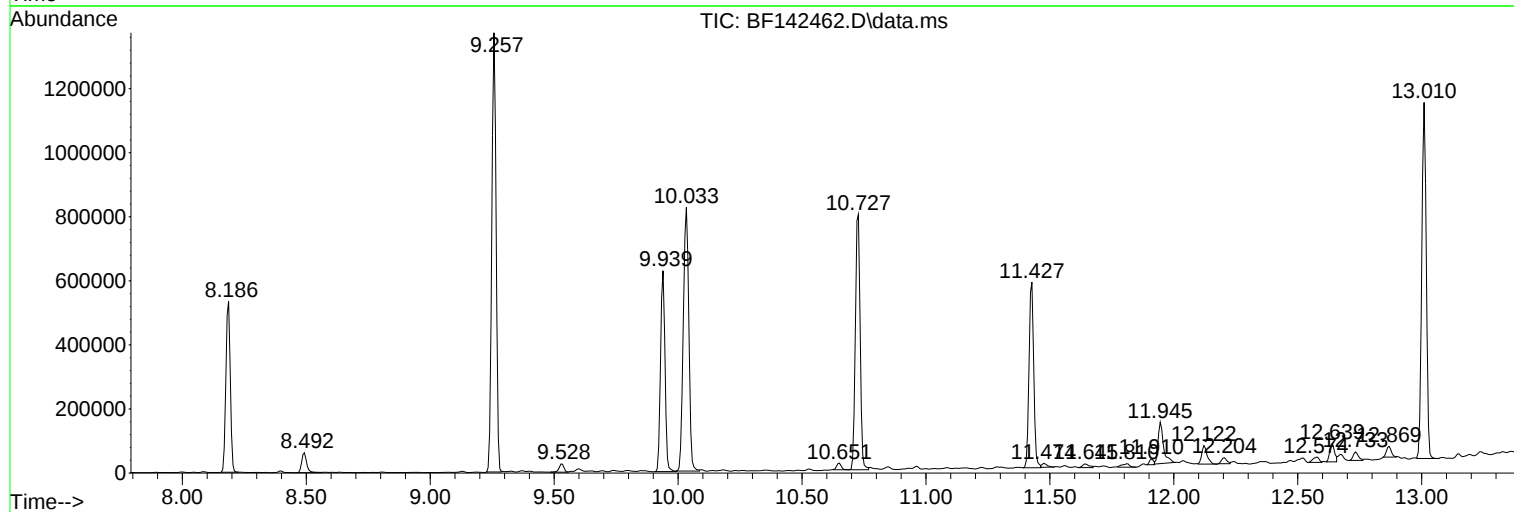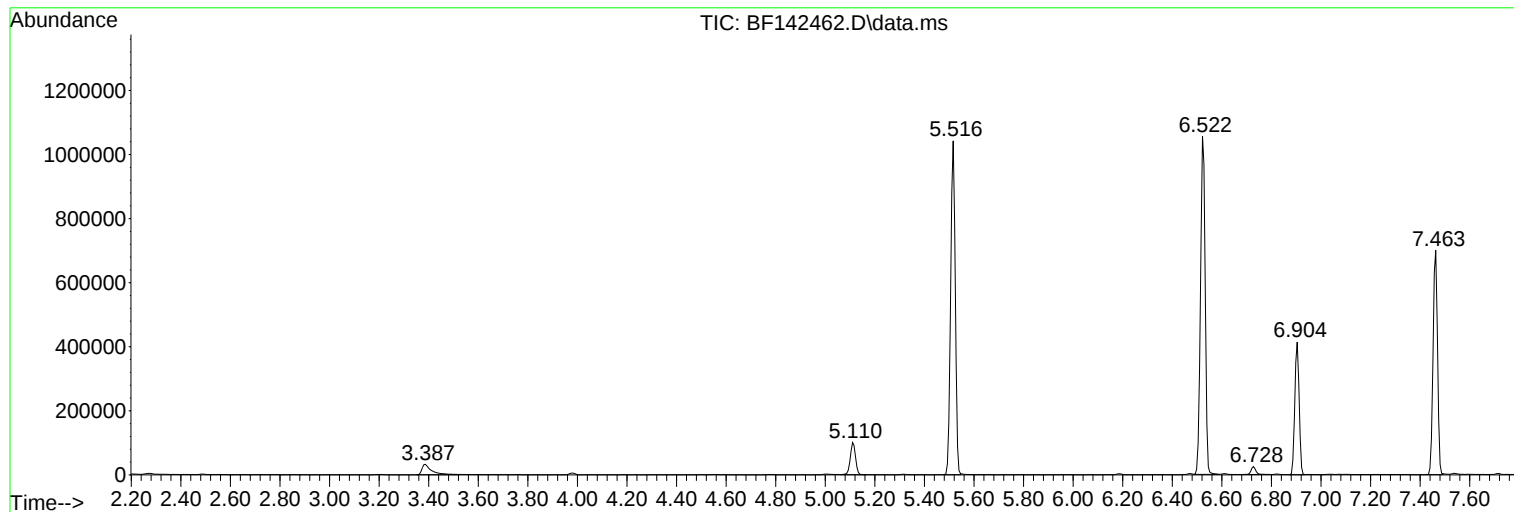

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051925\
Data File : BF142462.D
Acq On : 19 May 2025 20:23
Operator : RC/JU
Sample : Q1984-13
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-27-050725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051925\
Data File : BF142462.D
Acq On : 19 May 2025 20:23
Operator : RC/JU
Sample : Q1984-13
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-27-050725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------