


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051925\
Data File : BF142440.D
Acq On : 19 May 2025 09:40
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon May 05 18:41:44 2025

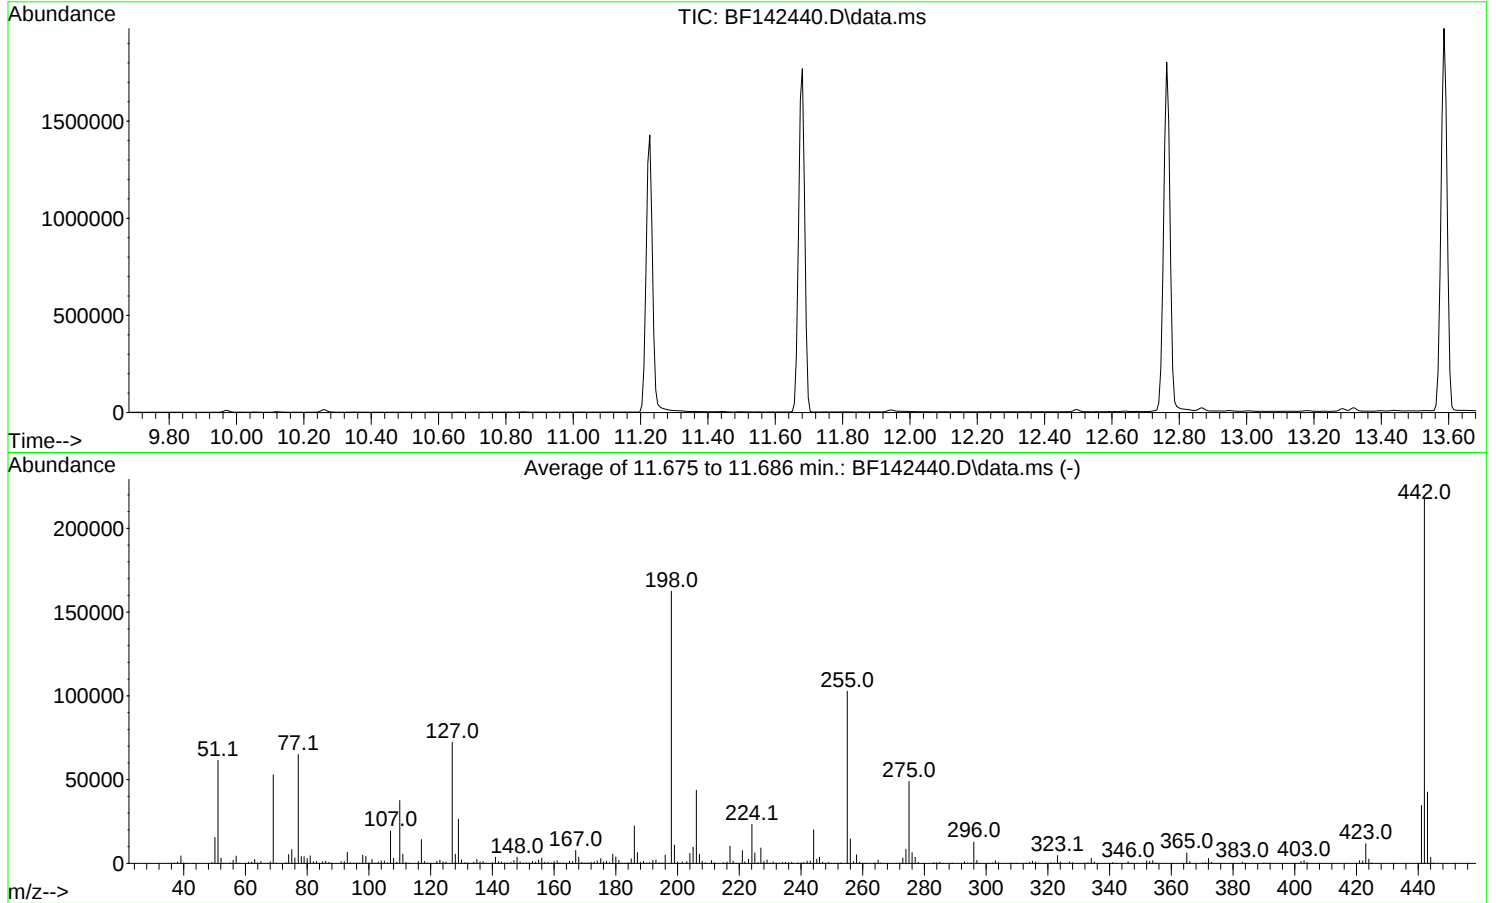

AutoFind: Scans 1612, 1613, 1614; Background Corrected with Scan 1605

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.9	61579	PASS
68	69	0.00	2	1.8	950	PASS
69	198	0.00	100	32.5	52867	PASS
70	69	0.00	2	0.6	296	PASS
127	198	10	80	44.5	72395	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	162520	PASS
199	198	5	9	6.7	10962	PASS
275	198	10	60	30.1	48963	PASS
365	198	1	100	3.8	6225	PASS
441	198	0.01	100	21.3	34565	PASS
442	442	50	100	100.0	218325	PASS
443	442	15	24	19.5	42557	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/19/2025	BNA_F	<u>BF142440.D</u>
Compound Name	Response	Retention Time
DDT	508668	13.586
DDD	8513	13.316
DDE	1079	12.951
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9592	518260	1.85

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051925\
Data File : BF142440.D
Acq On : 19 May 2025 09:40
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 19 11:53:17 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 05 18:41:44 2025
Response via : Initial Calibration

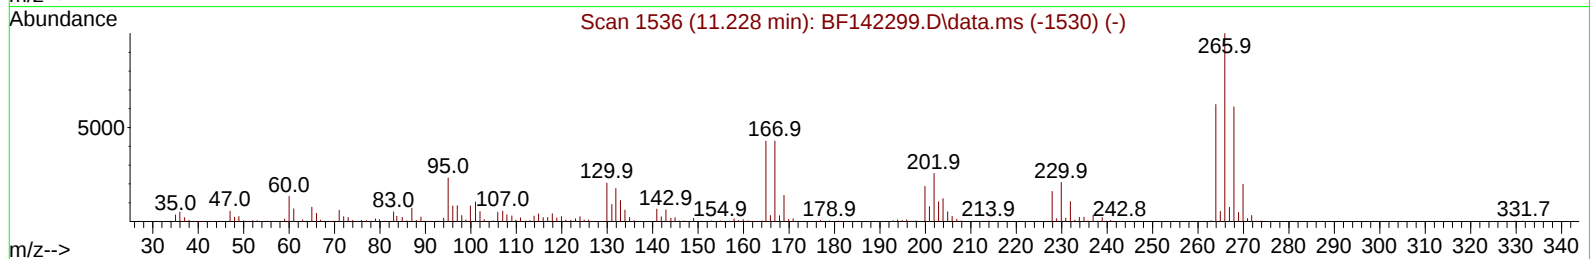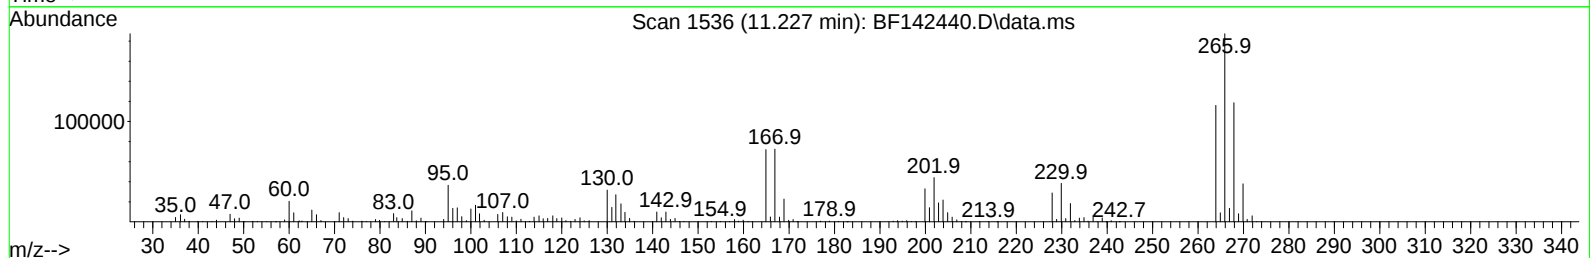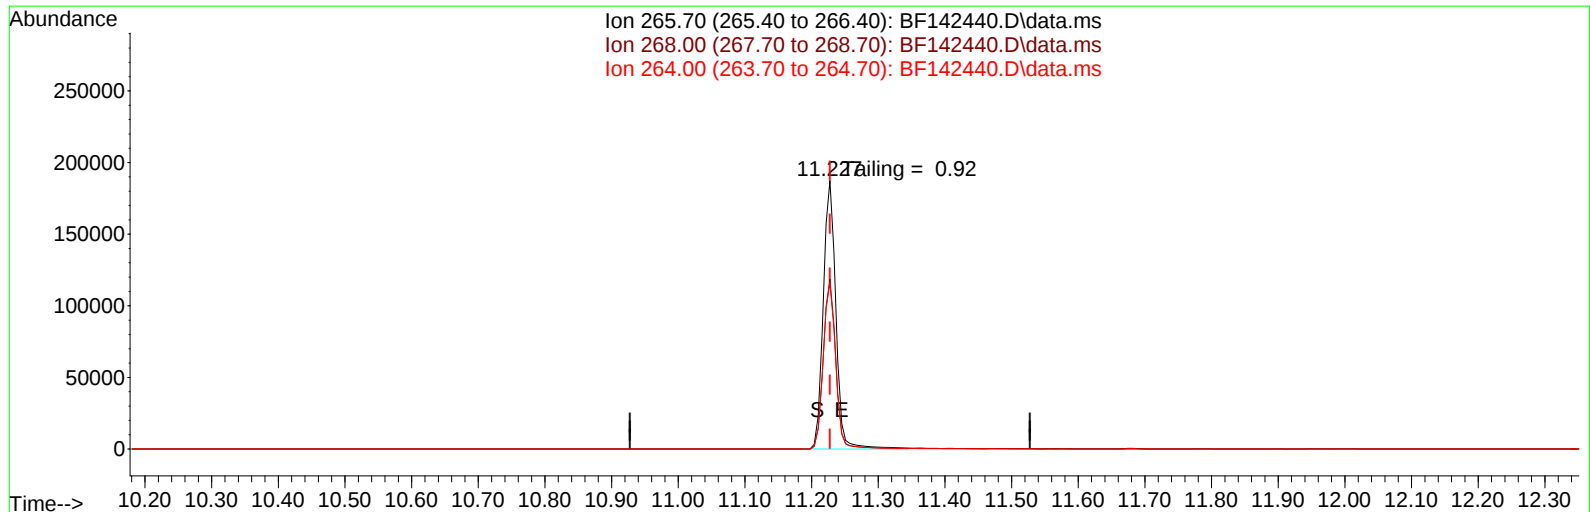

TIC: BF142440.D\data.ms

(70) Pentachlorophenol (C)

11.227min (-0.000) 66651.09 ng




response 247406

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	60.90	63.35
264.00	62.20	61.92
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051925\
Data File : BF142440.D
Acq On : 19 May 2025 09:40
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 19 11:53:17 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 05 18:41:44 2025
Response via : Initial Calibration

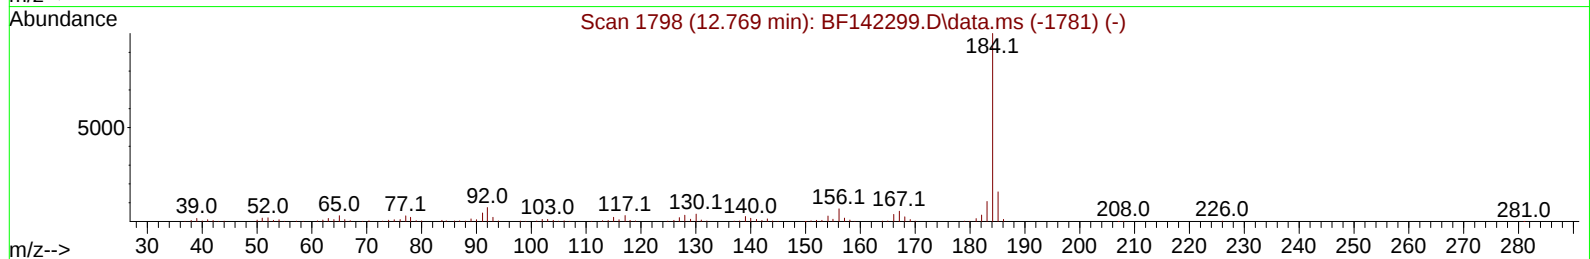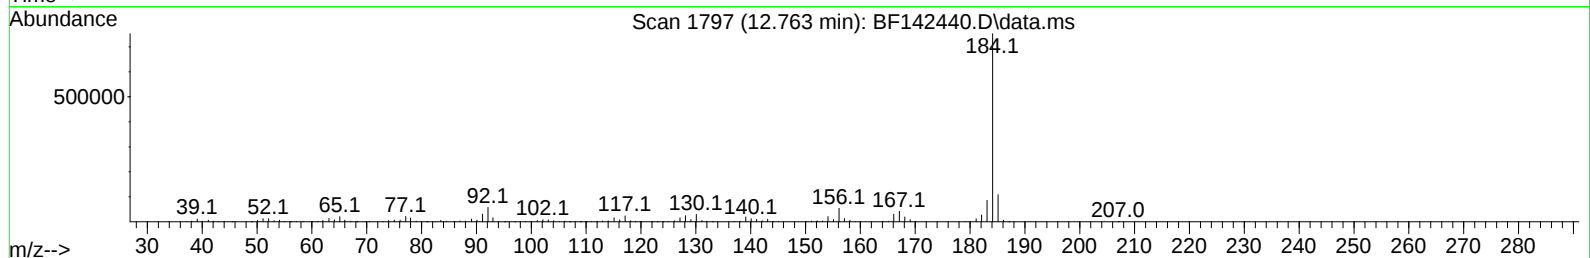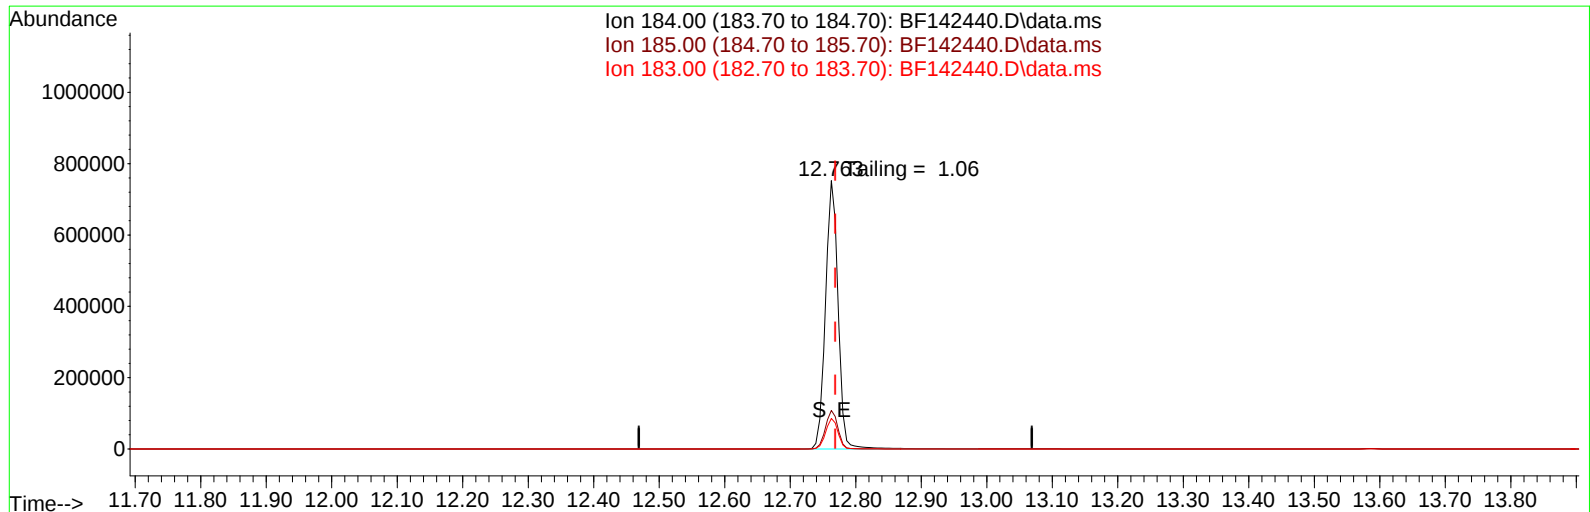

TIC: BF142440.D\data.ms

(77) Benzidine

12.763min (-0.006) 146948.14 ng

response 1009435

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.70	14.41
183.00	10.70	11.41
0.00	0.00	0.00