


Data Path : Z:\HPCHEM1\BNA_F\Data\BF052015\
 Data File : BF079378.D
 Acq On : 20 May 2015 13:59
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 20 05:08:22 2015

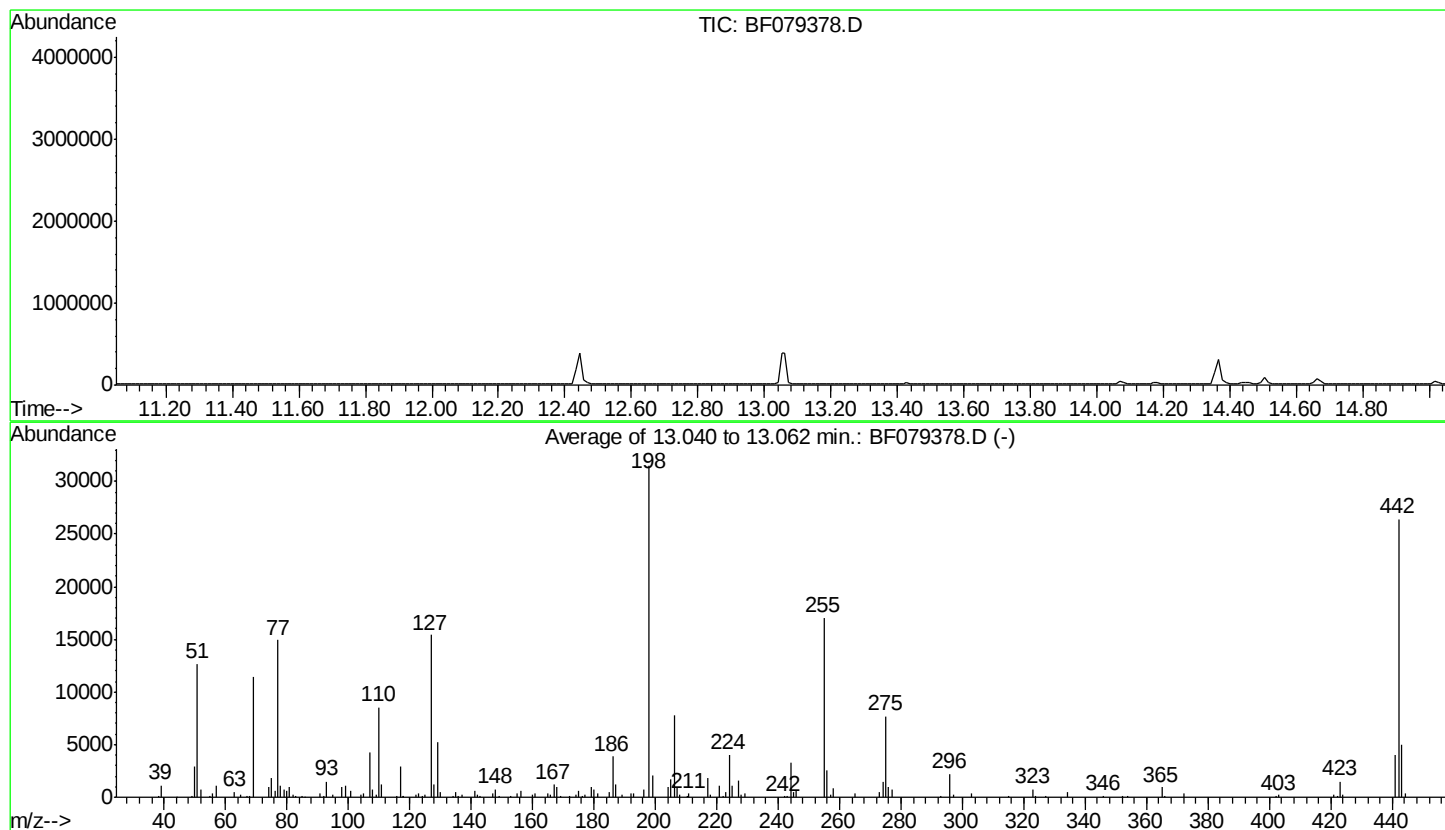

AutoFind: Scans 1037, 1038, 1039; Background Corrected with Scan 1034

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.2	12674	PASS
68	69	0.00	2	1.5	168	PASS
69	198	0.00	100	36.2	11387	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.9	15409	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	31498	PASS
199	198	5	9	6.6	2087	PASS
275	198	10	60	24.4	7671	PASS
365	198	1	100	3.1	968	PASS
441	442	0.01	24	15.2	4011	PASS
442	198	50	100	83.9	26418	PASS
443	442	15	24	19.0	5017	PASS