
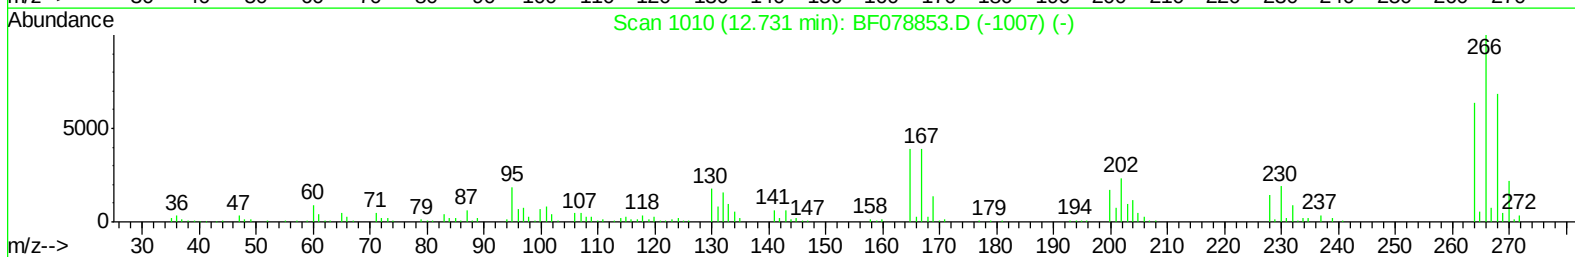
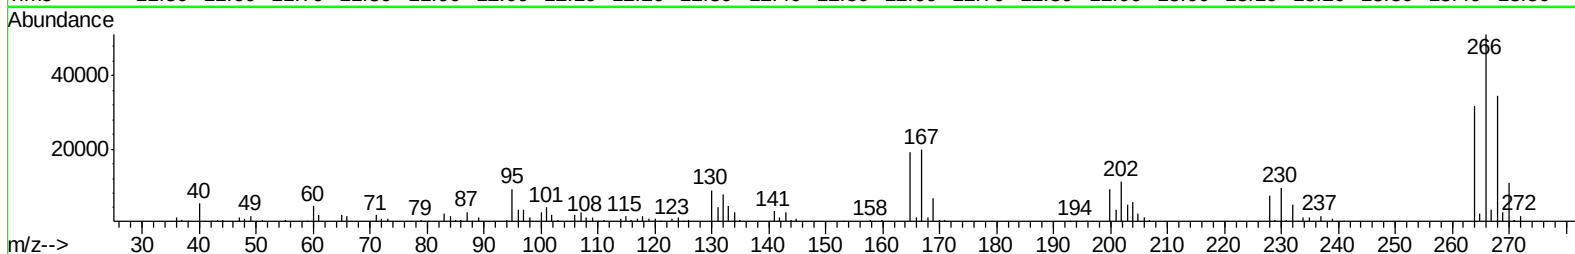


Data Path : Z:\HPCHEM1\BNA F\Data\BF052015\
Data File : BF079378.D
Acq On : 20 May 2015 13:59
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 21 08:36:22 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 20 05:08:22 2015
Response via : Initial Calibration

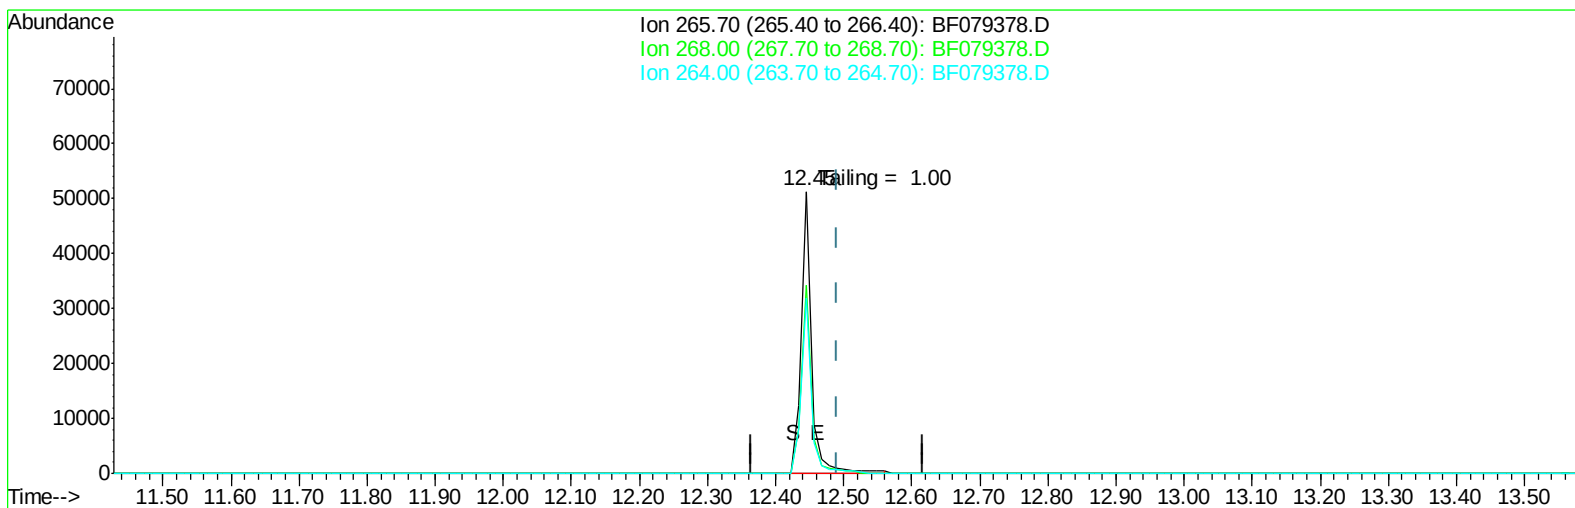

TIC: BF079378.D

(69) Pentachlorophenol (C)

12.445min (-0.046) 7494.91ng

response 55191

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	67.03
264.00	63.60	62.11
0.00	0.00	0.00

