

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052016\
 Data File : BF087243.D
 Acq On : 21 May 2016 00:21
 Operator : UM/SJ
 Sample : H3142-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 RAV-GTMW-3

Quant Time: May 21 00:53:53 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF051716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat May 21 00:19:36 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.56	152	120630	20.00	ng	0.00
21) Naphthalene-d8	7.84	136	533947	20.00	ng	-0.01
38) Acenaphthene-d10	9.59	164	273809	20.00	ng	0.00
63) Phenanthrene-d10	11.06	188	516185	20.00	ng	-0.01
75) Chrysene-d12	13.69	240	411306	20.00	ng	-0.01
86) Perylene-d12	15.04	264	286572	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.14	112	200086	27.88	ng	0.01
7) Phenol-d6	6.23	99	181869	18.89	ng	0.00
23) Nitrobenzene-d5	7.13	82	652771	60.93	ng	-0.01
41) 2,4,6-Tribromophenol	10.38	330	159228	52.62	ng	-0.01
44) 2-Fluorobiphenyl	8.92	172	1265473	76.54	ng	0.00
78) Terphenyl-d14	12.65	244	1219403	67.06	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	1.70	88	150322	40.72	ng	# 22
19) n-Nitroso-di-n-propylamine	7.13	70	90514	12.37	ng	# 72
25) Isophorone	7.13	82	631391	32.19	ng	# 68
49) Dimethylphthalate	9.32	163	91220	4.37	ng	99
50) 2,6-Dinitrotoluene	9.59	165	34684	7.65	ng	# 21
56) 2,4-Dinitrotoluene	9.59	165	34684	5.97	ng	# 16
66) 4-Bromophenyl-phenylether	10.38	248	10722	2.02	ng	# 1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052016\
Data File : BF087243.D
Acq On : 21 May 2016 00:21
Operator : UM/SJ
Sample : H3142-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
RAV-GTMW-3

Quant Time: May 21 00:53:53 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF051716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 21 00:19:36 2016
Response via : Initial Calibration

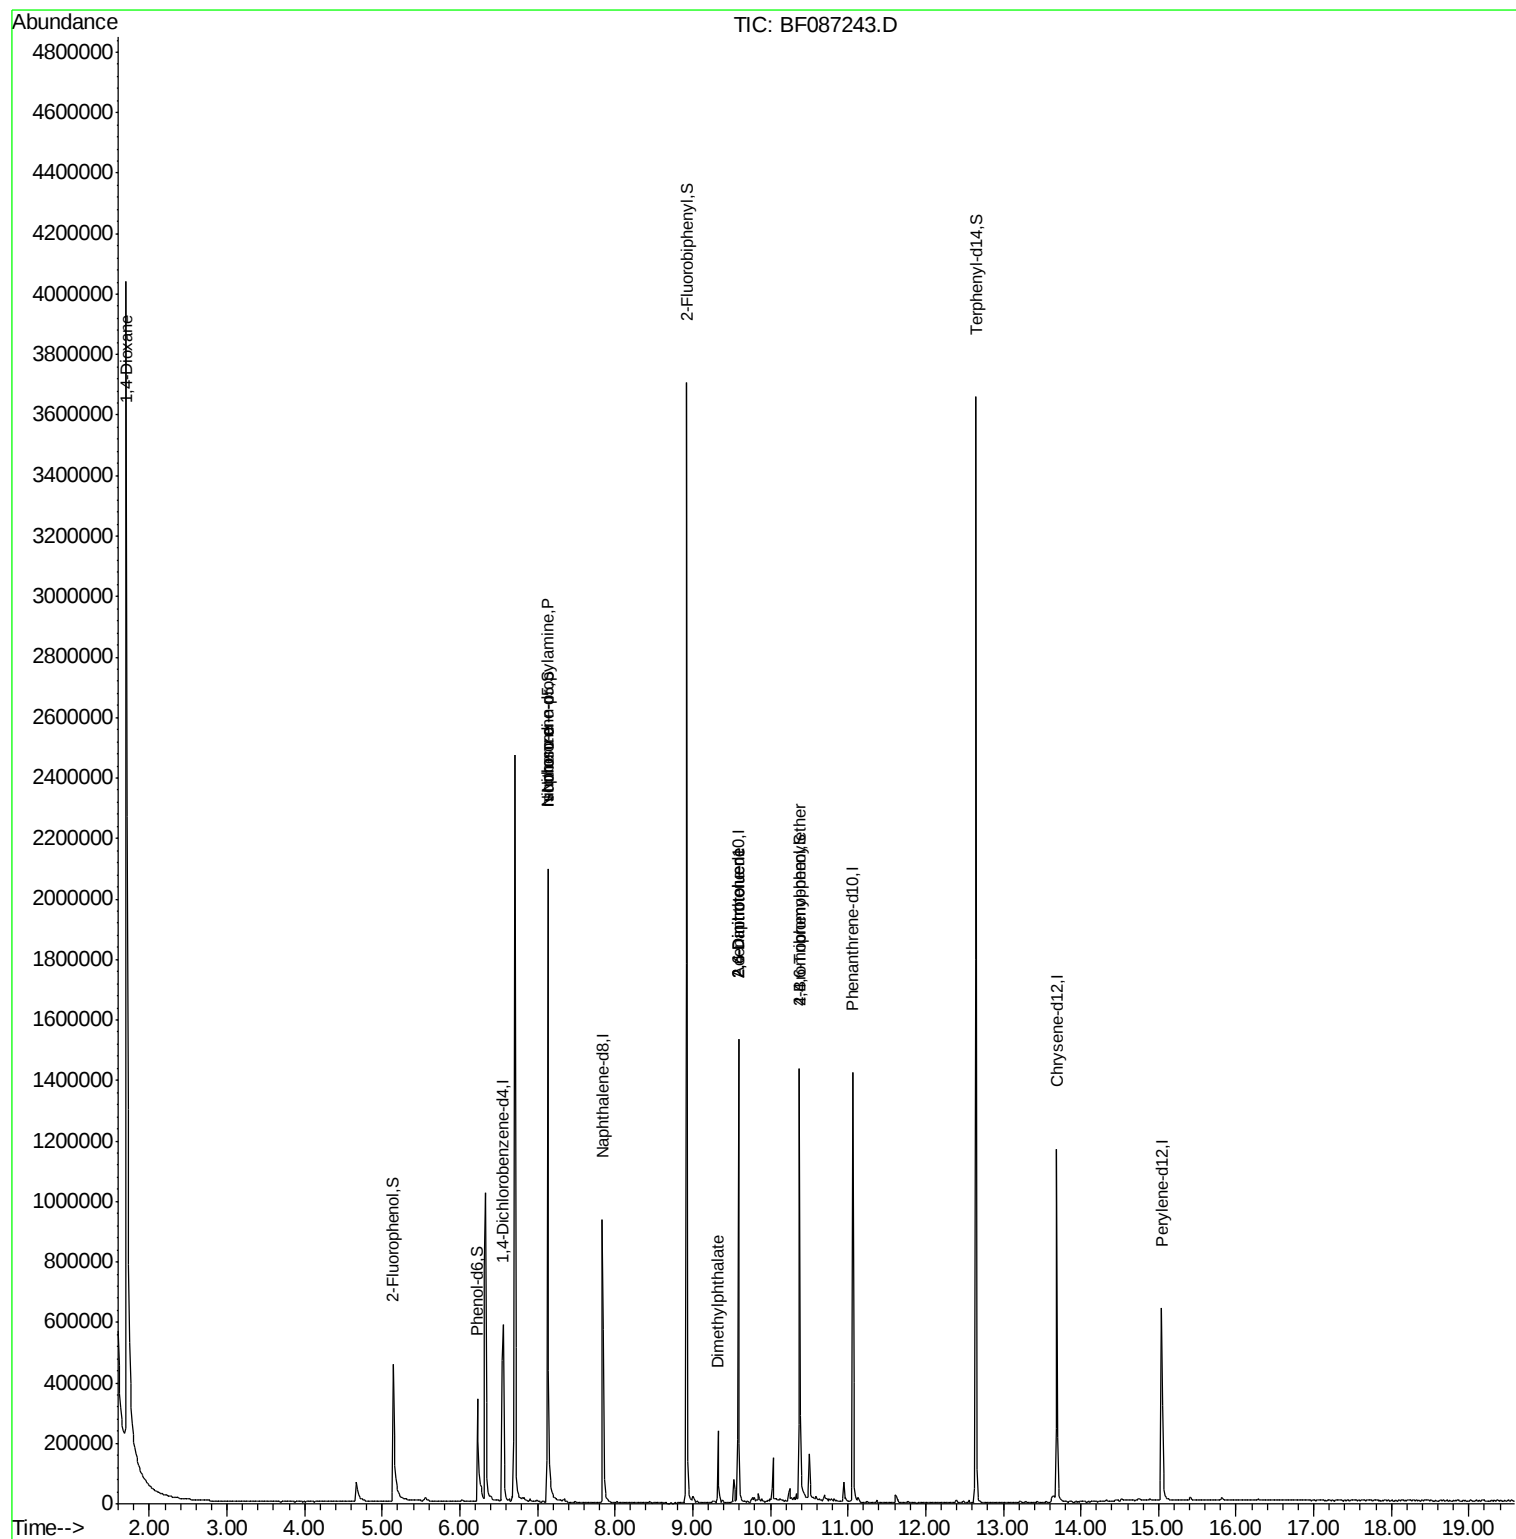



#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.56 min Scan# 435

Delta R.T. -0.00 min

Lab File: BF087243.D

Acq: 21 May 2016 00:21

Instrument :

BNA_F

ClientSampleId :

RAV-GTMW-3


Tgt Ion:152 Resp: 120630

Ion Ratio Lower Upper

152 100

150 157.0 125.8 188.6




115 59.3 51.5 77.3

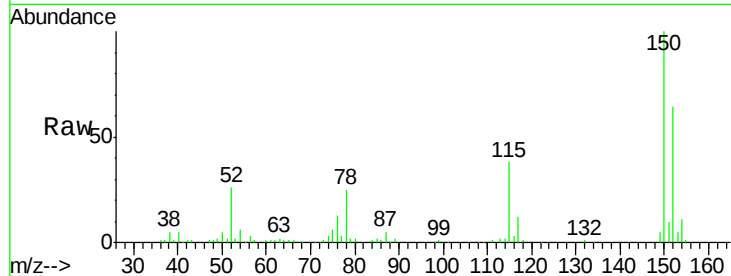

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

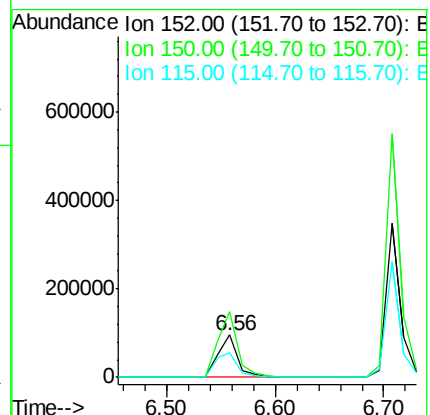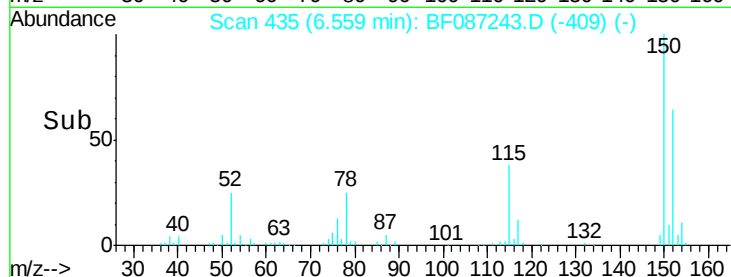

#2

1,4-Dioxane

Concen: 40.72 ng

RT: 1.70 min Scan# 10

Delta R.T. -0.26 min

Lab File: BF087243.D

Acq: 21 May 2016 00:21


Tgt Ion: 88 Resp: 150322

Ion Ratio Lower Upper

88 100

58 0.0 59.6 89.4#



43 0.0 21.8 32.6#




Abundance Ion 88.00 (87.70 to 88.70): BF0

Ion 58.00 (57.70 to 58.70): BF0

Ion 43.00 (42.70 to 43.70): BF0

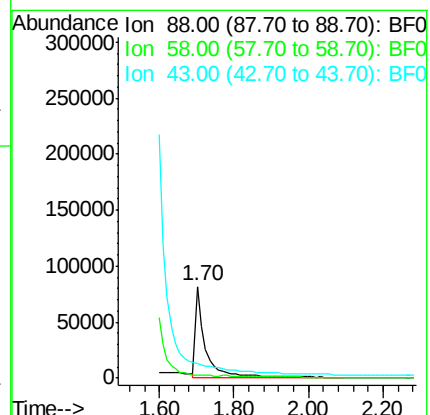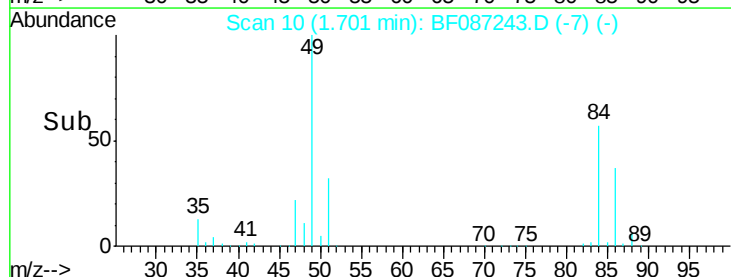

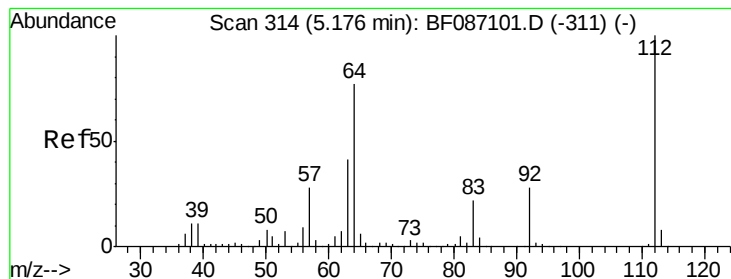

#5

2-Fluorophenol

Concen: 27.88 ng

RT: 5.14 min Scan# 311

Delta R.T. 0.01 min

Lab File: BF087243.D

Acq: 21 May 2016 00:21

Instrument :

BNA_F

ClientSampleId :

RAV-GTMW-3


Tgt Ion: 112 Resp: 200086

Ion Ratio Lower Upper

112 100

64 67.4 52.1 78.1




63 36.1 25.7 38.5



Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

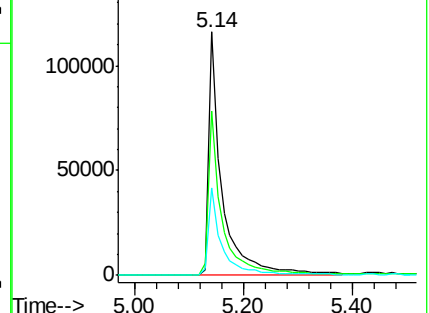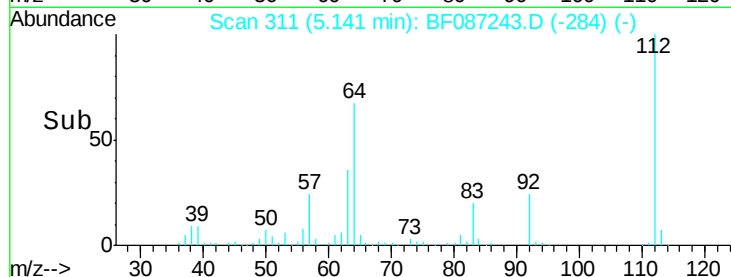

#7

Phenol-d6

Concen: 18.89 ng

RT: 6.23 min Scan# 406

Delta R.T. -0.00 min

Lab File: BF087243.D

Acq: 21 May 2016 00:21


Tgt Ion: 99 Resp: 181869

Ion Ratio Lower Upper

99 100

42 28.5 13.6 20.4#



71 37.1 24.6 36.8#




Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0



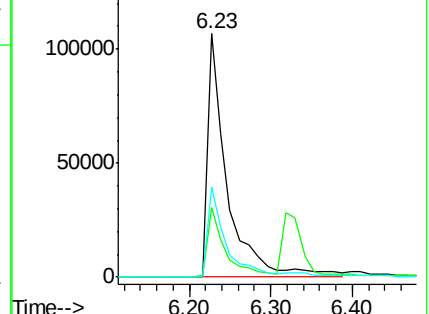
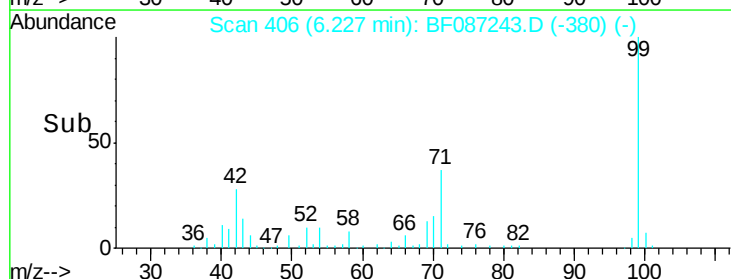


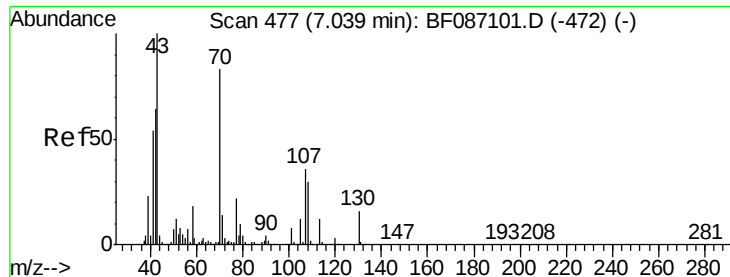

#19
n-Nitroso-di-n-propylamine
Concen: 12.37 ng
RT: 7.13 min Scan# 485
Delta R.T. 0.14 min
Lab File: BF087243.D
Acq: 21 May 2016 00:21




Instrument :
BNA_F
ClientSampleId :
RAV-GTMW-3


Tgt Ion:	70	Resp:	90514
Ion	Ratio	Lower	Upper
70	100		
42	68.6	43.1	64.7#
101	0.0	8.1	12.1#
130	1.9	18.6	28.0#

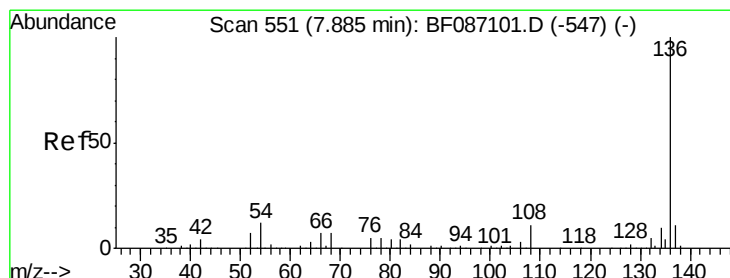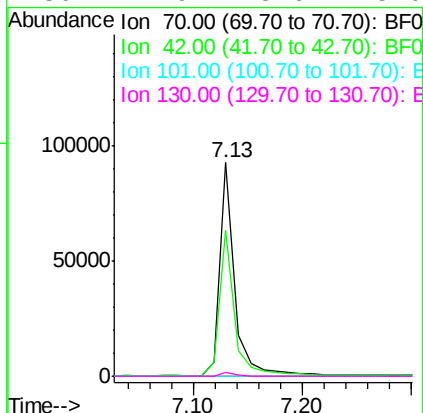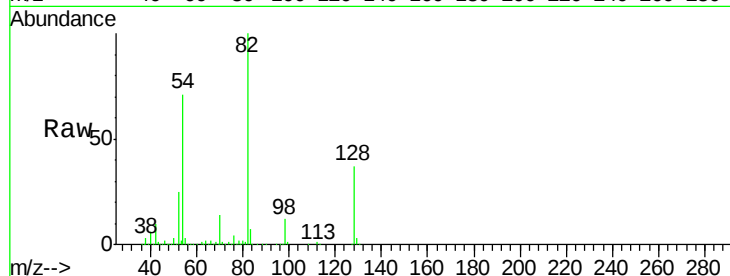

#21
Naphthalene-d8
Concen: 20.00 ng
RT: 7.84 min Scan# 547
Delta R.T. -0.01 min
Lab File: BF087243.D
Acq: 21 May 2016 00:21

Tgt Ion:	136	Resp:	533947
Ion	Ratio	Lower	Upper
136	100		
137	11.3	8.8	13.2
54	15.0	5.0	7.4#
68	7.5	4.4	6.6#



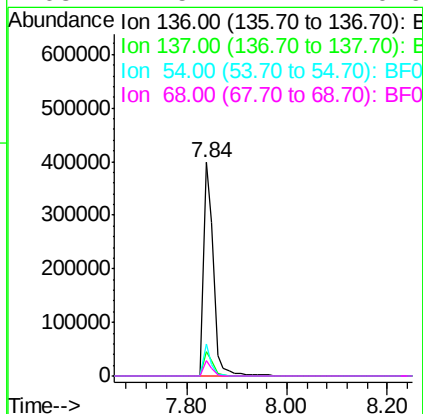
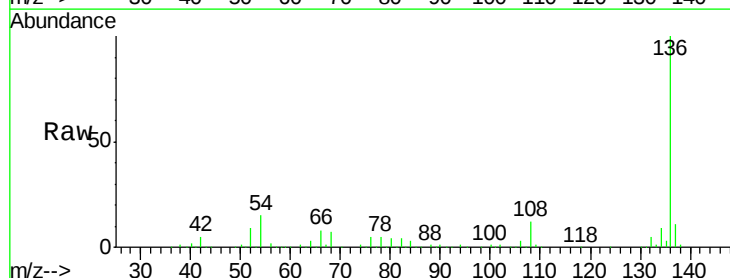


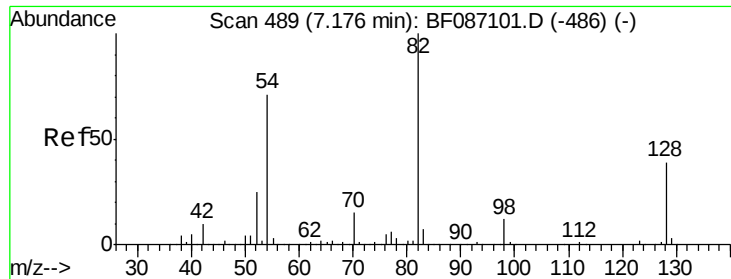

#23
Nitrobenzene-d5
Concen: 60.93 ng
RT: 7.13 min Scan# 485
Delta R.T. -0.01 min
Lab File: BF087243.D
Acq: 21 May 2016 00:21




Instrument :
BNA_F
ClientSampleId :
RAV-GTMW-3


Tgt Ion: 82 Resp: 652771
Ion Ratio Lower Upper
82 100
128 37.3 40.6 61.0#
54 71.2 38.1 57.1#

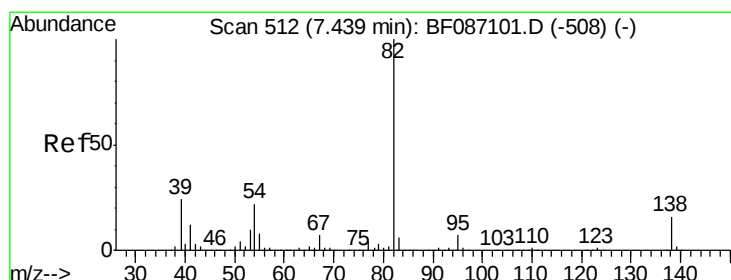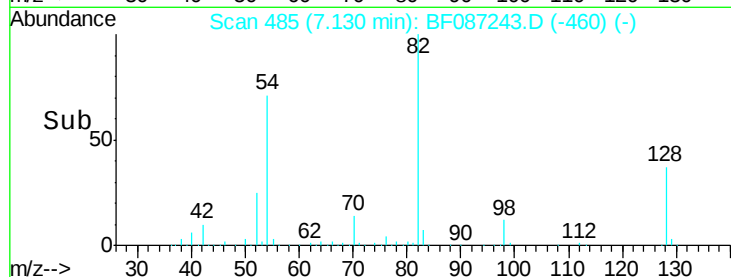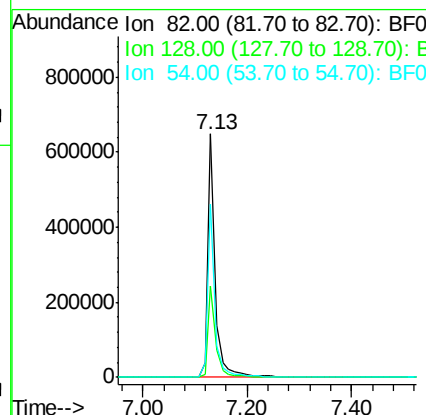

#25
Isophorone
Concen: 32.19 ng
RT: 7.13 min Scan# 485
Delta R.T. -0.27 min
Lab File: BF087243.D
Acq: 21 May 2016 00:21

Tgt Ion: 82 Resp: 631391
Ion Ratio Lower Upper
82 100
95 0.0 5.1 7.7#
138 0.0 12.4 18.6#

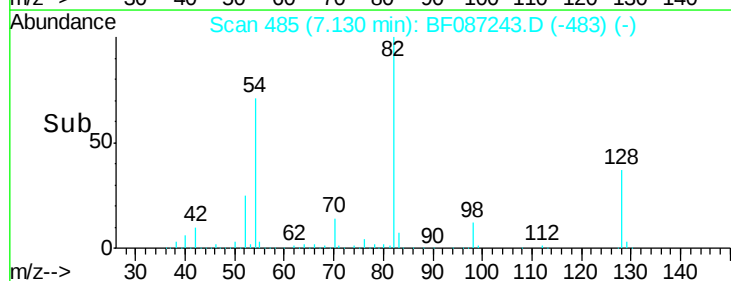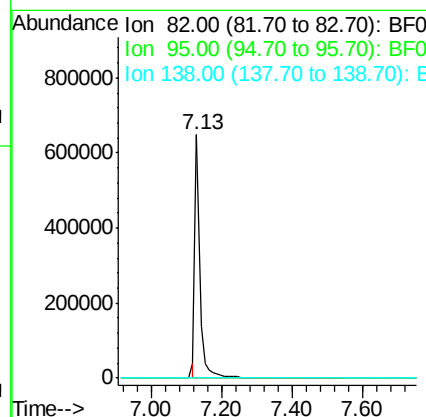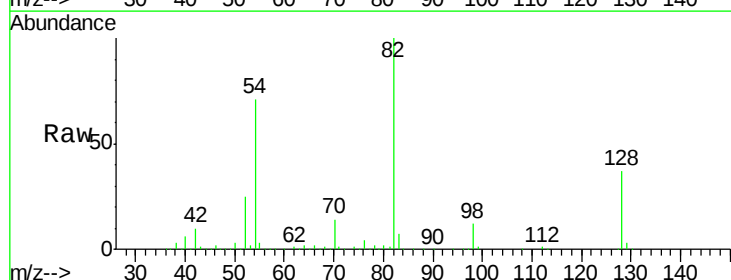

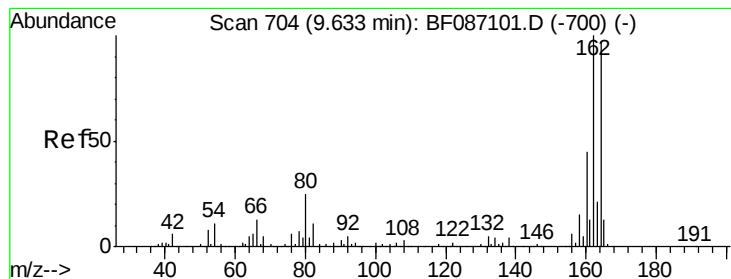

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 9.59 min Scan# 700

Delta R.T. -0.00 min

Lab File: BF087243.D

Acq: 21 May 2016 00:21

Instrument :

BNA_F

ClientSampleId :

RAV-GTMW-3


Tgt Ion:164 Resp: 273809

Ion Ratio Lower Upper

164 100

162 103.7 82.8 124.2




160 47.5 36.9 55.3



Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

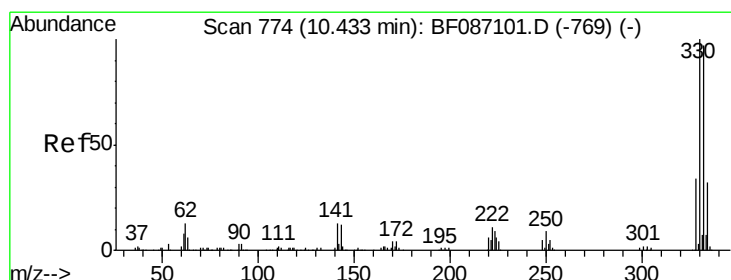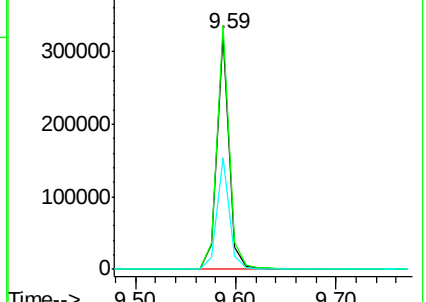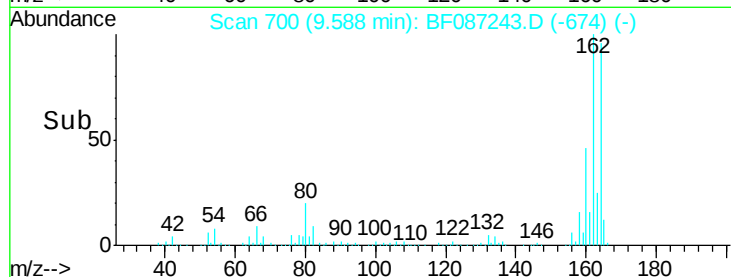

#41

2,4,6-Tribromophenol

Concen: 52.62 ng

RT: 10.38 min Scan# 769

Delta R.T. -0.01 min

Lab File: BF087243.D

Acq: 21 May 2016 00:21


Tgt Ion:330 Resp: 159228

Ion Ratio Lower Upper

330 100

332 97.4 79.0 118.4



141 42.4 31.2 46.8




Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

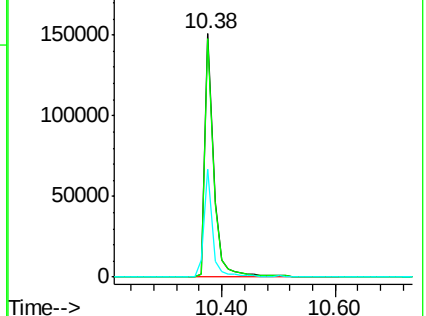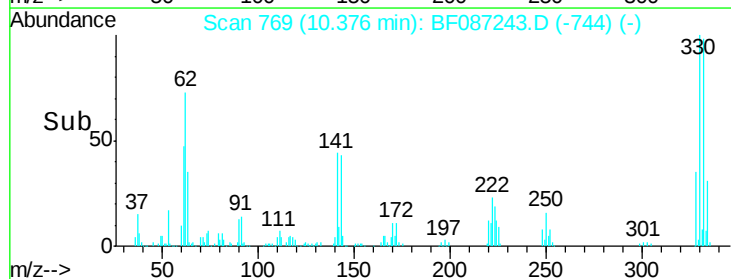



#44

2-Fluorobiphenyl

Concen: 76.54 ng

RT: 8.92 min Scan# 642

Delta R.T. -0.00 min

Lab File: BF087243.D

Acq: 21 May 2016 00:21

Instrument :

BNA_F

ClientSampleId :

RAV-GTMW-3


Tgt Ion:172 Resp: 1265473

Ion Ratio Lower Upper

172 100

171 36.5 29.0 43.6




170 24.3 19.8 29.8

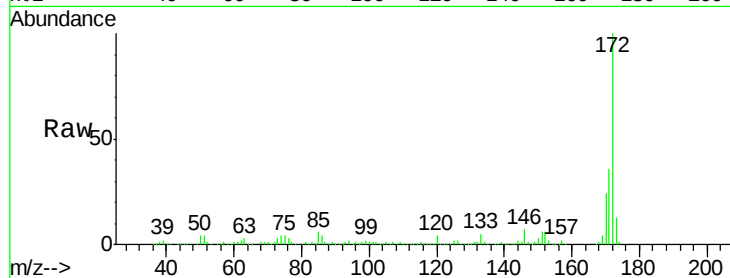

Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

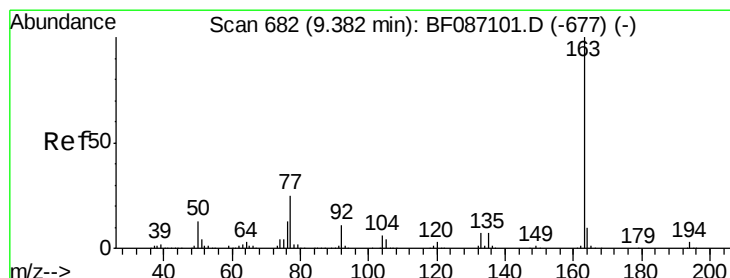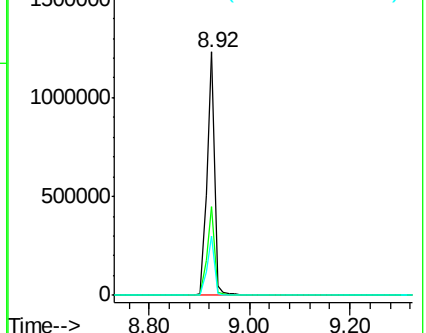

#49

Dimethylphthalate

Concen: 4.37 ng

RT: 9.32 min Scan# 677

Delta R.T. -0.01 min

Lab File: BF087243.D

Acq: 21 May 2016 00:21


Tgt Ion:163 Resp: 91220

Ion Ratio Lower Upper

163 100

194 3.0 2.6 4.0



164 10.0 8.2 12.4

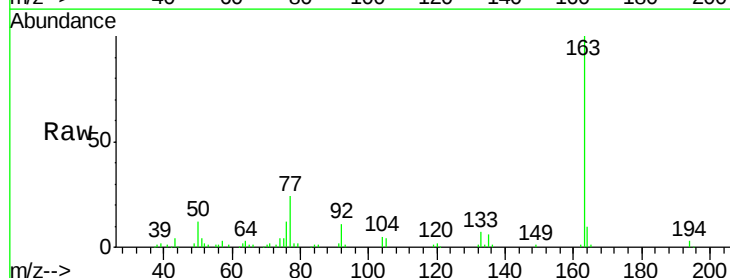


Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

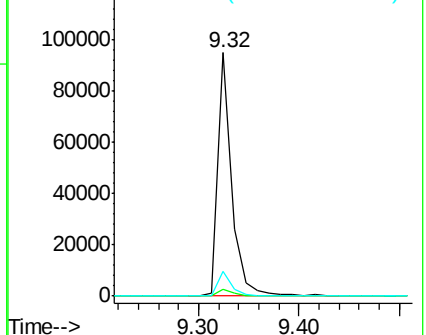

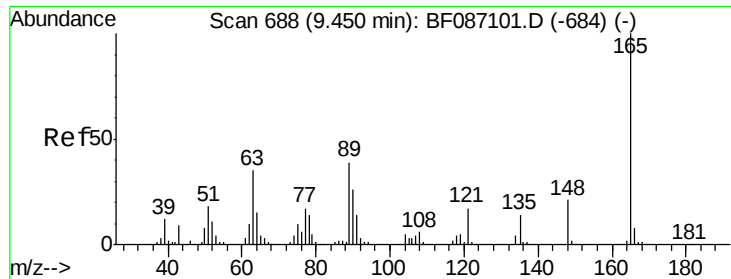

#50

2,6-Dinitrotoluene

Concen: 7.65 ng

RT: 9.59 min Scan# 700

Delta R.T. 0.18 min

Lab File: BF087243.D

Acq: 21 May 2016 00:21

Instrument :

BNA_F

ClientSampleId :

RAV-GTMW-3


Tgt Ion:165 Resp: 34684

Ion Ratio Lower Upper

165 100

63 1.6 51.8 77.8#




89 2.2 50.7 76.1#



Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF0

Ion 89.00 (88.70 to 89.70): BF0

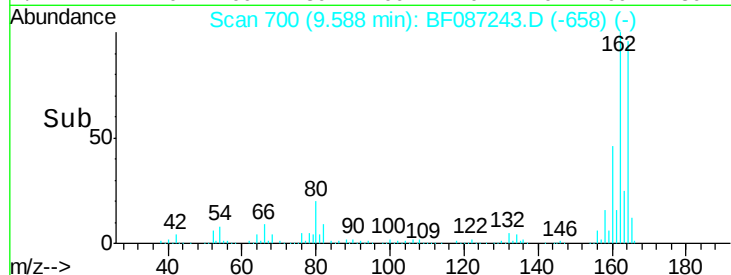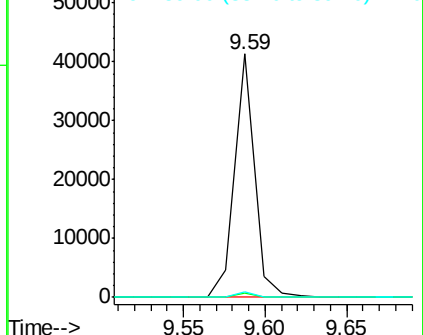

#56

2,4-Dinitrotoluene

Concen: 5.97 ng

RT: 9.59 min Scan# 700

Delta R.T. -0.23 min

Lab File: BF087243.D

Acq: 21 May 2016 00:21

Tgt Ion:165 Resp: 34684


Ion Ratio Lower Upper

165 100

63 1.6 44.3 66.5#

89 2.2 70.0 105.0#

182 0.0 1.8 2.6#






Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF0

Ion 89.00 (88.70 to 89.70): BF0

Ion 182.00 (181.70 to 182.70): E



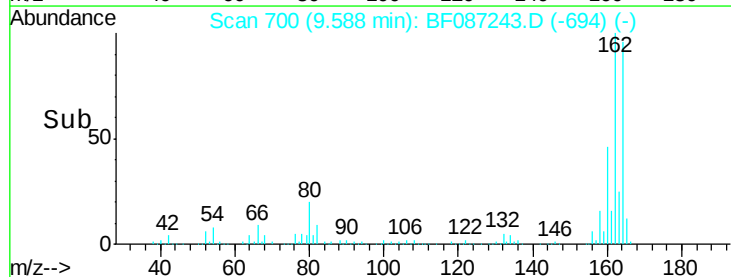
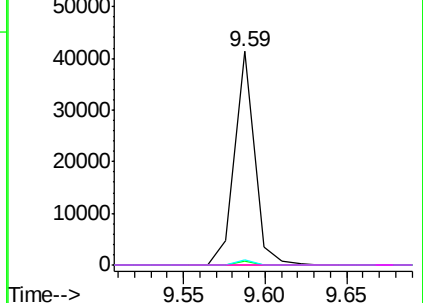


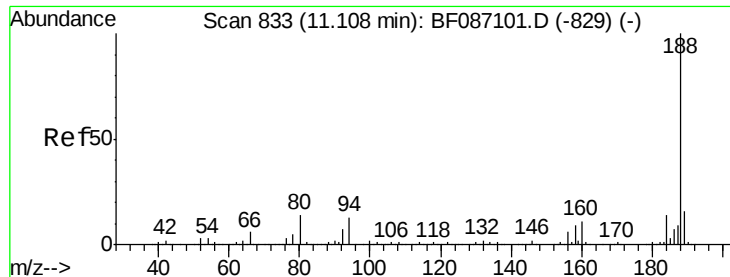

#63
 Phenanthrene-d10
 Concen: 20.00 ng
 RT: 11.06 min Scan# 829
 Delta R.T. -0.01 min
 Lab File: BF087243.D
 Acq: 21 May 2016 00:21




Instrument :
 BNA_F
 ClientSampleId :
 RAV-GTMW-3


Tgt Ion:188 Resp: 516185
 Ion Ratio Lower Upper
 188 100
 94 11.0 6.8 10.2#
 80 12.5 7.1 10.7#

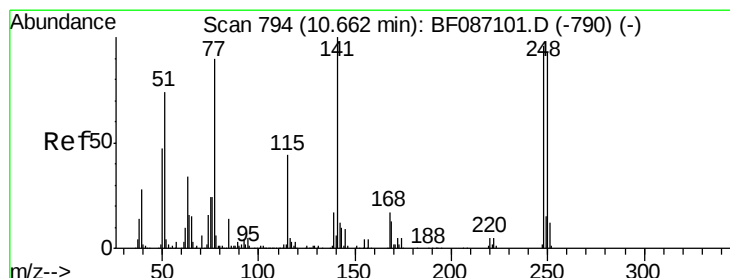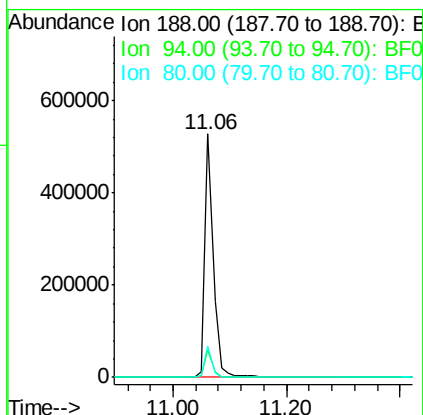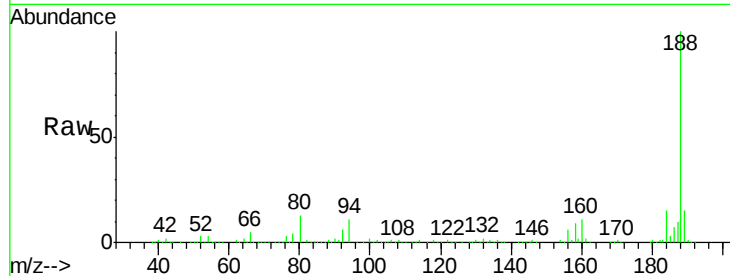

#66
 4-Bromophenyl-phenylether
 Concen: 2.02 ng
 RT: 10.38 min Scan# 769
 Delta R.T. -0.24 min
 Lab File: BF087243.D
 Acq: 21 May 2016 00:21

Tgt Ion:248 Resp: 10722
 Ion Ratio Lower Upper
 248 100
 250 204.9 78.6 117.8#
 141 581.1 76.0 114.0#

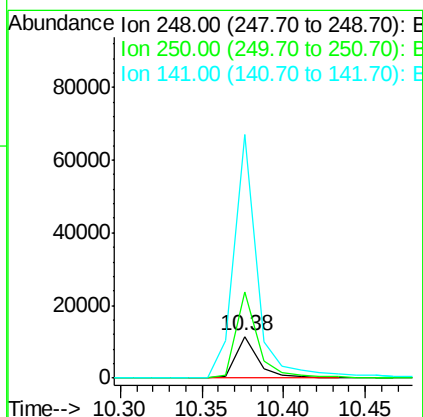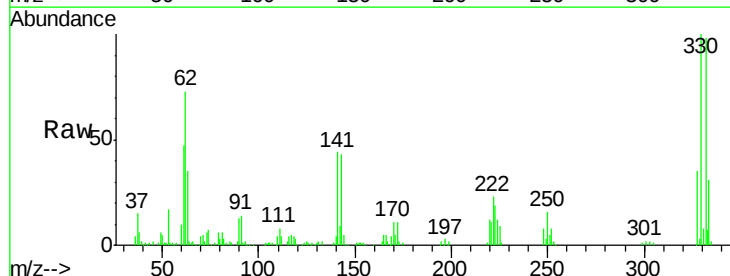

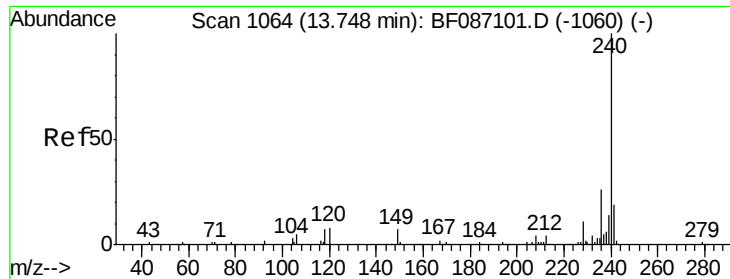

#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.69 min Scan# 1059

Delta R.T. -0.01 min

Lab File: BF087243.D

Acq: 21 May 2016 00:21

Instrument :

BNA_F

ClientSampleId :

RAV-GTMW-3


Tgt Ion:240 Resp: 411306

Ion Ratio Lower Upper

240 100

120 10.6 11.2 16.8#




236 26.3 21.2 31.8

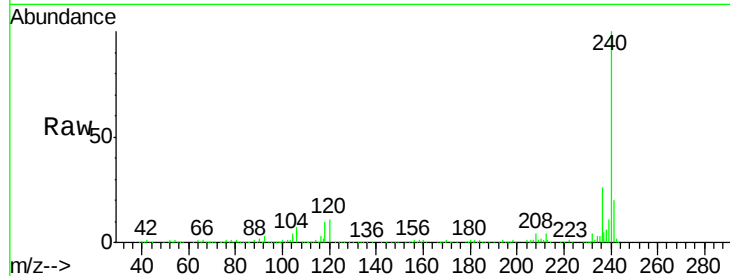

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

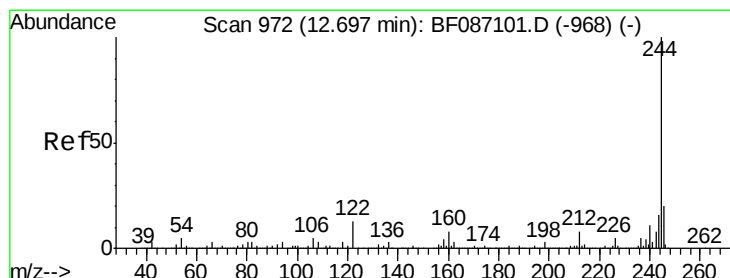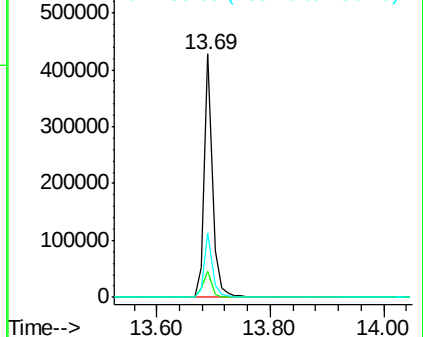

#78

Terphenyl-d14

Concen: 67.06 ng

RT: 12.65 min Scan# 968

Delta R.T. -0.00 min

Lab File: BF087243.D

Acq: 21 May 2016 00:21


Tgt Ion:244 Resp: 1219403

Ion Ratio Lower Upper

244 100

212 7.6 6.2 9.2



122 10.2 12.0 18.0#

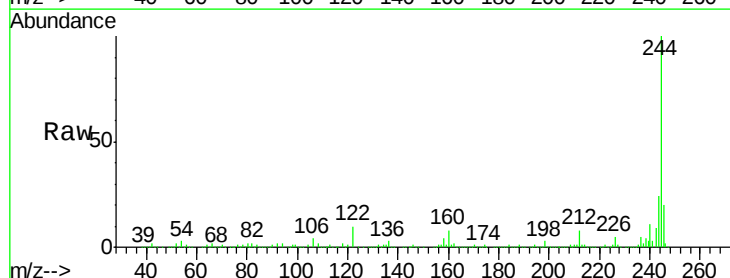


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

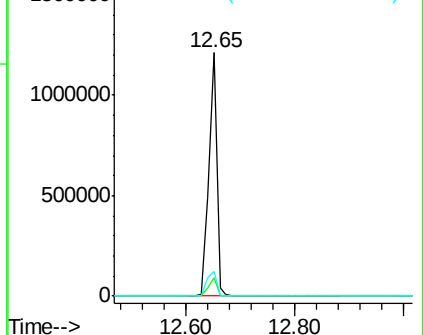

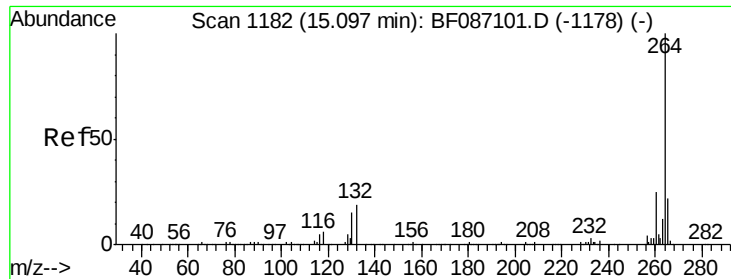

#86
Perylene-d12
Concen: 20.00 ng
RT: 15.04 min Scan# 1177
Delta R.T. -0.00 min
Lab File: BF087243.D
Acq: 21 May 2016 00:21

Instrument :
BNA_F
ClientSampleId :
RAV-GTMW-3

Tgt Ion	Ratio	Lower	Upper
264	100		
260	23.9	19.5	29.3
265	21.4	17.3	25.9

