

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052016\
 Data File : BF087252.D
 Acq On : 21 May 2016 5:13
 Operator : UM/SJ
 Sample : SSTDCCC040
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SSTDCCC040

Quant Time: May 21 05:37:58 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\BFDDTBREAKDOWN.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 01 16:14:27 2010
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	10.30	152	73653	40.00	ng	0.03
2) Naphthalene-d8	11.65	136	1645	40.00	ng	-0.08
3) Acenaphthene-d10	14.71	164	315	40.00	ng	-0.20
4) Phenanthrene-d10	14.99	188	472	40.00	ng	-0.10
8) Chrysene-d12	0.00	240	0	0.00	ng	-30.93
9) Perylene-d12	0.00	264	0	0.00	ng	-34.56
Target Compounds						Qvalue
5) DDE	10.62	246	451	2.04	ng	# 1
6) DDD	10.68	235	1247	N.D.		
7) DDT	10.89	235	1363	N.D.		




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052016\
Data File : BF087252.D
Acq On : 21 May 2016 5:13
Operator : UM/SJ
Sample : SSTDCCC040
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SSTDCCC040

Quant Time: May 21 05:37:58 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\BFDDTBREAKDOWN.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 01 16:14:27 2010
Response via : Initial Calibration

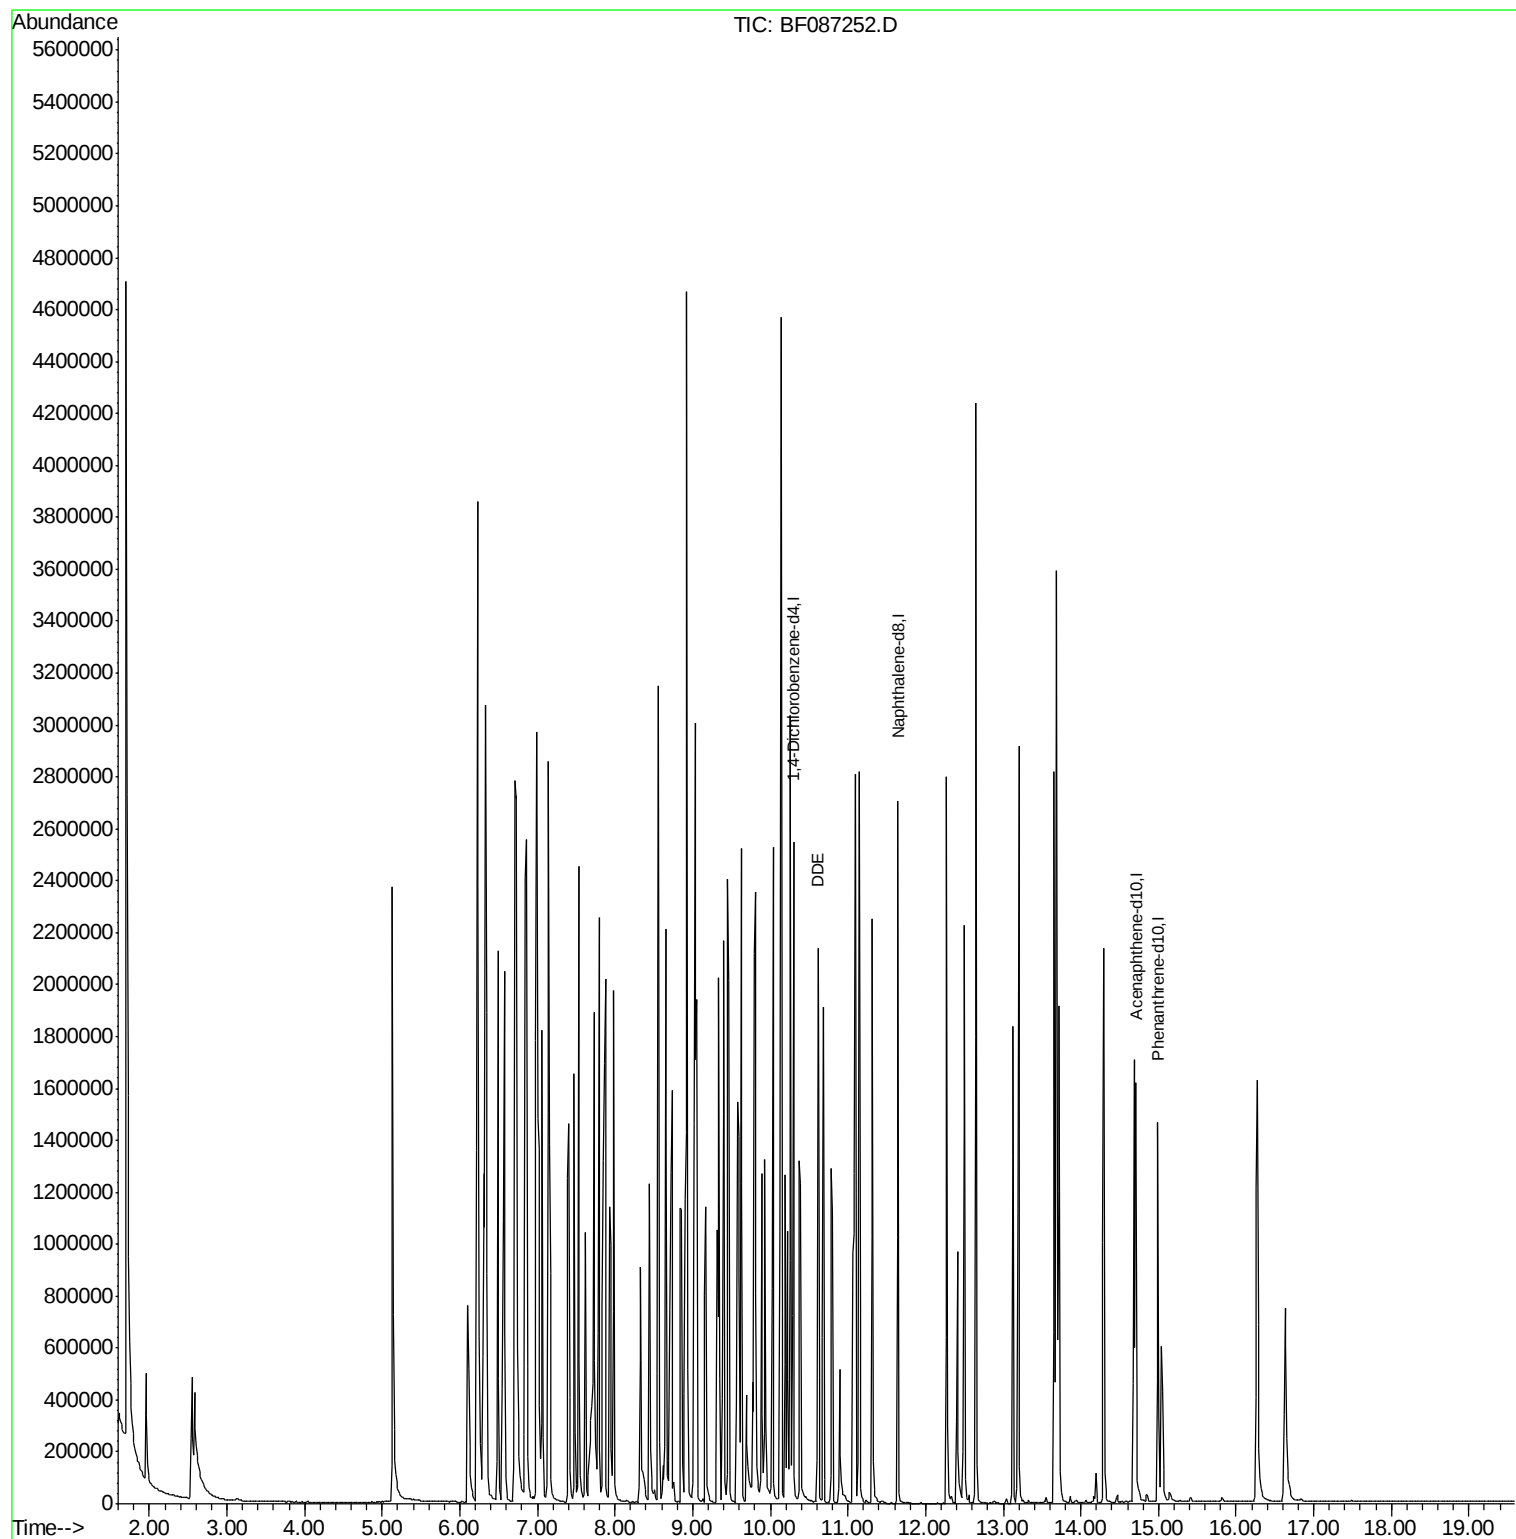

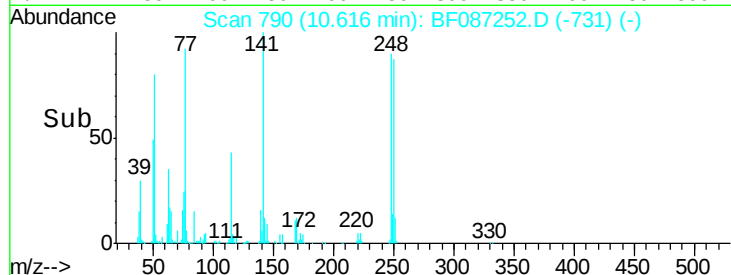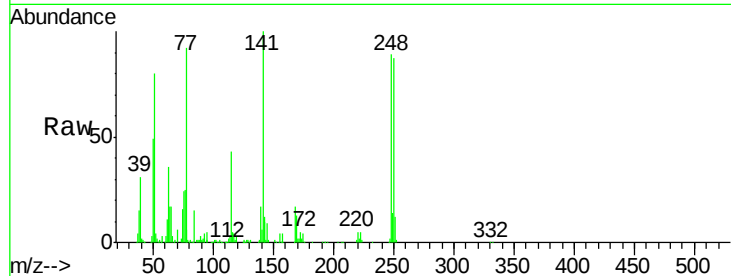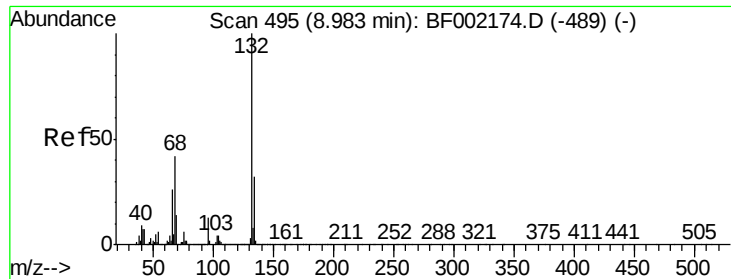

#5

DDE

Concen: 2.04 ng

RT: 10.62 min Scan# 790

Delta R.T. 0.18 min

Lab File: BF087252.D

Acq: 21 May 2016 5:13

Instrument :

BNA_F

ClientSampleId :

SSTDCCC040

Tgt Ion:246 Resp: 451





Ion Ratio Lower Upper

246 100

248 46706.7 1434.9 2152.3#

318 0.0 161.5 242.3#

176 0.0 3844.2 5766.4#

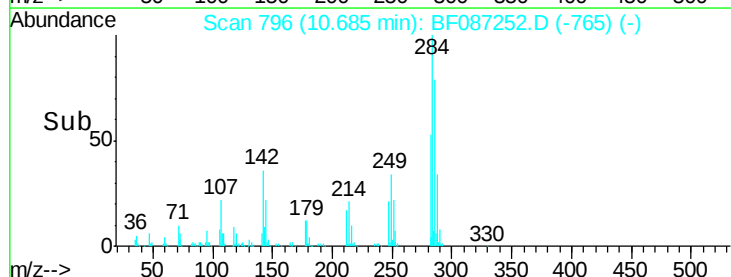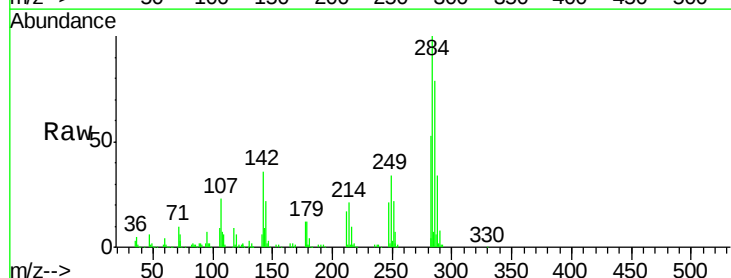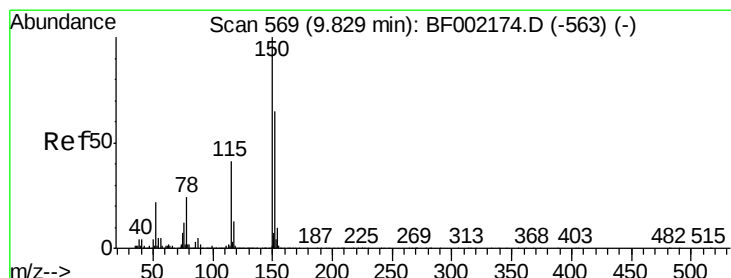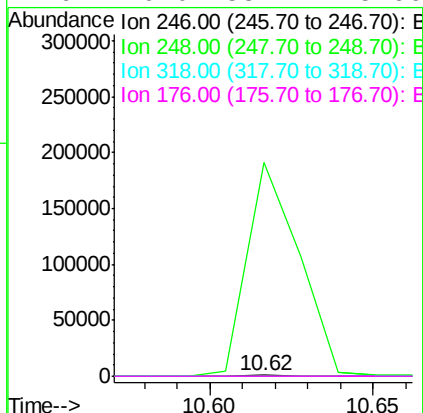

#6

DDD

Concen: Below Cal

RT: 10.68 min Scan# 796

Delta R.T. -0.15 min

Lab File: BF087252.D

Acq: 21 May 2016 5:13


Tgt Ion:235 Resp: 1247


Ion Ratio Lower Upper

235 100

237 145.9 4800.0 7200.0#

165 441.2 4800.0 7200.0#

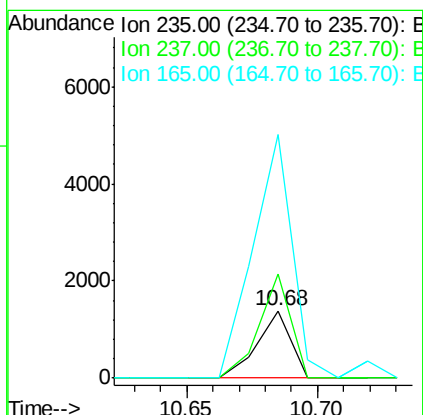

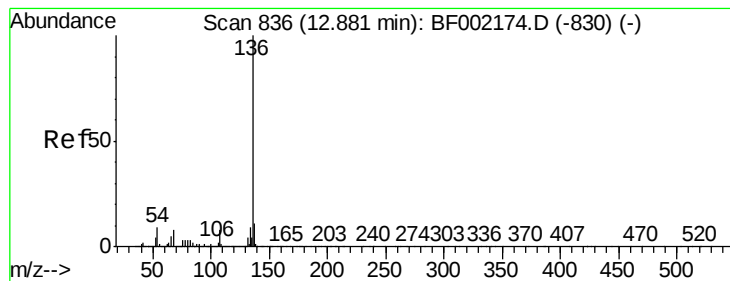

#7

DDT

Concen: Below Cal

RT: 10.89 min Scan# 814

Delta R.T. -0.30 min

Lab File: BF087252.D

Acq: 21 May 2016 5:13

Instrument :

BNA_F

ClientSampleId :

SSTDCCC040



Tgt Ion: 235 Resp: 1363

Ion Ratio Lower Upper

235 100

237 174.4 0.0 0.0#

165 2886.1 0.2 0.2#

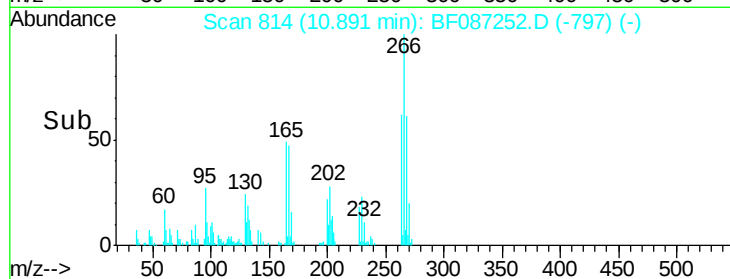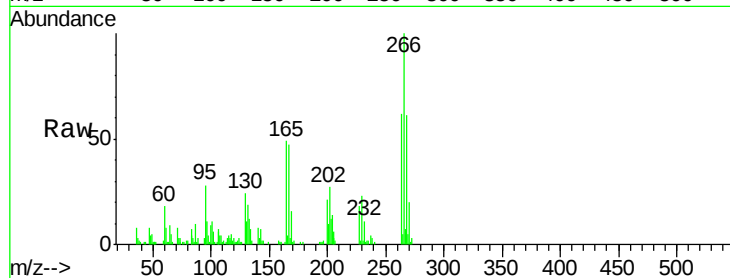

Abundance Ion 235.00 (234.70 to 235.70): E

Ion 237.00 (236.70 to 237.70): E

Ion 165.00 (164.70 to 165.70): E

