


Data Path : Z:\HPCHEM1\BNA F\DATA\BF052016\
 Data File : BF087227.D
 Acq On : 20 May 2016 16:32
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF051716.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon May 23 13:51:43 2016

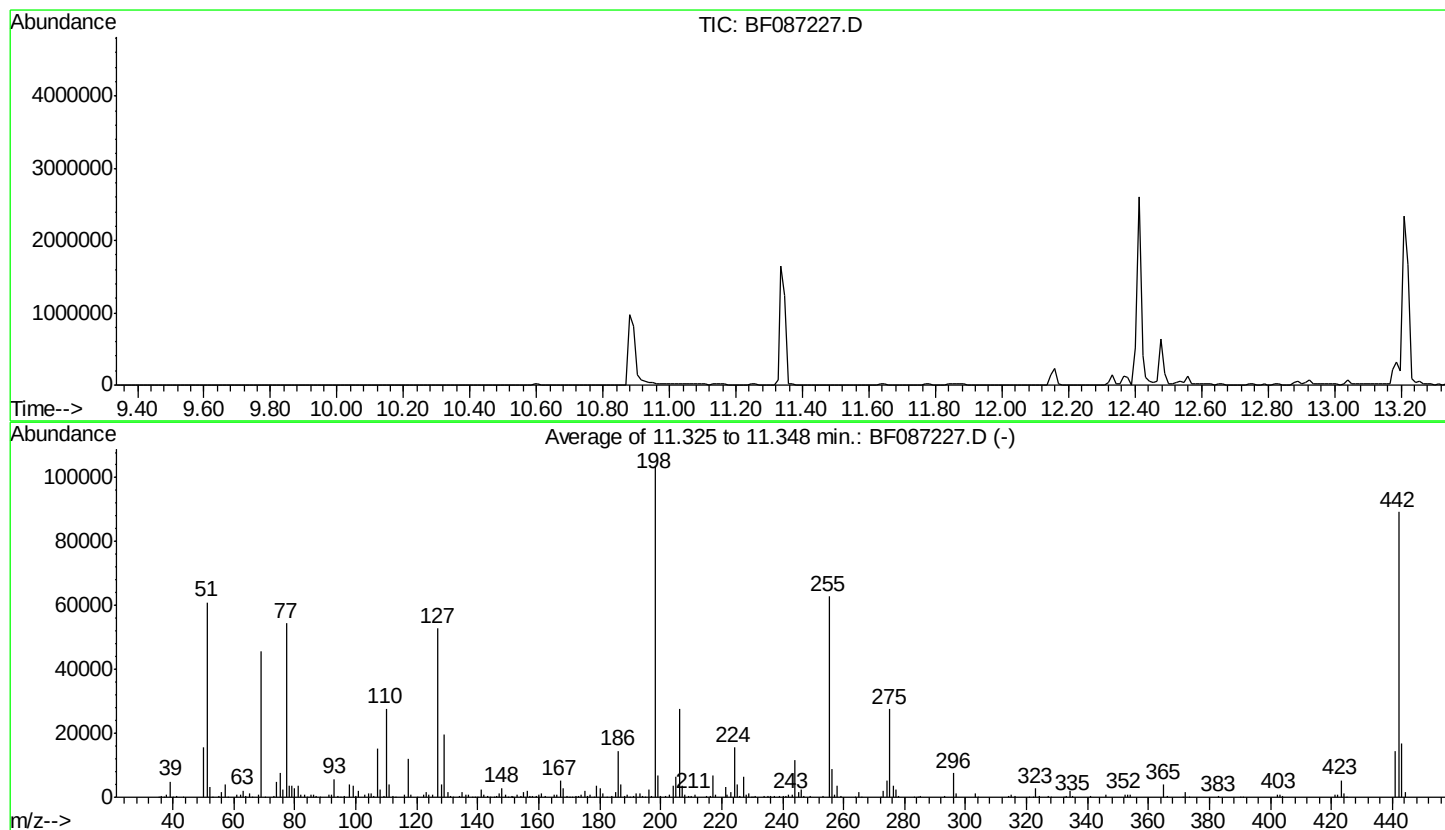

AutoFind: Scans 852, 853, 854; Background Corrected with Scan 849

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	58.8	61056	PASS
68	69	0.00	2	1.9	879	PASS
69	198	0.00	100	44.1	45752	PASS
70	69	0.00	2	0.4	190	PASS
127	198	10	80	50.8	52714	PASS
197	198	0.00	2	0.4	383	PASS
198	198	100	100	100.0	103806	PASS
199	198	5	9	6.5	6781	PASS
275	198	10	60	26.6	27641	PASS
365	198	1	100	3.7	3858	PASS
441	442	0.01	24	16.1	14337	PASS
442	198	50	100	85.9	89187	PASS
443	442	15	24	18.7	16686	PASS