


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052016\
 Data File : BF087251.D
 Acq On : 21 May 2016 4:44
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF051716.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon May 23 13:51:43 2016

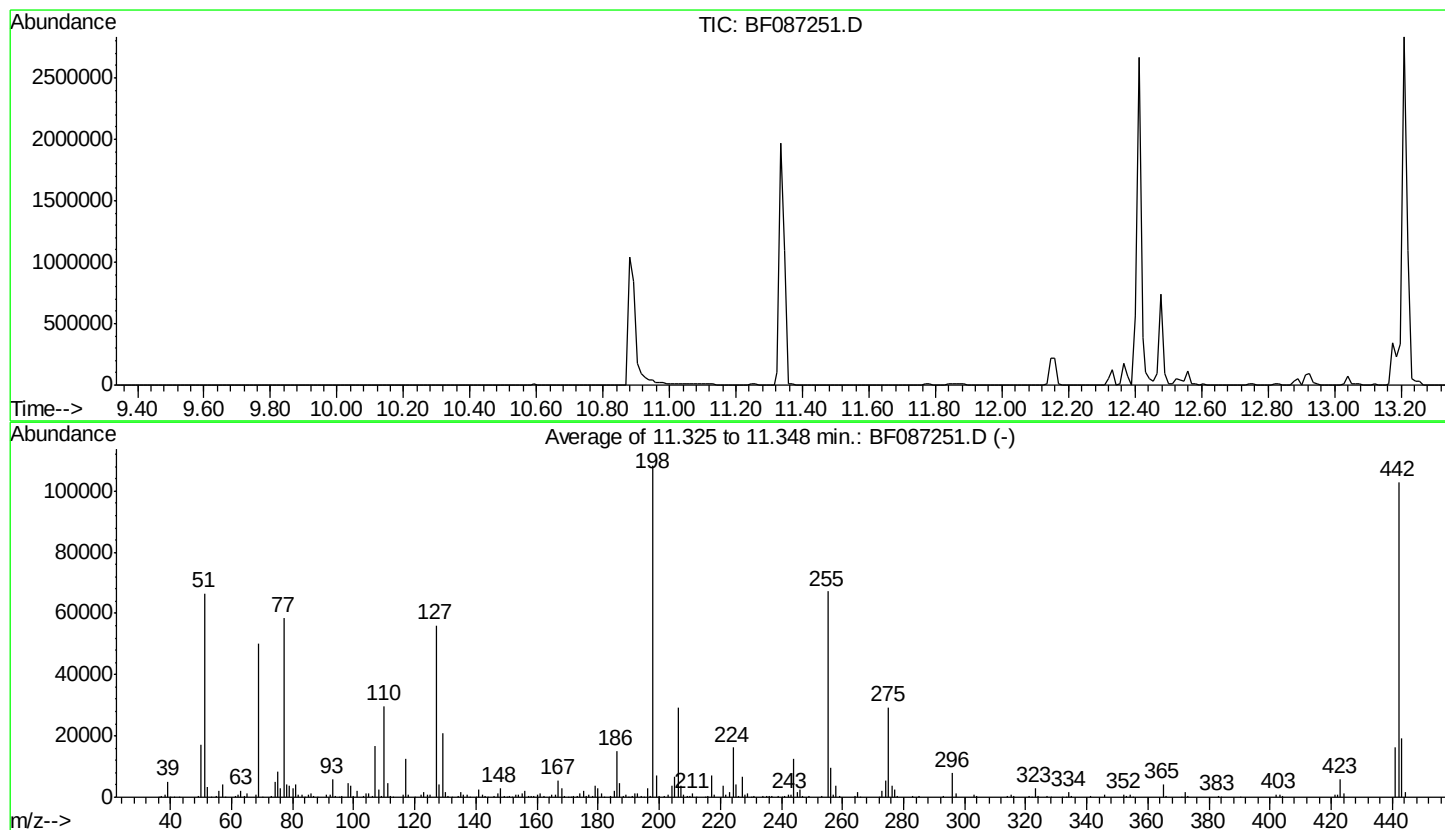

AutoFind: Scans 852, 853, 854; Background Corrected with Scan 849

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	61.4	66497	PASS
68	69	0.00	2	1.8	924	PASS
69	198	0.00	100	46.3	50106	PASS
70	69	0.00	2	0.4	207	PASS
127	198	10	80	51.8	56131	PASS
197	198	0.00	2	0.2	257	PASS
198	198	100	100	100.0	108285	PASS
199	198	5	9	6.6	7098	PASS
275	198	10	60	27.1	29337	PASS
365	198	1	100	3.9	4194	PASS
441	442	0.01	24	15.8	16295	PASS
442	198	50	100	95.0	102874	PASS
443	442	15	24	18.6	19092	PASS