

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF052020\
 Data File : BF120369.D
 Acq On : 20 May 2020 14:37
 Operator : MA/SJ
 Sample : PB129015BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB129015BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051420.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.198	525	529	547	rBV	6046574	7132393	85.93%	11.930%
2	6.251	703	708	738	rBV	5656480	7635138	91.99%	12.771%
3	6.592	762	766	787	rBV	1344954	1732846	20.88%	2.899%
4	6.745	787	792	828	rVB	4910862	5812923	70.03%	9.723%
5	7.163	857	863	887	rBV	3677766	4784541	57.64%	8.003%
6	7.875	979	984	1007	rBV	2083741	2384178	28.72%	3.988%
7	8.957	1162	1168	1183	rBV	6776775	8300048	100.00%	13.883%
8	9.627	1276	1282	1306	rBV	2437589	2567998	30.94%	4.295%
9	10.422	1411	1417	1434	rBV	4168271	5003818	60.29%	8.370%
10	11.110	1529	1534	1557	rBV	2443226	2602516	31.36%	4.353%
11	12.710	1798	1806	1809	rBV	6547089	7491600	90.26%	12.531%
12	13.751	1979	1983	1995	rBV	2021317	2008755	24.20%	3.360%
13	14.527	2110	2115	2119	rBV	93861	98627	1.19%	0.165%
14	14.827	2161	2166	2171	rBV	128547	144613	1.74%	0.242%
15	15.139	2213	2219	2223	rBV	1393222	1816470	21.89%	3.038%
16	15.551	2283	2289	2296	rVB	114607	161667	1.95%	0.270%
17	15.992	2358	2364	2369	rVB2	61147	105635	1.27%	0.177%


Sum of corrected areas: 59783766

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF052020\
Data File : BF120369.D
Acq On : 20 May 2020 14:37
Operator : MA/SJ
Sample : PB129015BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB129015BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

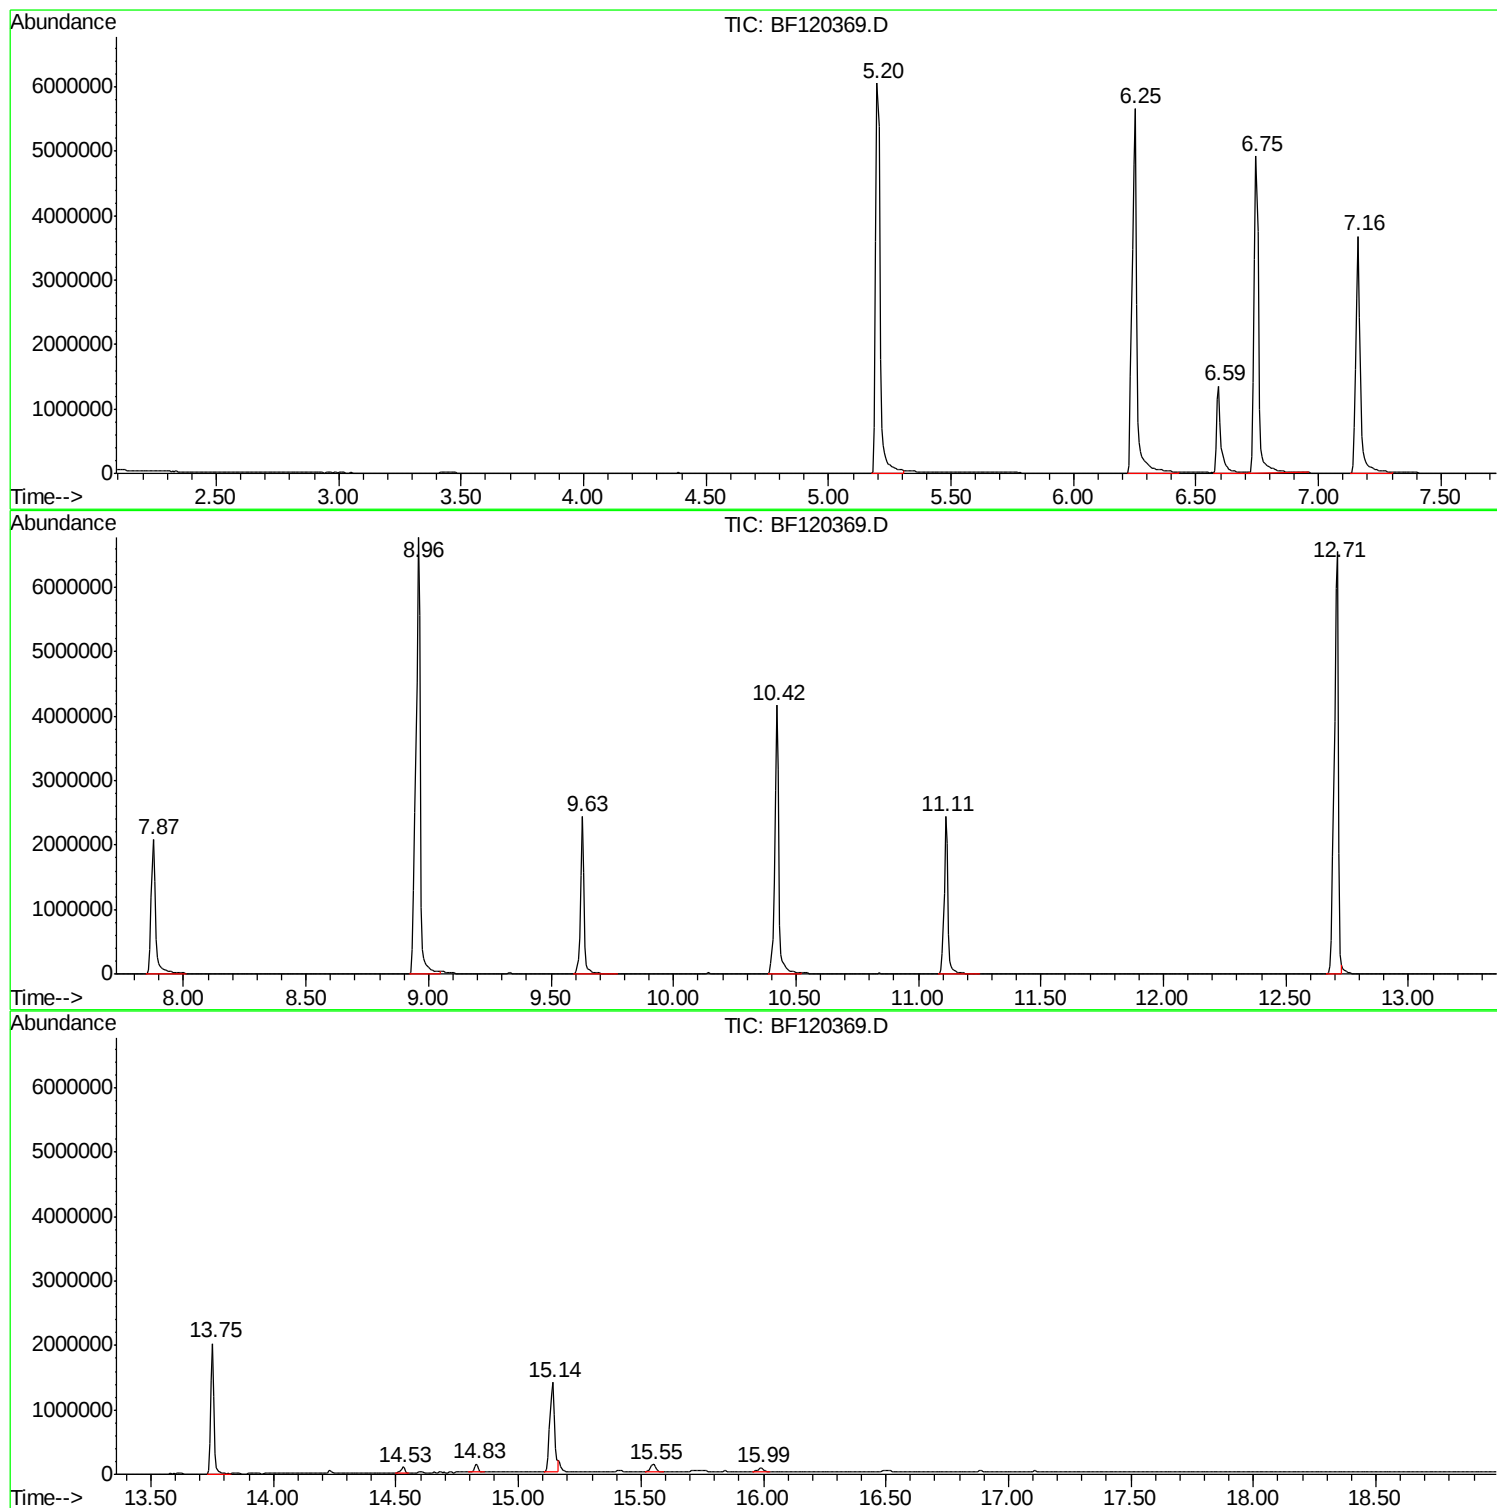

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF052020\
Data File : BF120369.D
Acq On : 20 May 2020 14:37
Operator : MA/SJ
Sample : PB129015BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB129015BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF052020\
Data File : BF120369.D
Acq On : 20 May 2020 14:37
Operator : MA/SJ
Sample : PB129015BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB129015BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc