


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF052020\  
 Data File : BF120367.D  
 Acq On : 20 May 2020 12:30  
 Operator : MA/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF051420.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Wed May 20 13:33:43 2020

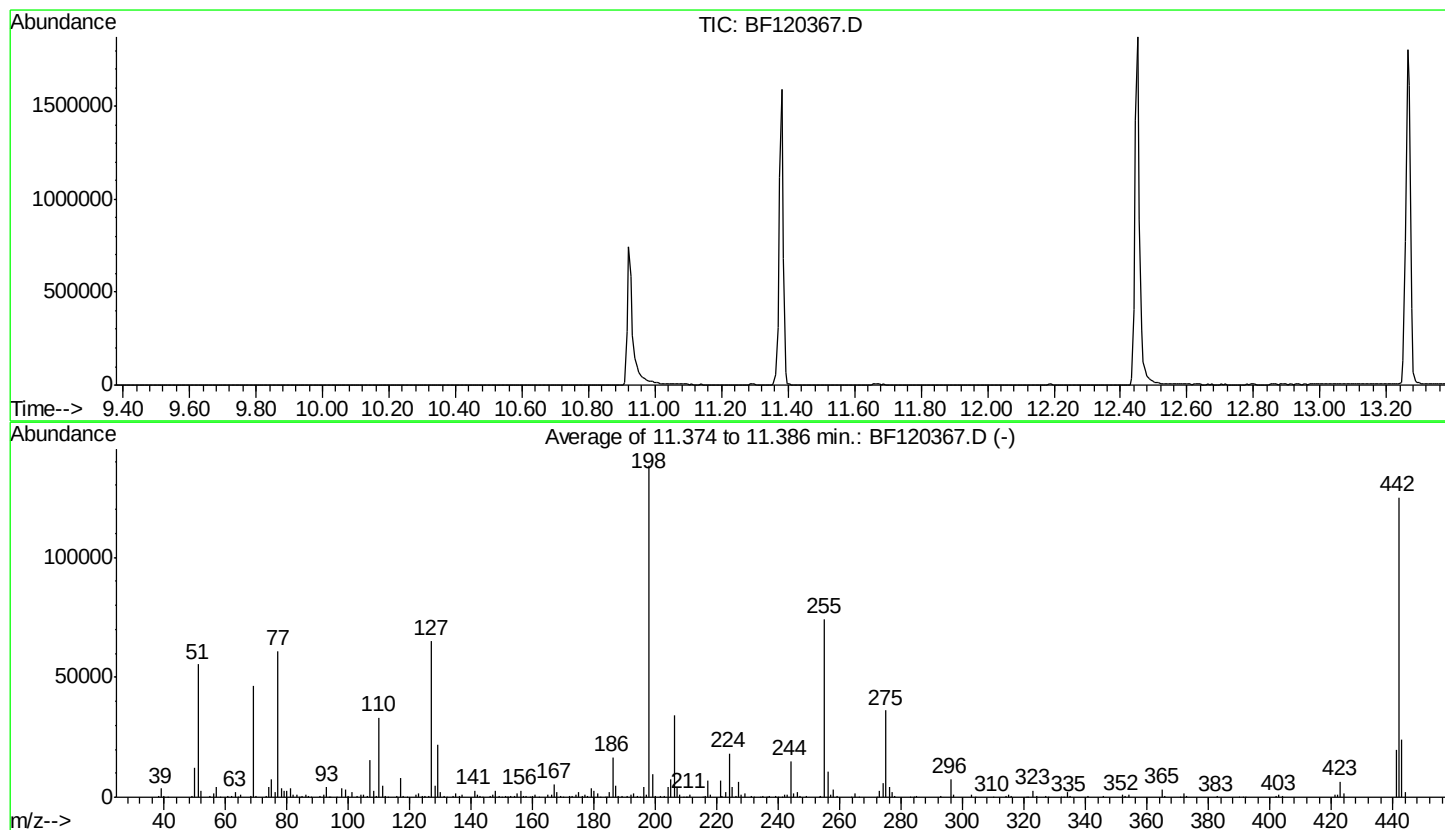

AutoFind: Scans 1579, 1580, 1581; Background Corrected with Scan 1573

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 40.1      | 55354   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.4       | 662     | PASS             |
| 69          | 198          | 0.00         | 100          | 33.6      | 46368   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.7       | 321     | PASS             |
| 127         | 198          | 10           | 80           | 47.2      | 65269   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.7       | 930     | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 138197  | PASS             |
| 199         | 198          | 5            | 9            | 6.8       | 9406    | PASS             |
| 275         | 198          | 10           | 60           | 26.2      | 36173   | PASS             |
| 365         | 198          | 1            | 100          | 2.5       | 3461    | PASS             |
| 441         | 198          | 0.01         | 100          | 14.4      | 19949   | PASS             |
| 442         | 198          | 50           | 100          | 90.4      | 124922  | PASS             |
| 443         | 442          | 15           | 24           | 19.3      | 24072   | PASS             |