
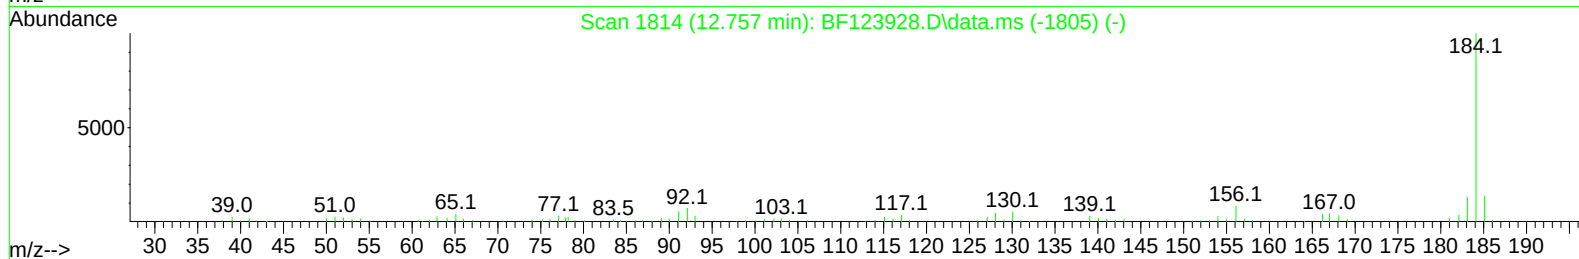
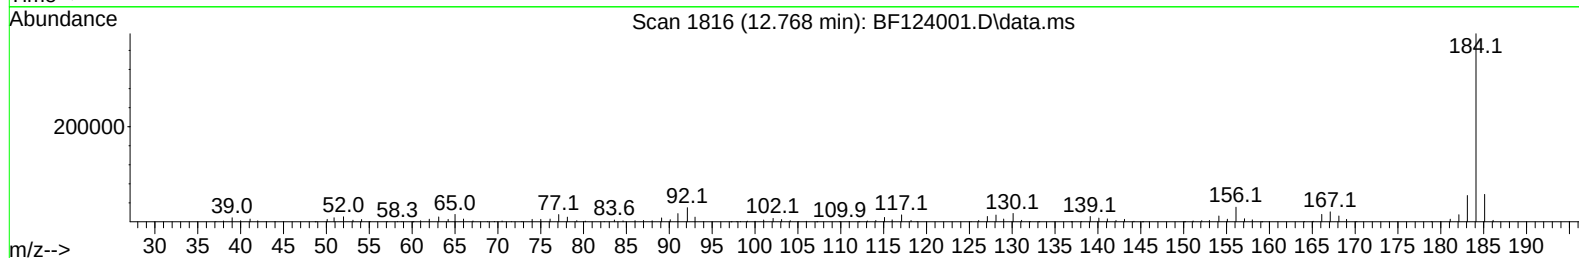


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052021\
Data File : BF124001.D
Acq On : 20 May 2021 9:41
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 20 11:02:37 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 14 19:05:57 2021
Response via : Initial Calibration

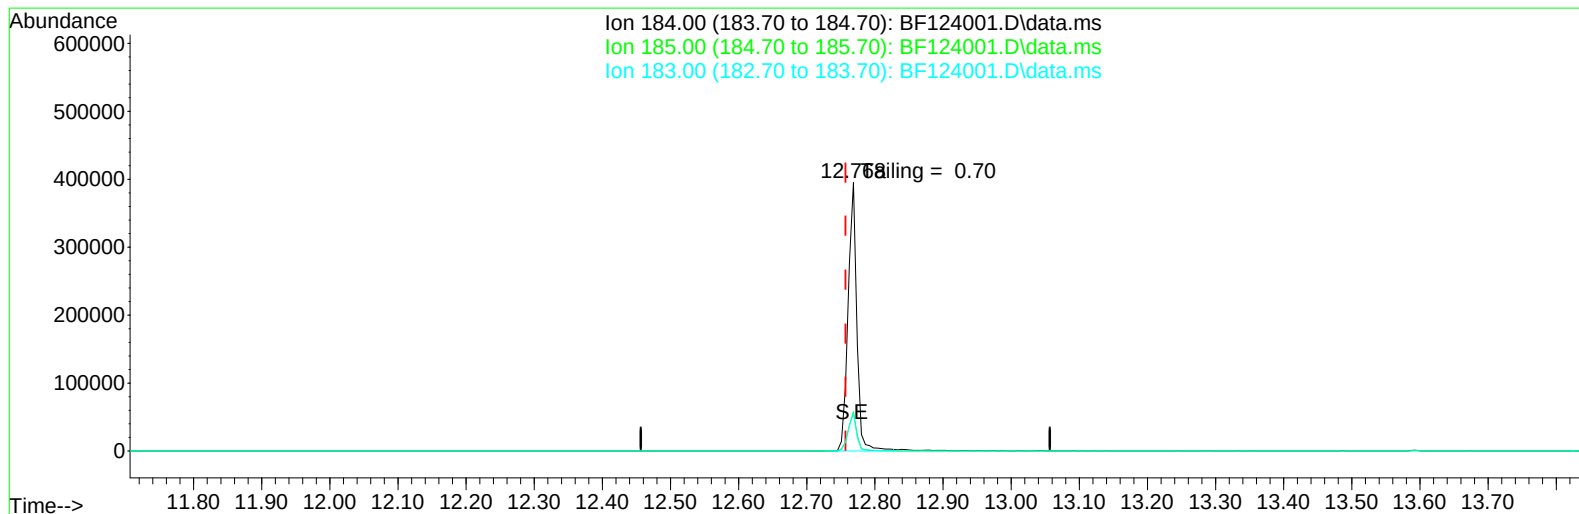

TIC: BF124001.D\data.ms

(77) Benzidine




12.768min (+ 0.012) 0.00 ng

response 352559

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.64
183.00	9.80	14.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052021\
Data File : BF124001.D
Acq On : 20 May 2021 9:41
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 20 11:02:37 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 14 19:05:57 2021
Response via : Initial Calibration

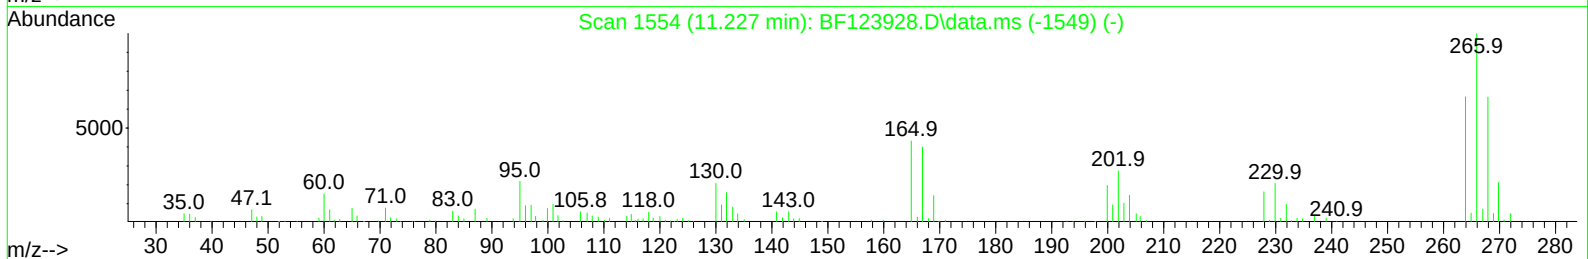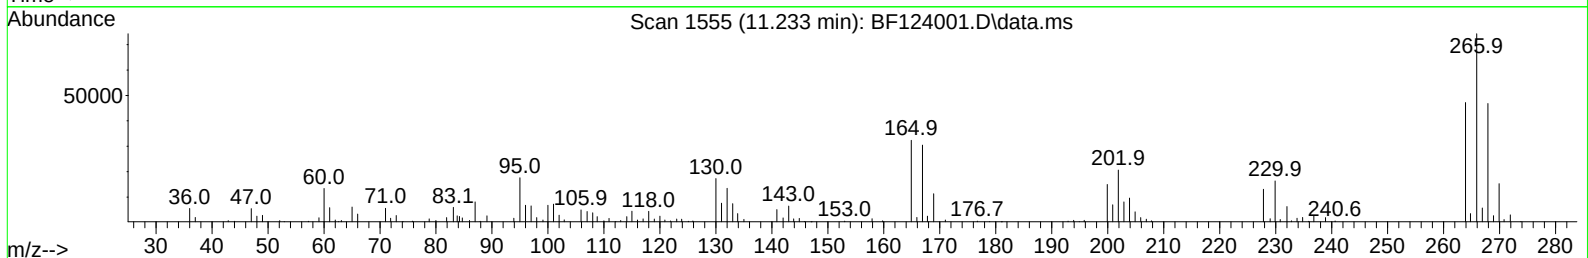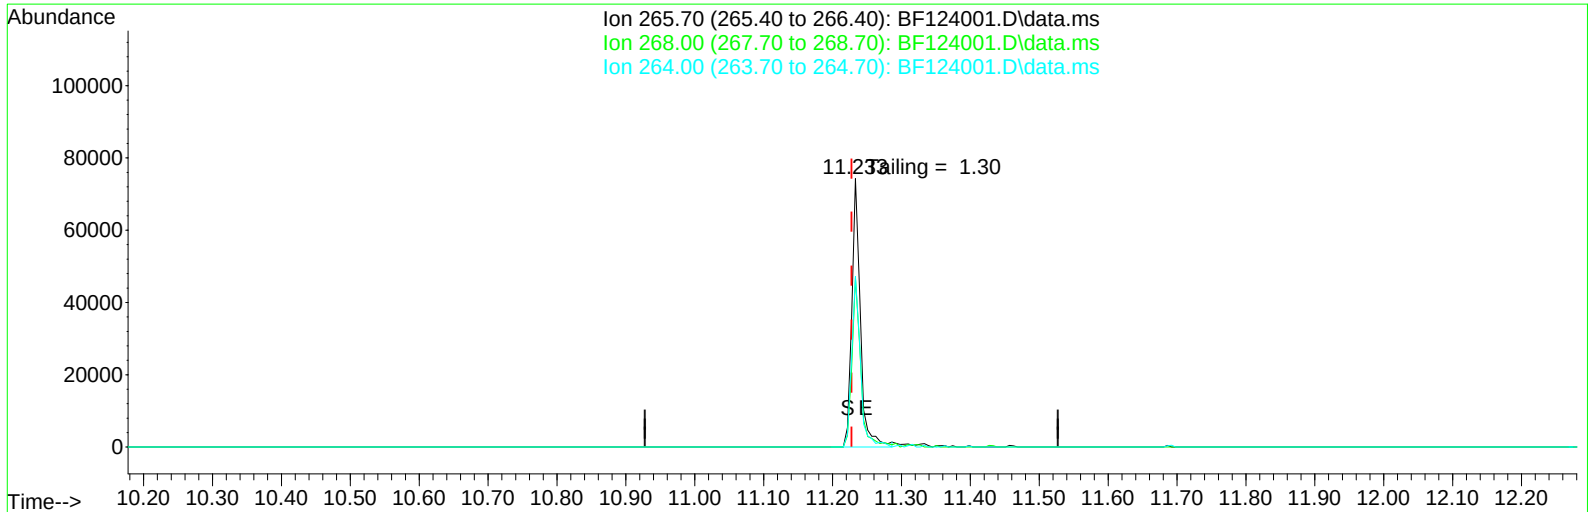

TIC: BF124001.D\data.ms

(70) Pentachlorophenol (C)

11.233min (+ 0.006) 11358.74 ng

response 64021

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.09
264.00	65.70	63.58
0.00	0.00	0.00