
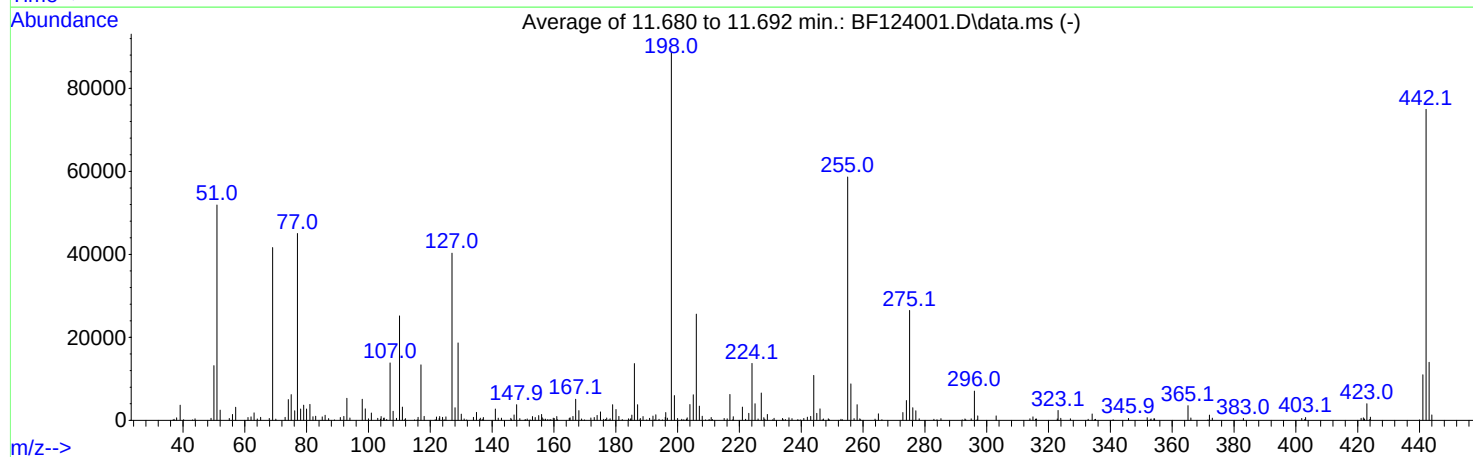


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052021\
 Data File : BF124001.D
 Acq On : 20 May 2021 9:41
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 14 19:05:57 2021

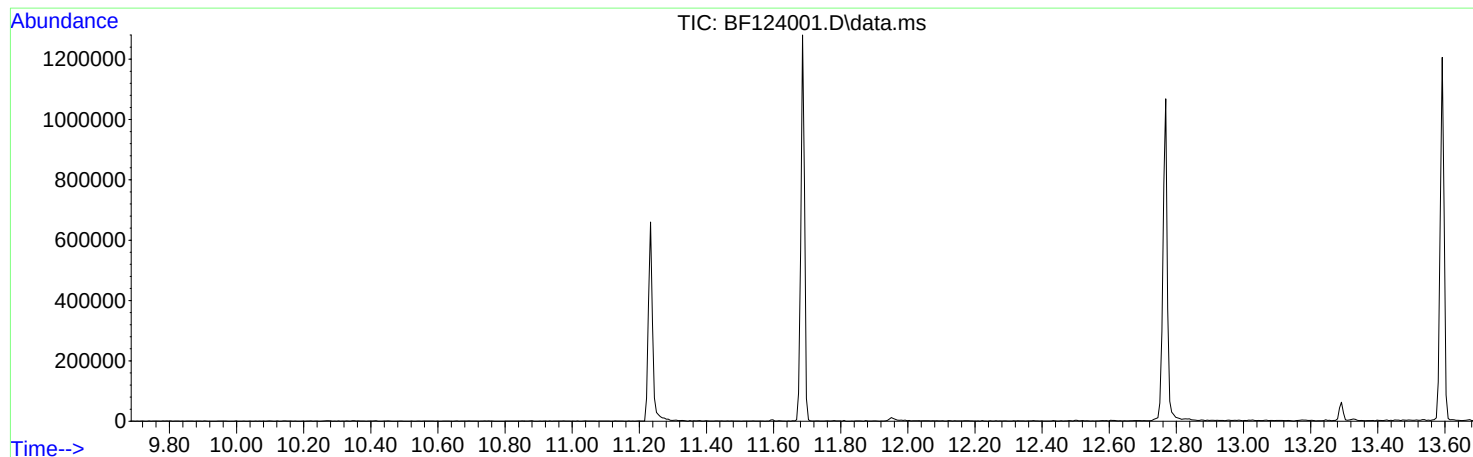




AutoFind: Scans 1631, 1632, 1633; Background Corrected with Scan 1626

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	58.5	51877	PASS
68	69	0.00	2	1.1	466	PASS
69	198	0.00	100	47.0	41635	PASS
70	69	0.00	2	0.7	295	PASS
127	198	10	80	45.5	40293	PASS
197	198	0.00	2	0.6	530	PASS
198	198	100	100	100.0	88637	PASS
199	198	5	9	6.8	5993	PASS
275	198	10	60	29.9	26481	PASS
365	198	1	100	4.0	3557	PASS
441	198	0.01	100	12.4	10983	PASS
442	442	50	100	100.0	74944	PASS
443	442	15	24	18.7	13988	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052021\
 Data File : BF124001.D
 Acq On : 20 May 2021 9:41
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: May 20 11:02:37 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 14 19:05:57 2021
 Response via : Initial Calibration

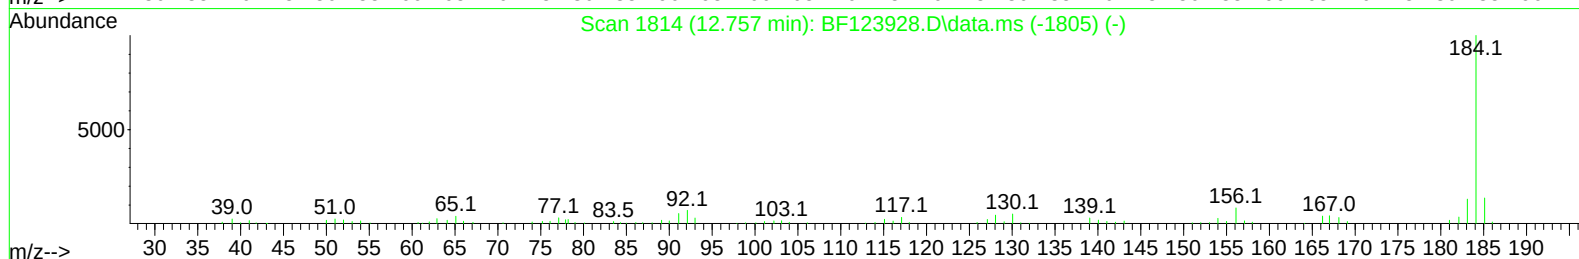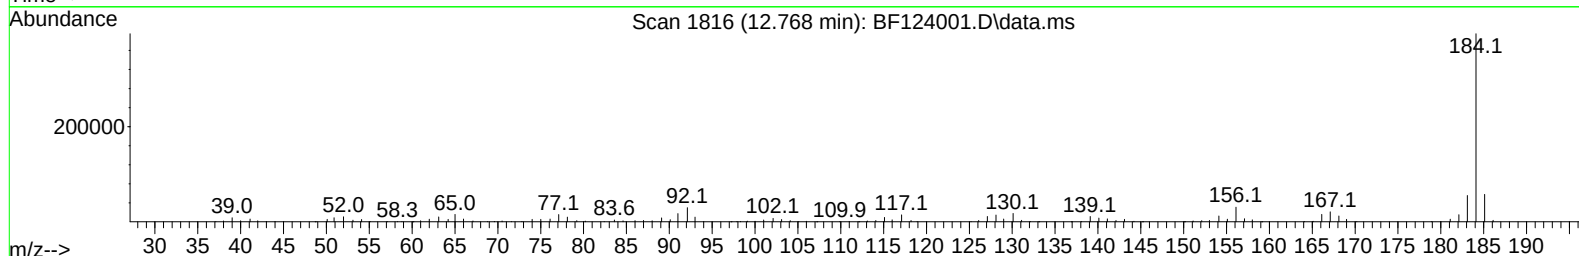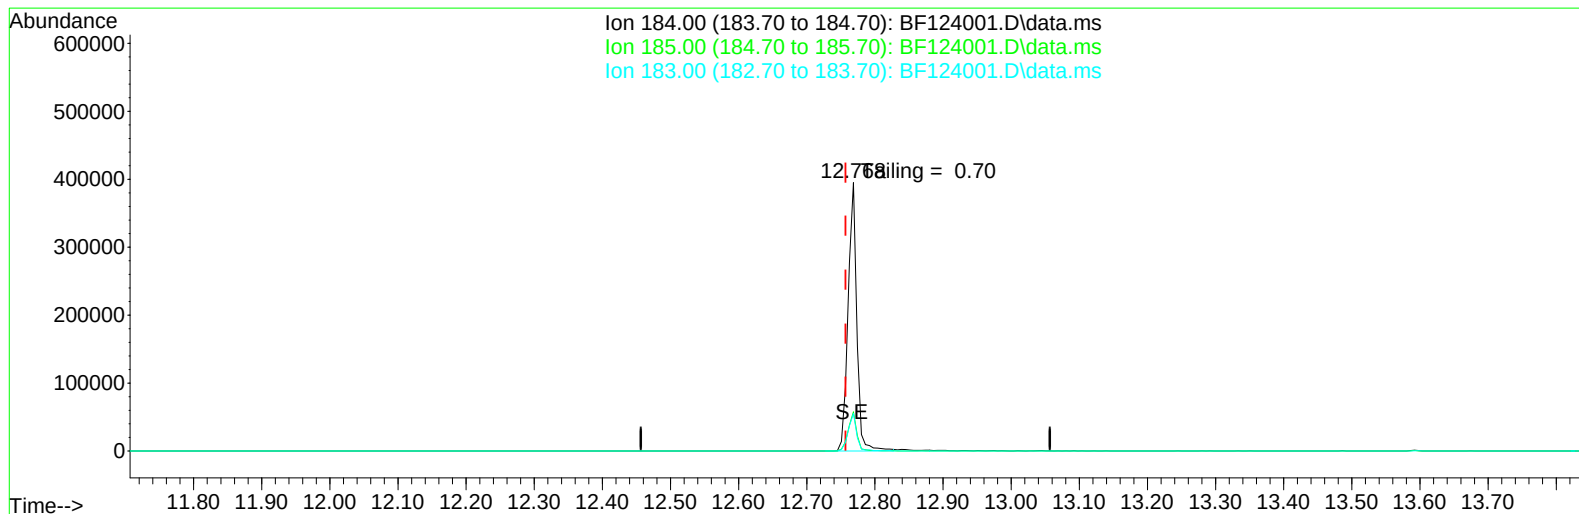

TIC: BF124001.D\data.ms

(77) Benzidine

12.768min (+ 0.012) 0.00 ng




response 352559

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.64
183.00	9.80	14.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052021\
Data File : BF124001.D
Acq On : 20 May 2021 9:41
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 20 11:02:37 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 14 19:05:57 2021
Response via : Initial Calibration

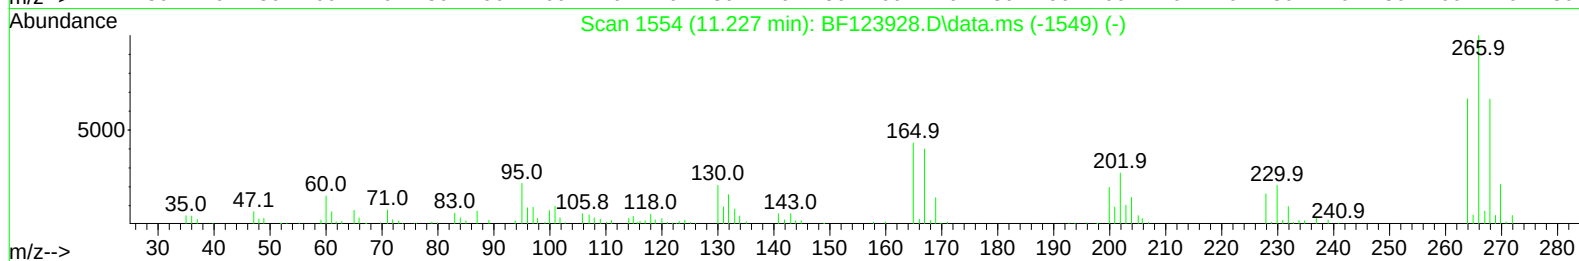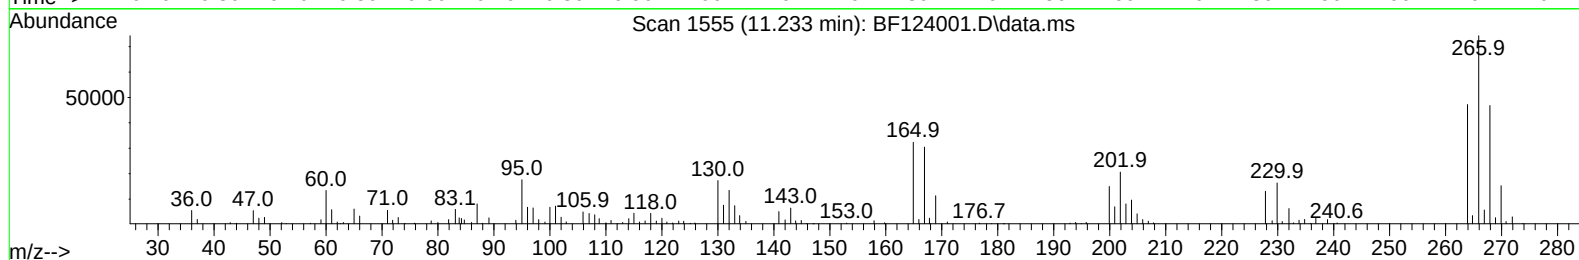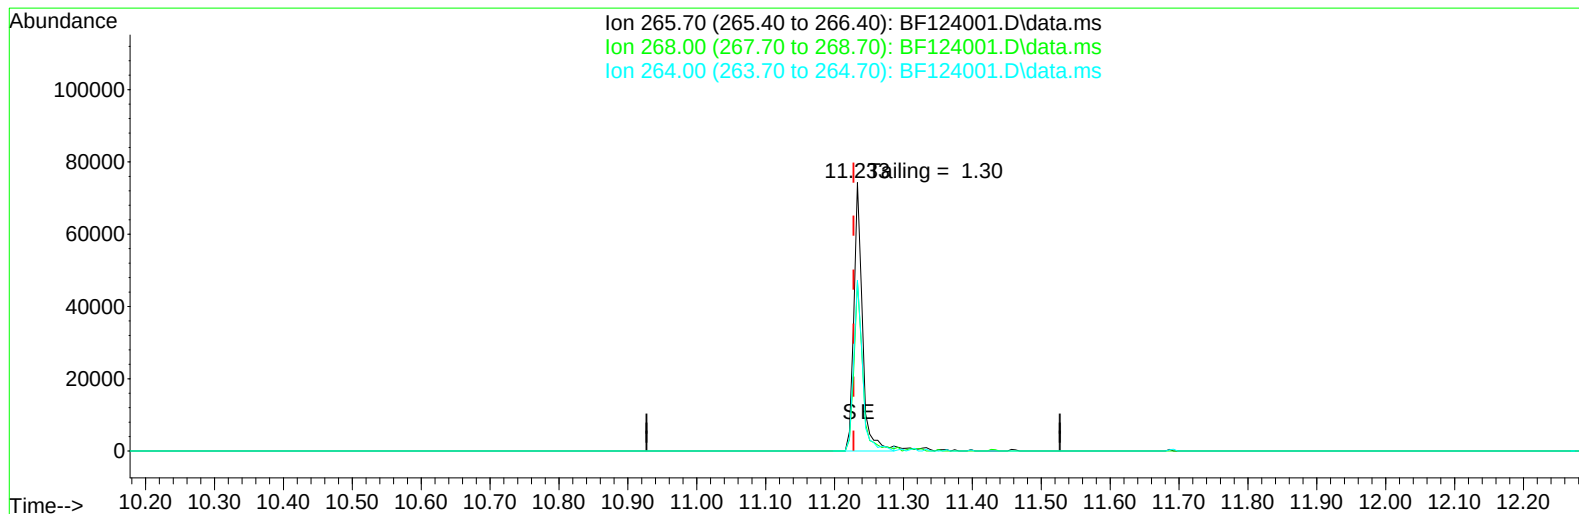

TIC: BF124001.D\data.ms

(70) Pentachlorophenol (C)

11.233min (+ 0.006) 11358.74 ng

response 64021

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.09
264.00	65.70	63.58
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/20/2021	BNA_F	BF124001.D
Compound Name	Response	Retention Time
DDT	177707	13.59
DDD	10188	13.29
DDE	525	12.96
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10713	188420	5.69