
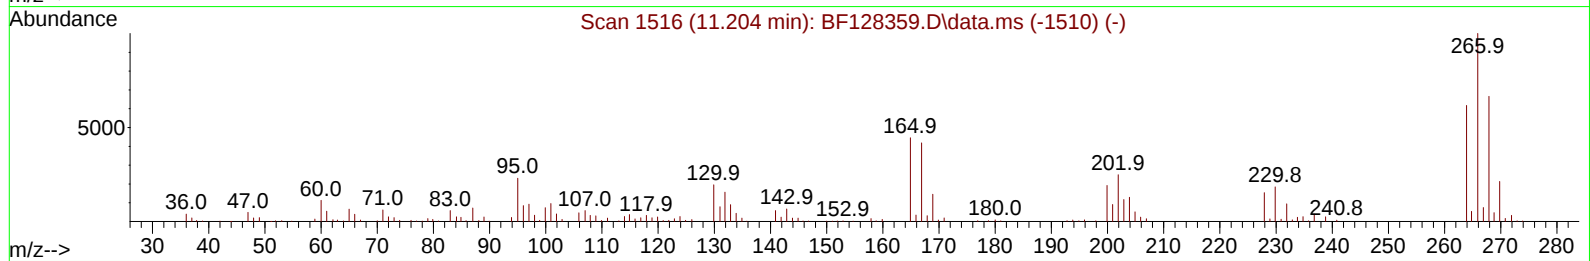
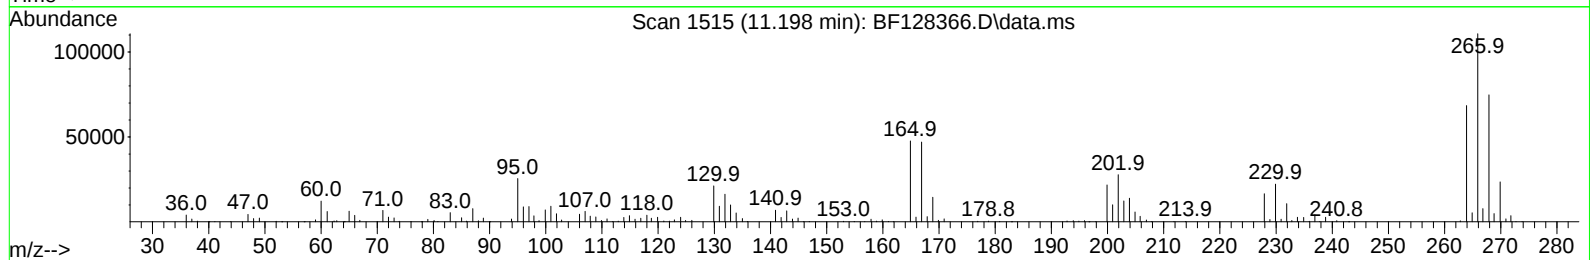


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052022\
Data File : BF128366.D
Acq On : 20 May 2022 16:09
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 23 04:02:35 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 21 05:28:09 2022
Response via : Initial Calibration

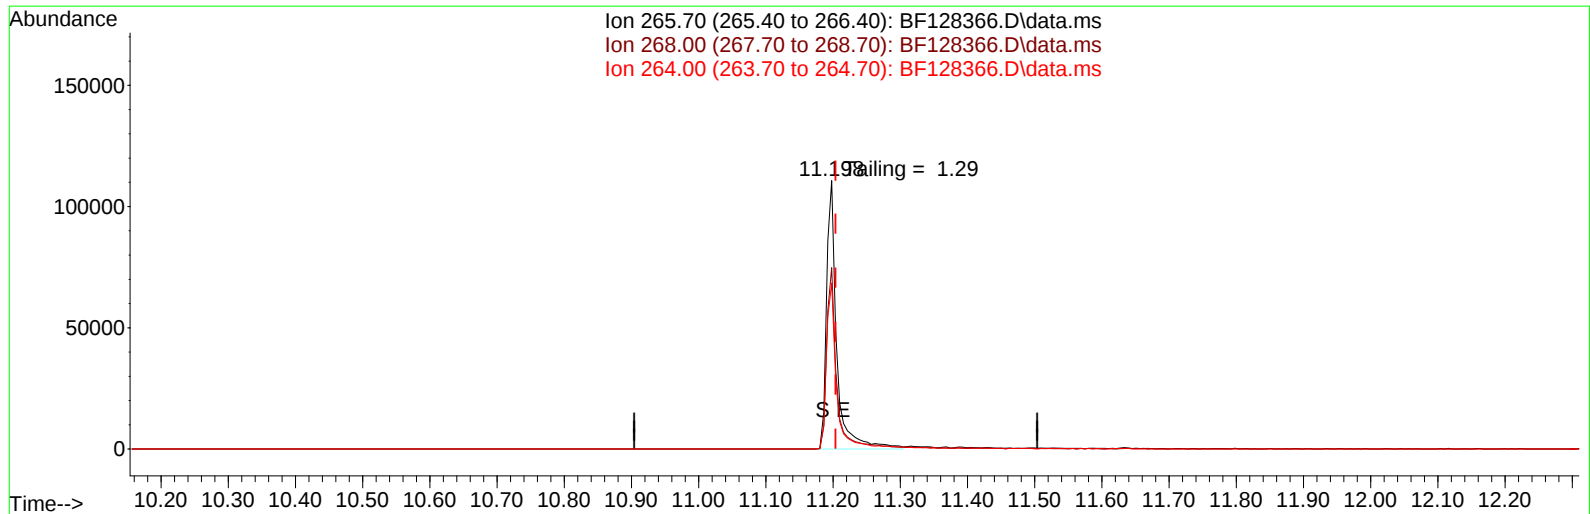

TIC: BF128366.D\data.ms




(70) Pentachlorophenol (C)

11.198min (-0.006) 38440.35 ng

response 118065

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.30	67.55
264.00	66.40	61.81
0.00	0.00	0.00

Quant Time: May 23 04:02:35 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 21 05:28:09 2022
Response via : Initial Calibration

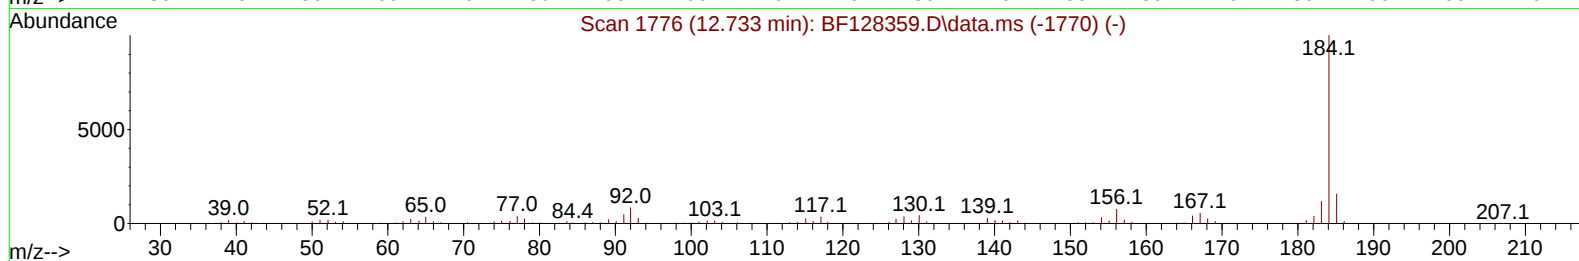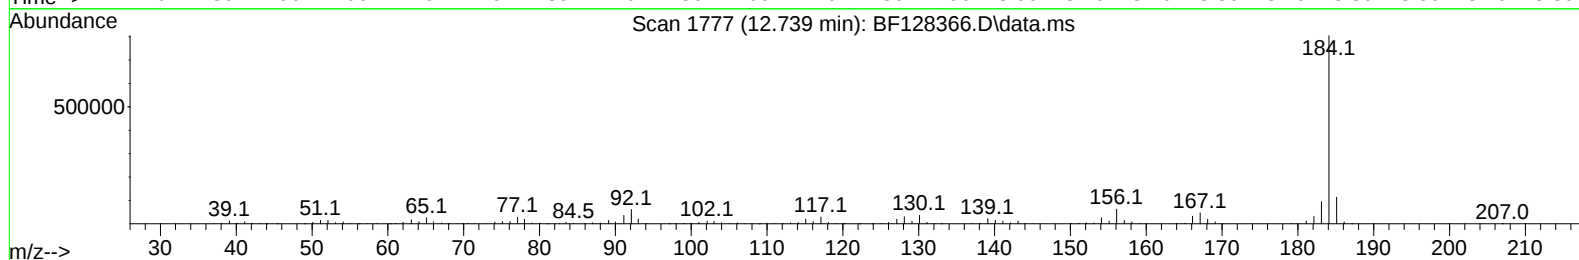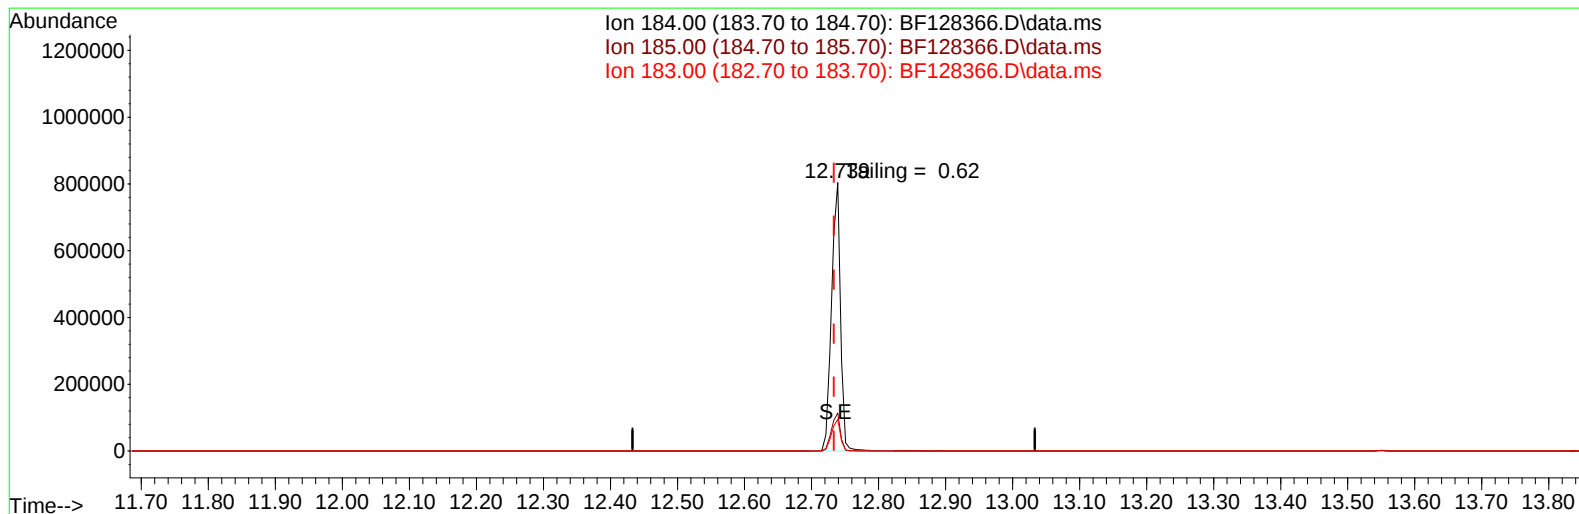

TIC: BF128366.D\data.ms

(77) Benzidine

12.739min (+ 0.006) 0.00 ng

response **747699**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.16
183.00	11.20	11.76
0.00	0.00	0.00