

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052022\
 Data File : BF128375.D
 Acq On : 20 May 2022 20:37
 Operator : CG\JU
 Sample : N2943-06
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-18R

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128375.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.475	539	542	553	rBV	1098017	1144555	37.73%	7.566%
2	6.487	711	714	731	rBV	783500	723746	23.86%	4.784%
3	6.857	773	777	784	rBV	635272	531095	17.51%	3.511%
4	7.428	869	874	877	rBV	1772345	1797971	59.28%	11.886%
5	8.139	991	995	1010	rBV	831329	687021	22.65%	4.542%
6	9.216	1173	1178	1181	rBV	3345298	3033174	100.00%	20.051%
7	9.898	1290	1294	1297	rBV	871033	749358	24.71%	4.954%
8	10.692	1425	1429	1432	rBV	1935087	1720137	56.71%	11.371%
9	11.386	1544	1547	1551	rBV	773555	723442	23.85%	4.782%
10	11.904	1632	1635	1640	rBV3	31339	37928	1.25%	0.251%
11	12.980	1813	1818	1821	rBV	2687561	2545688	83.93%	16.829%
12	13.892	1969	1973	1983	rVB4	26889	51194	1.69%	0.338%
13	14.039	1994	1998	2002	rBV	633455	545412	17.98%	3.606%
14	14.133	2009	2014	2019	rBV	83221	84215	2.78%	0.557%
15	15.133	2180	2184	2188	rBV	33611	38245	1.26%	0.253%
16	15.527	2245	2251	2260	rVB	446579	583587	19.24%	3.858%
17	15.957	2319	2324	2327	rBV	33795	48368	1.59%	0.320%
18	16.468	2406	2411	2415	rBV2	27700	45647	1.50%	0.302%
19	17.068	2509	2513	2519	rVB2	19755	36293	1.20%	0.240%




Sum of corrected areas: 15127076

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052022\
Data File : BF128375.D
Acq On : 20 May 2022 20:37
Operator : CG\JU
Sample : N2943-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-18R

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

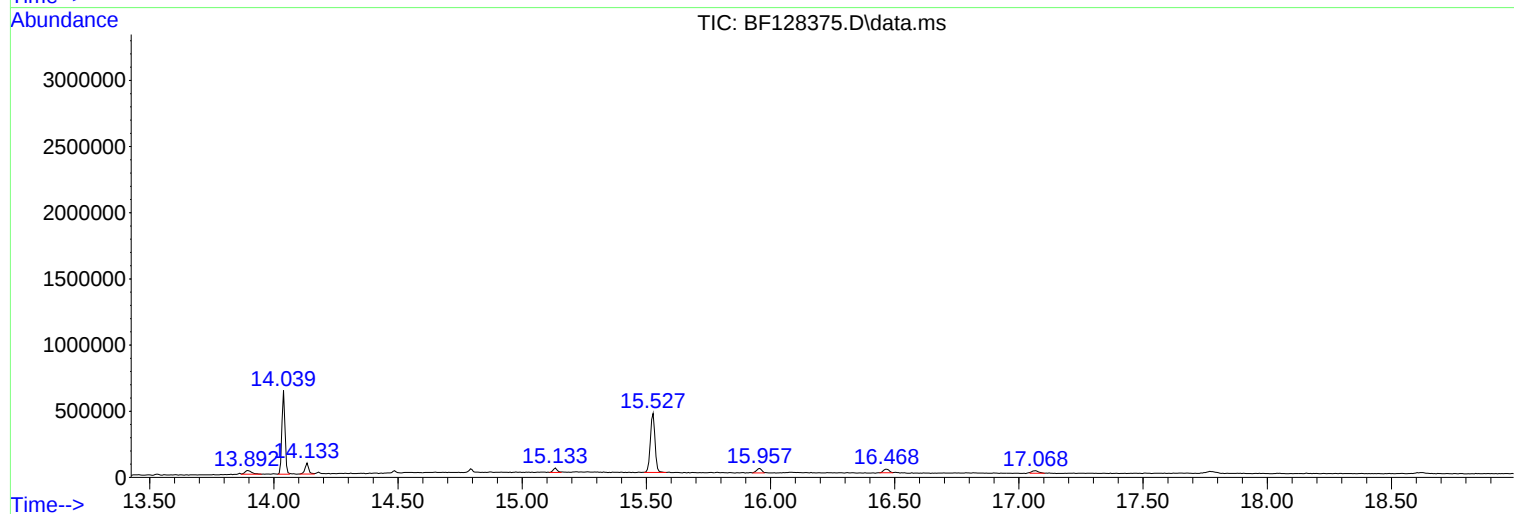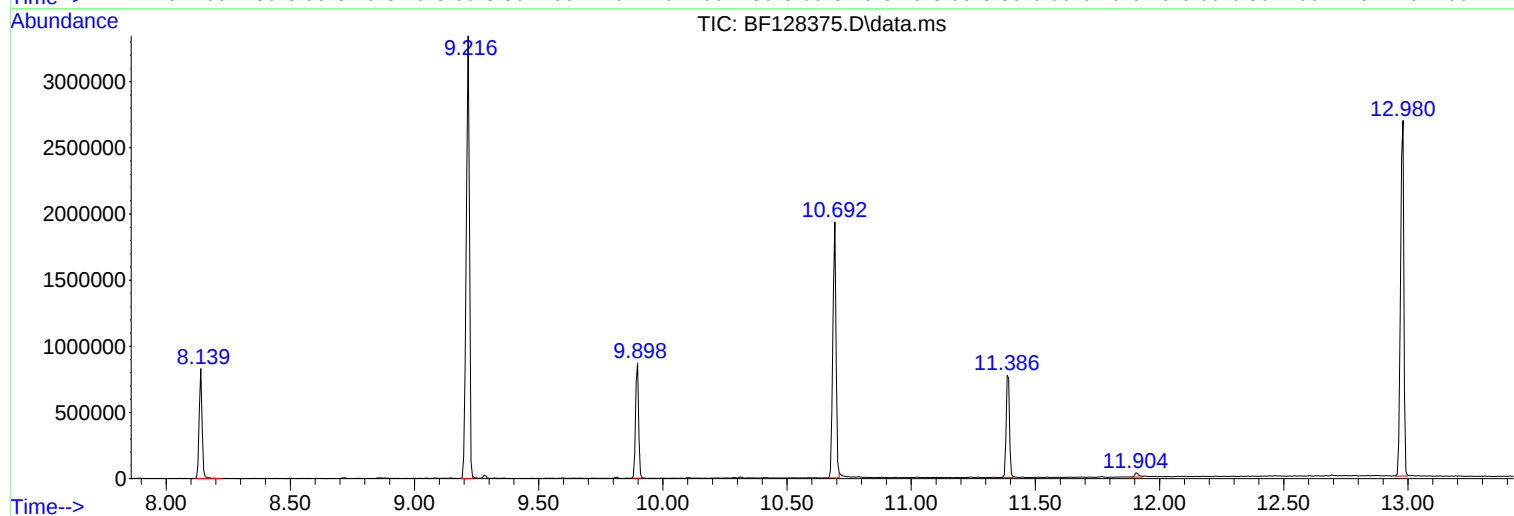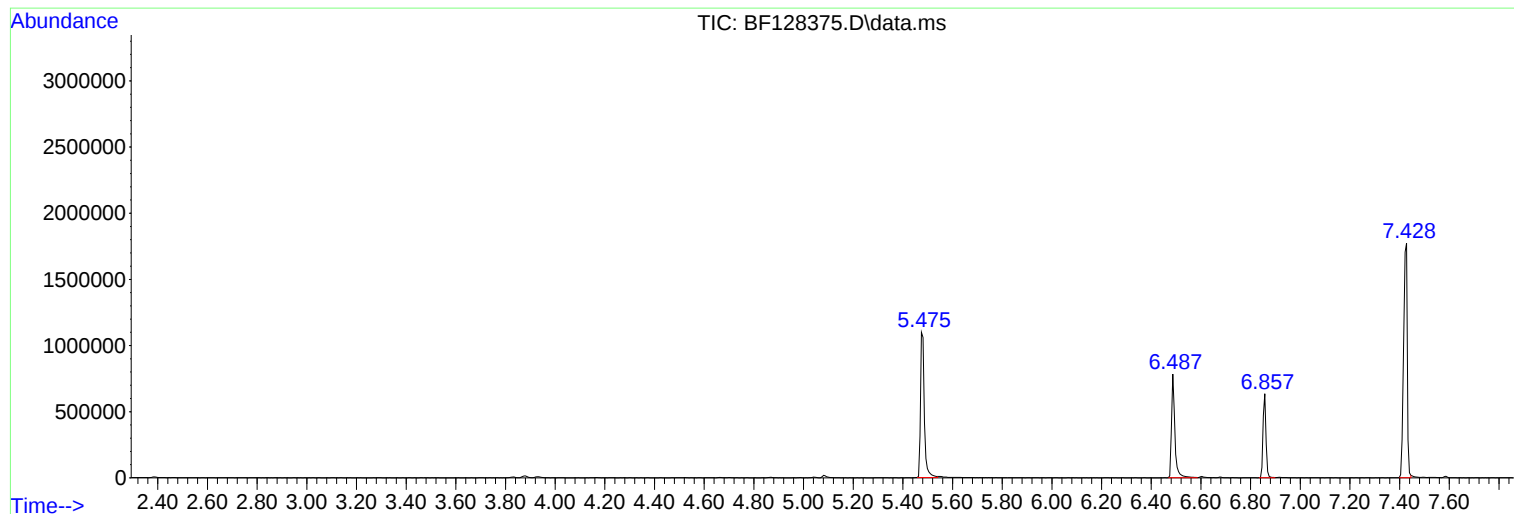

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052022\
Data File : BF128375.D
Acq On : 20 May 2022 20:37
Operator : CG\JU
Sample : N2943-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-18R










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.133	3.09 ng	84215	Chrysene-d12	14.039

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	83
2			Formaldehyde, (triphenylphosphor...	304	C19H17N2P	015990-54-2	56
3			(E)-7-Benzylidene-1-azabicyclo[3...	293	C15H19N03S	1000483-83-4	52
4			Cobalt,(.eta.<5>-2,4-cyclopentad...	277	C16H15BCo	036682-12-9	37
5			2-Phenyl-6-(trifluoromethyl)-1H...	277	C15H10F3NO	1000387-59-3	37

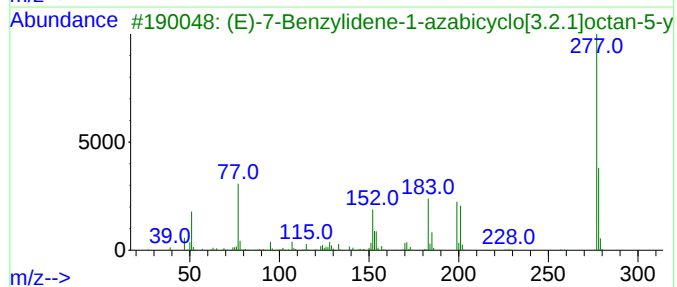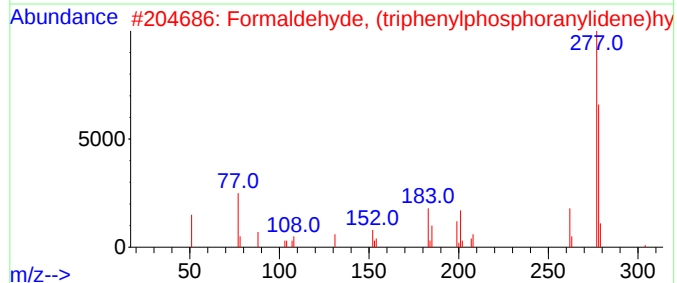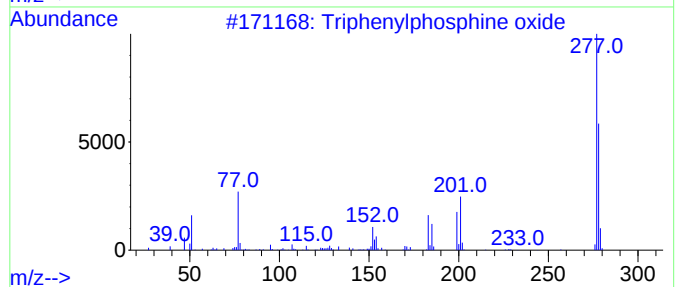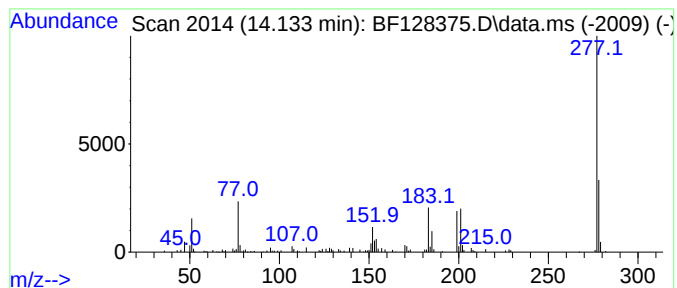

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052022\
Data File : BF128375.D
Acq On : 20 May 2022 20:37
Operator : CG\JU
Sample : N2943-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-18R

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Triphenylphosph...	14.133	3.1	ng	84215	5	14.039	545412	20.0