

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052022\
 Data File : BF128388.D
 Acq On : 21 May 2022 03:00
 Operator : CG\JU
 Sample : N2939-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 B1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128388.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.110	476	480	488	rBV	34437	49181	1.59%	0.258%
2	5.493	540	545	563	rBV	2559960	2674512	86.49%	14.005%
3	6.498	711	716	719	rBV	2542080	2582028	83.50%	13.521%
4	6.857	773	777	784	rBV	634272	528800	17.10%	2.769%
5	7.428	869	874	877	rBV	1840102	1832711	59.27%	9.597%
6	8.140	991	995	1003	rBV	782460	667399	21.58%	3.495%
7	9.216	1173	1178	1181	rBV	3313980	3092180	100.00%	16.193%
8	9.610	1242	1245	1249	rBV	68296	54031	1.75%	0.283%
9	9.898	1290	1294	1297	rBV	907842	778430	25.17%	4.076%
10	10.692	1425	1429	1432	rBV	2127694	1861416	60.20%	9.748%
11	11.392	1544	1548	1551	rBV	829798	763881	24.70%	4.000%
12	12.980	1813	1818	1821	rBV	2956092	2713439	87.75%	14.209%
13	13.886	1969	1972	1981	rVB5	23514	50880	1.65%	0.266%
14	14.039	1994	1998	2005	rBV	640539	548976	17.75%	2.875%
15	14.127	2009	2013	2019	rBV	60725	64091	2.07%	0.336%
16	14.792	2123	2126	2132	rVB	38649	39079	1.26%	0.205%
17	15.133	2180	2184	2188	rVB	38122	41610	1.35%	0.218%
18	15.527	2245	2251	2262	rVB	452741	603340	19.51%	3.159%
19	15.951	2319	2323	2331	rVB2	36368	55808	1.80%	0.292%
20	16.463	2405	2410	2419	rBV3	25537	55728	1.80%	0.292%
21	17.062	2507	2512	2519	rVB3	19912	38789	1.25%	0.203%




Sum of corrected areas: 19096309

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052022\
Data File : BF128388.D
Acq On : 21 May 2022 03:00
Operator : CG\JU
Sample : N2939-01
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
B1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

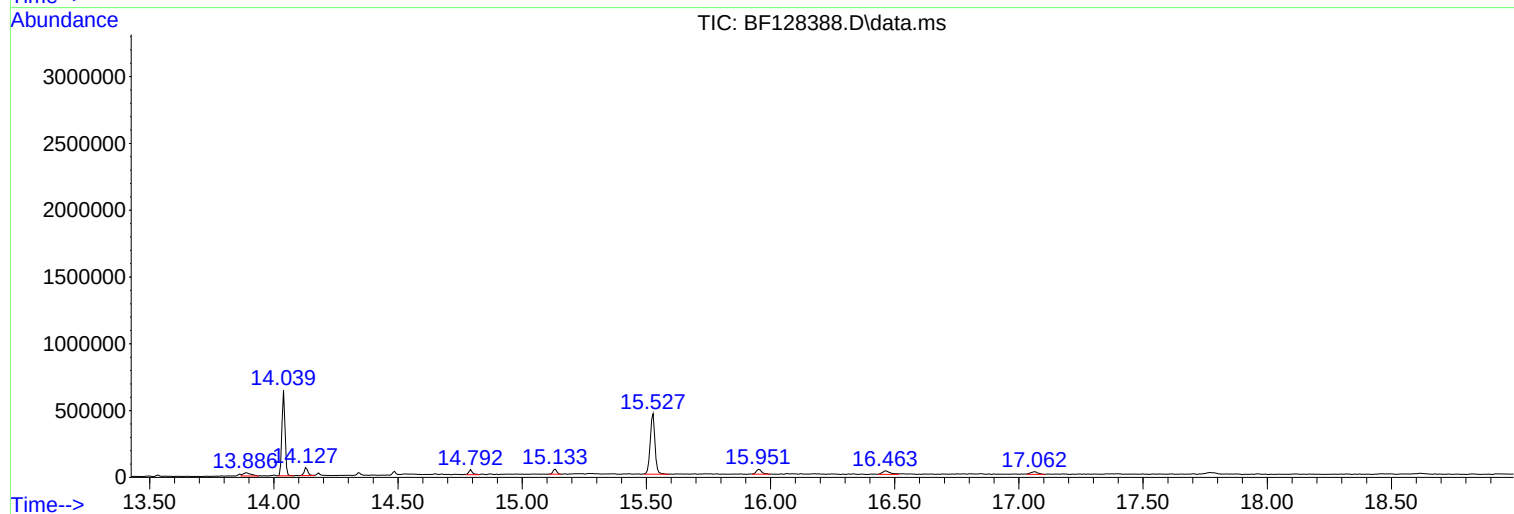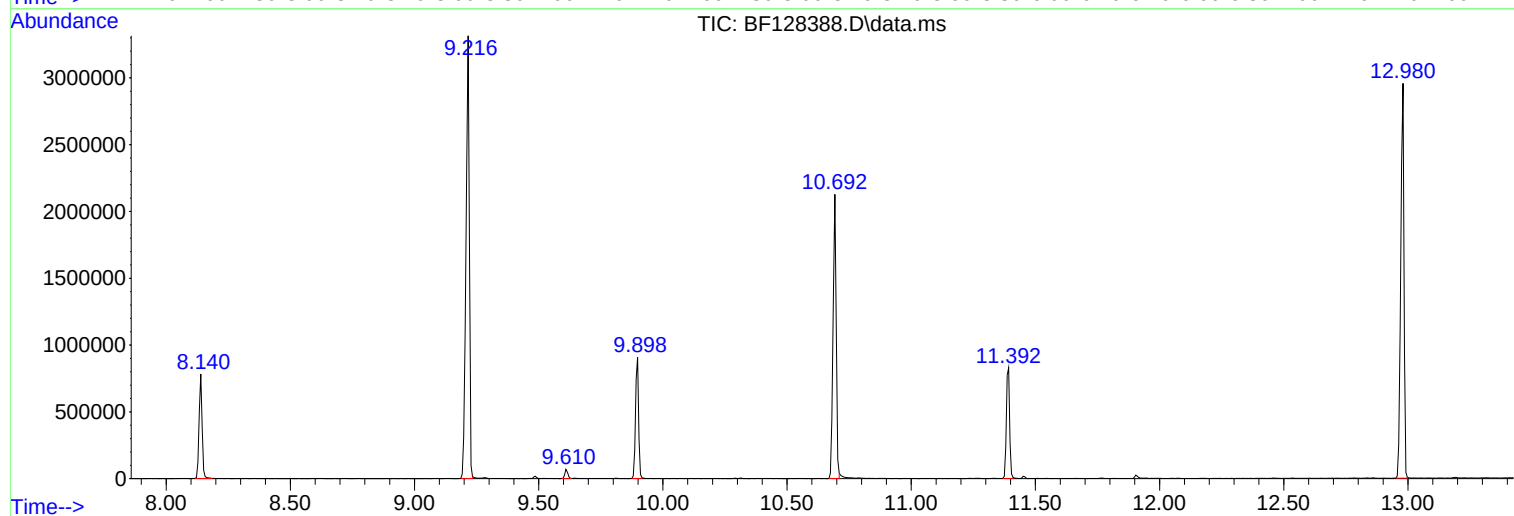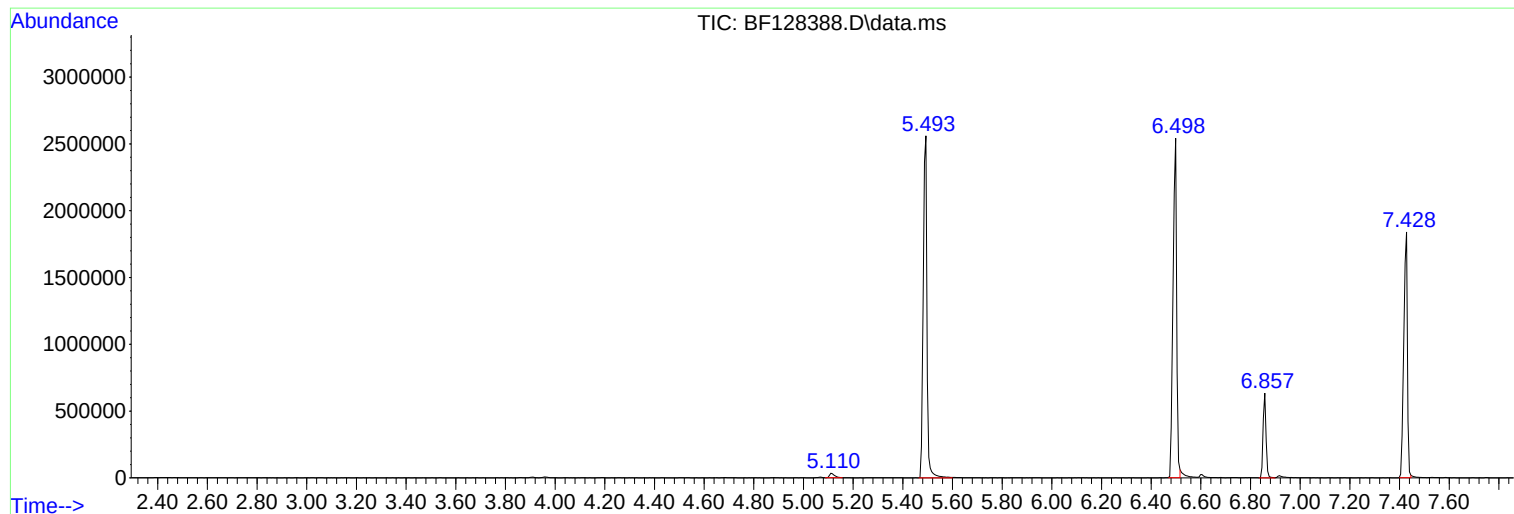

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052022\
Data File : BF128388.D
Acq On : 21 May 2022 03:00
Operator : CG\JU
Sample : N2939-01
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
B1










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.127	2.33 ng	64091	Chrysene-d12	14.039

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	96
2			(E)-7-Benzylidene-1-azabicyclo[3...	293	C15H19NO3S	1000483-83-4	58
3			Formaldehyde, (triphenylphosphor...	304	C19H17N2P	015990-54-2	50
4			3-(3,4-Dichlorophenyl)-2-thioxo...	277	C9H5Cl2NOS2	017046-34-3	35
5			Cobalt,(.eta.<5>-2,4-cyclopentad...	277	C16H15BCo	036682-12-9	32

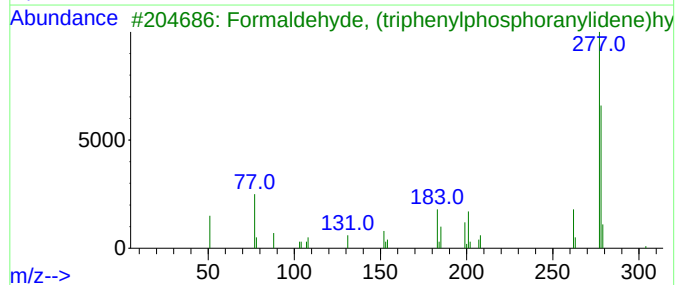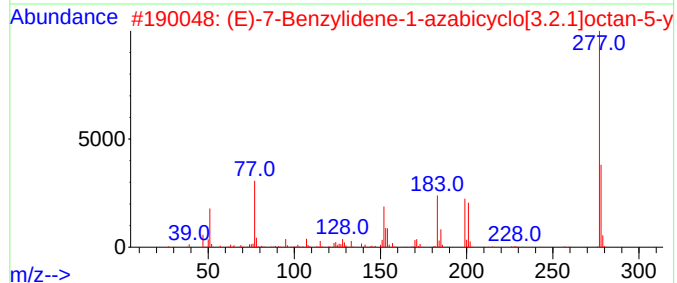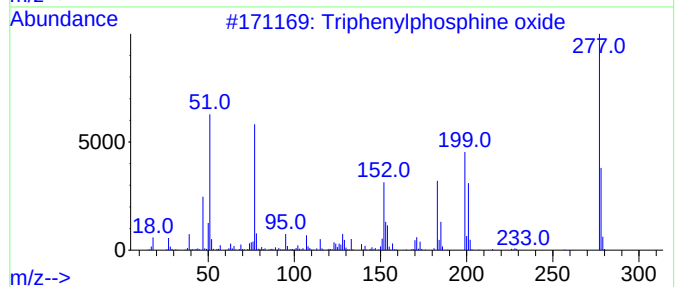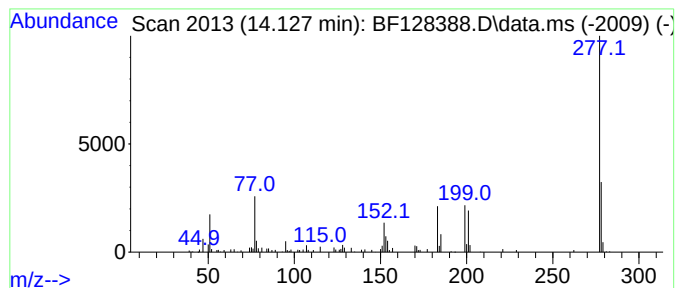

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052022\
Data File : BF128388.D
Acq On : 21 May 2022 03:00
Operator : CG\JU
Sample : N2939-01
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
B1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Triphenylphosph...	14.127	2.3	ng	64091	5	14.039	548976	20.0