
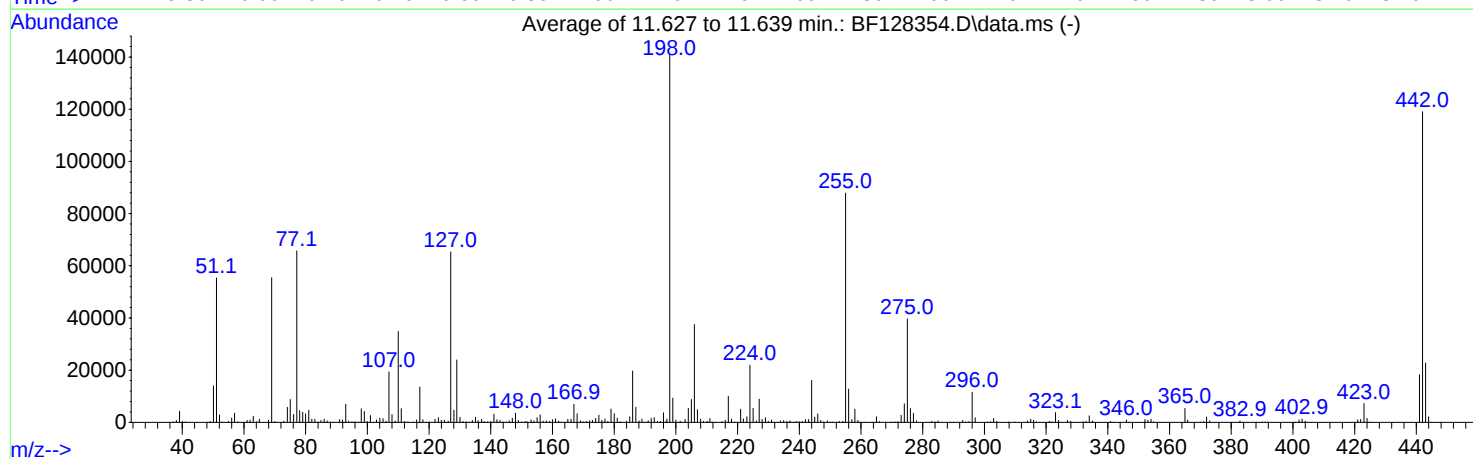


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052022\
 Data File : BF128354.D
 Acq On : 20 May 2022 09:45
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat May 21 05:28:09 2022

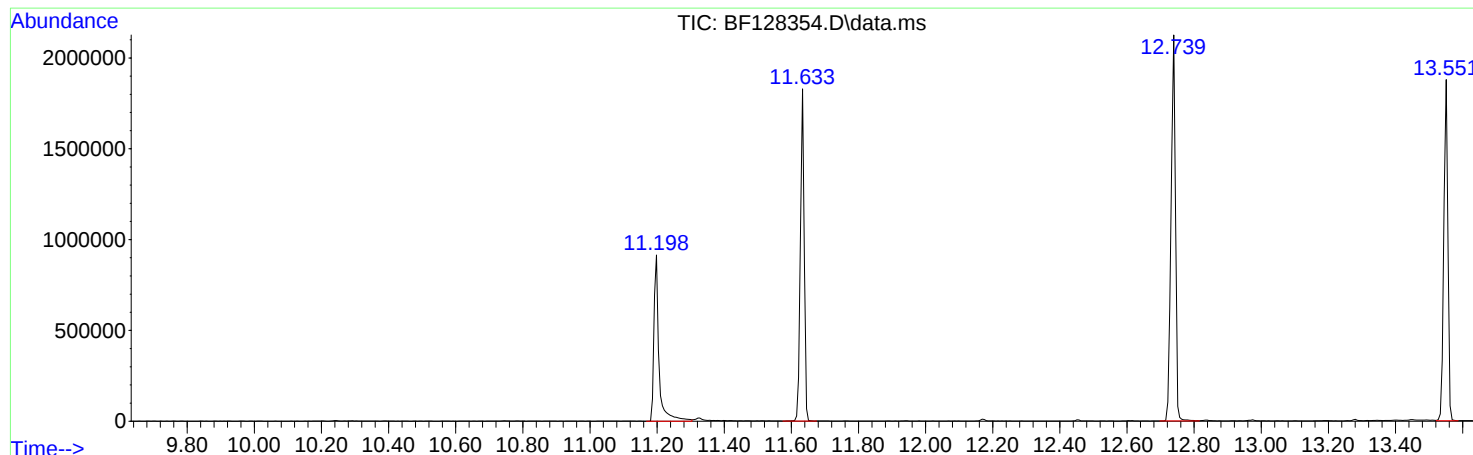




AutoFind: Scans 1588, 1589, 1590; Background Corrected with Scan 1582

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.2	55280	PASS
68	69	0.00	2	1.5	837	PASS
69	198	0.00	100	39.3	55416	PASS
70	69	0.00	2	0.5	289	PASS
127	198	10	80	46.3	65293	PASS
197	198	0.00	2	0.9	1314	PASS
198	198	100	100	100.0	140963	PASS
199	198	5	9	6.6	9349	PASS
275	198	10	60	28.2	39691	PASS
365	198	1	100	3.8	5367	PASS
441	198	0.01	100	13.0	18259	PASS
442	442	50	100	100.0	118987	PASS
443	442	15	24	19.1	22745	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052022\
Data File : BF128354.D
Acq On : 20 May 2022 09:45
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 20 13:07:03 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 20 13:02:47 2022
Response via : Initial Calibration

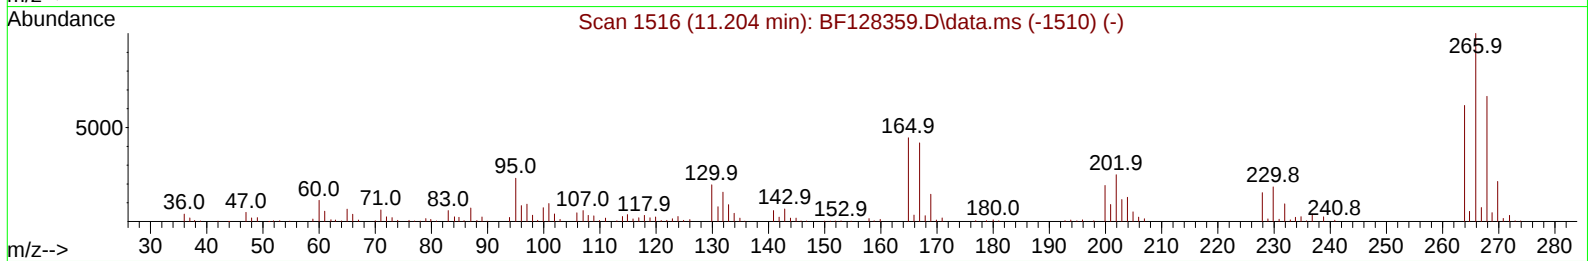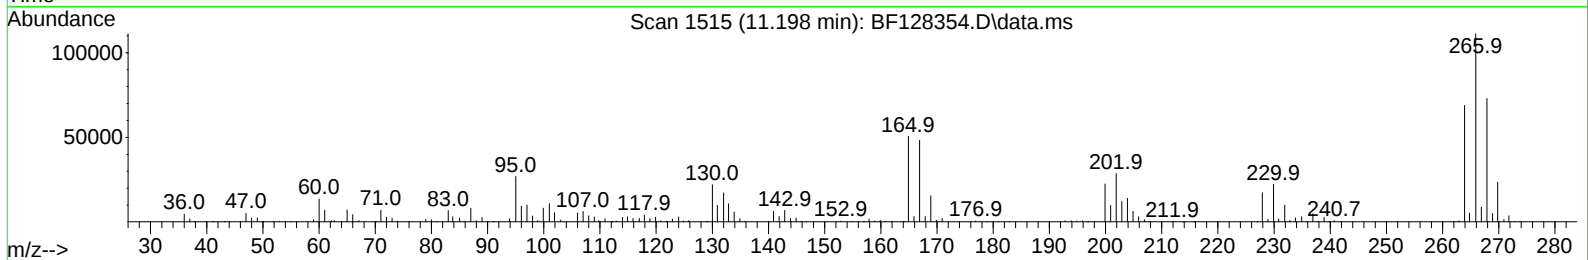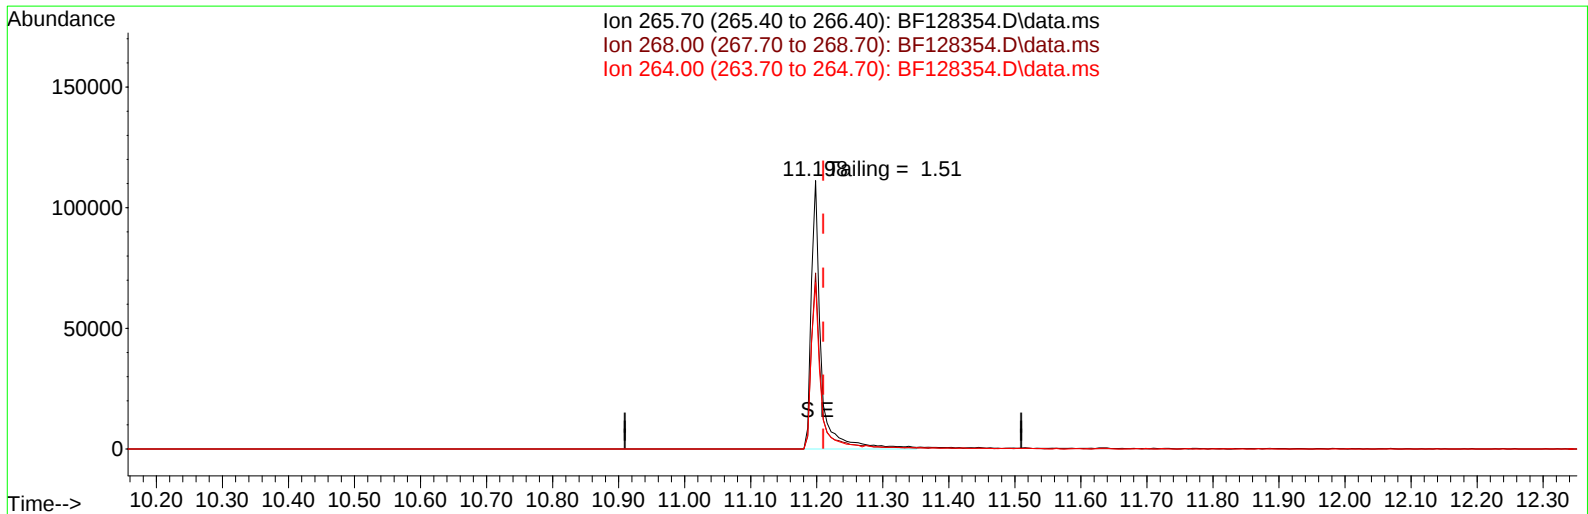

TIC: BF128354.D\data.ms

(70) Pentachlorophenol (C)

11.198min (-0.012) 32674.71 ng




response 114962

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.30	65.59
264.00	66.40	61.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052022\
Data File : BF128354.D
Acq On : 20 May 2022 09:45
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 20 13:07:03 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 20 13:02:47 2022
Response via : Initial Calibration

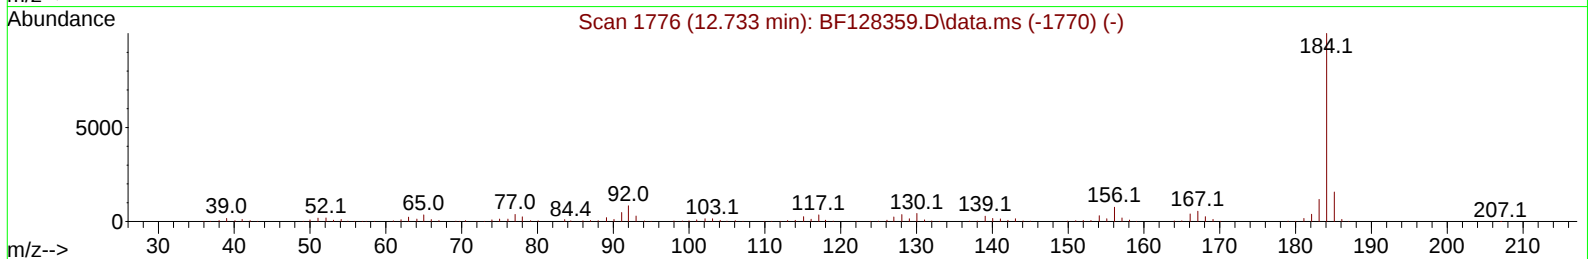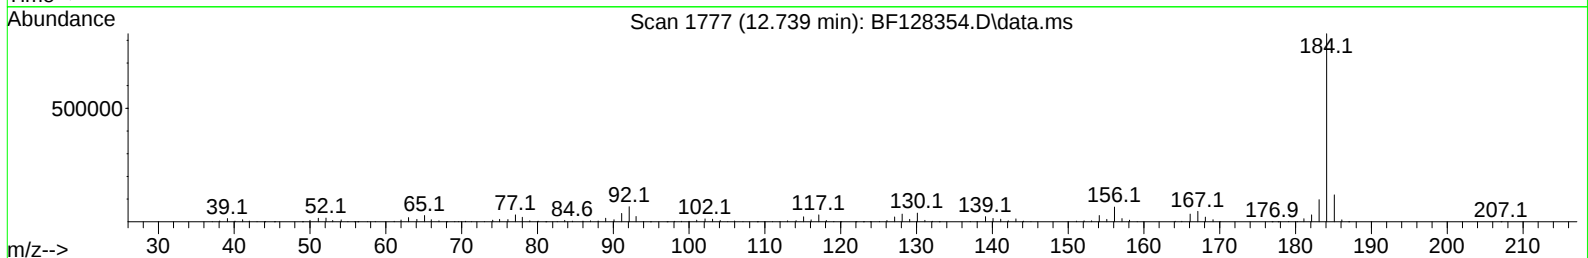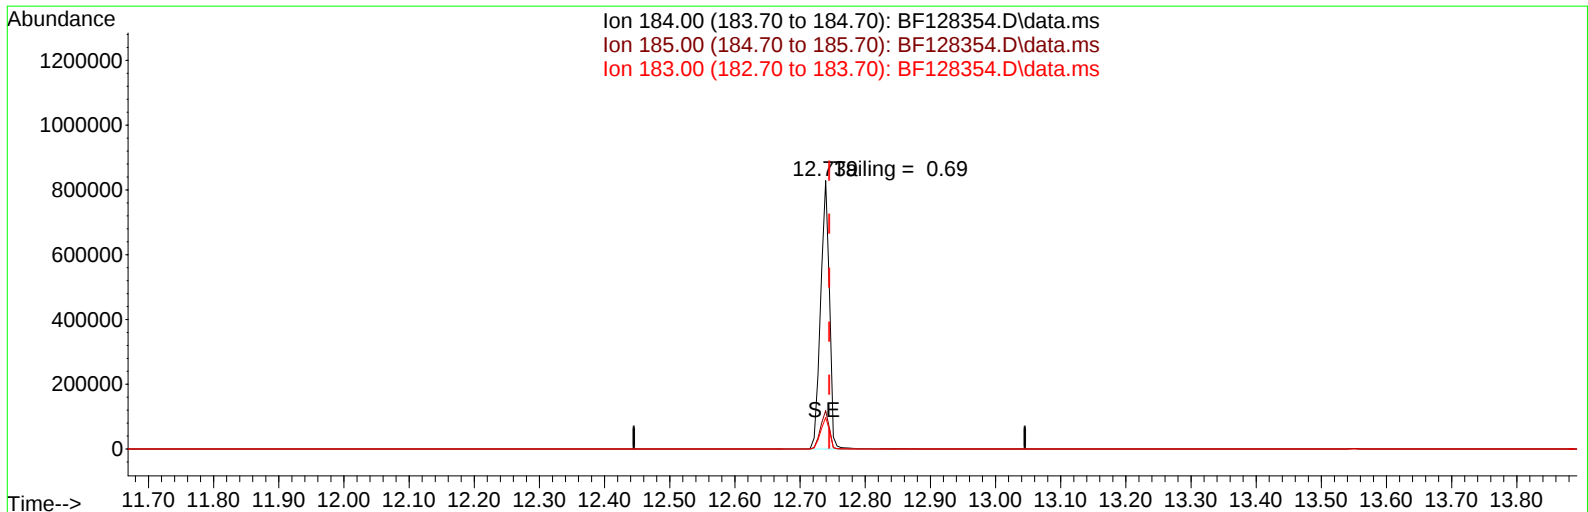

TIC: BF128354.D\data.ms

(77) Benzidine

12.739min (-0.006) 0.00 ng

response 782439

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.30
183.00	11.20	11.78
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/20/2022	BNA_F	<u>BF128354.D</u>
Compound Name	Response	Retention Time
DDT	301892	13.551
DDD	2893	13.28
DDE	673	12.922
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3566	305458	1.17

Instrument :
BNA_F
ClientSampleId :
DFTPP