
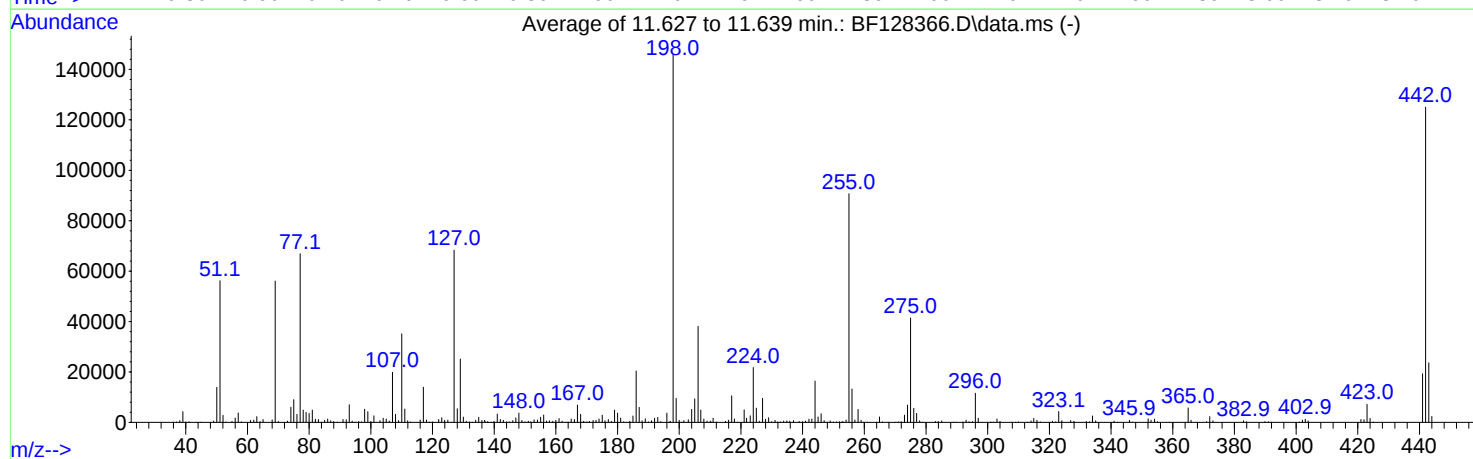


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052022\
 Data File : BF128366.D
 Acq On : 20 May 2022 16:09
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat May 21 05:28:09 2022

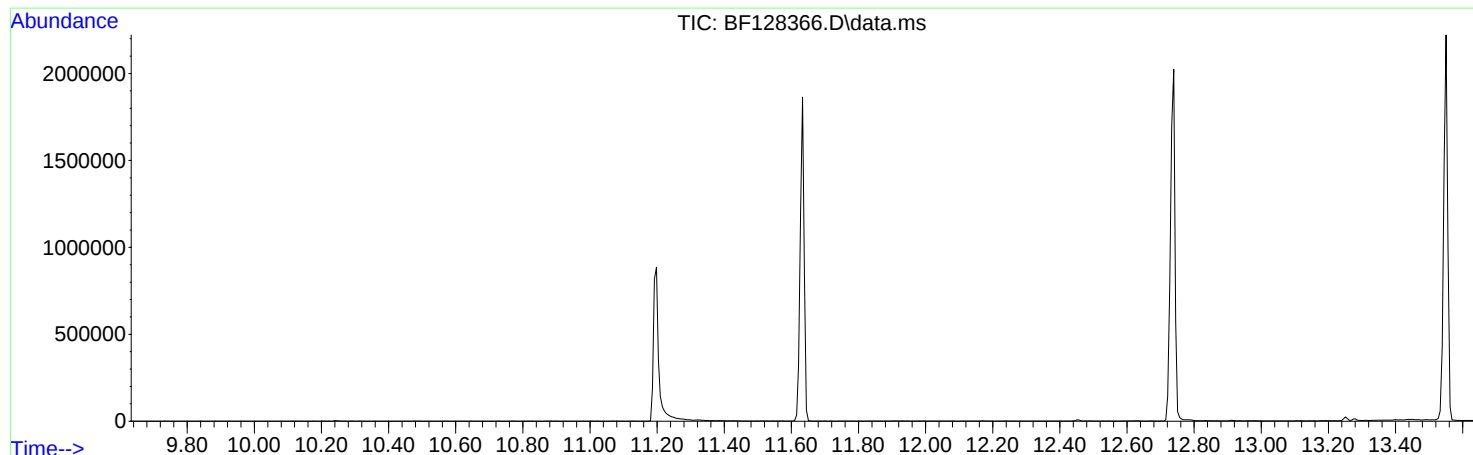




AutoFind: Scans 1588, 1589, 1590; Background Corrected with Scan 1582

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.5	56171	PASS
68	69	0.00	2	1.9	1044	PASS
69	198	0.00	100	38.4	56024	PASS
70	69	0.00	2	0.5	300	PASS
127	198	10	80	46.8	68272	PASS
197	198	0.00	2	0.3	386	PASS
198	198	100	100	100.0	145928	PASS
199	198	5	9	6.5	9506	PASS
275	198	10	60	28.4	41403	PASS
365	198	1	100	3.9	5738	PASS
441	198	0.01	100	13.2	19285	PASS
442	442	50	100	100.0	125059	PASS
443	442	15	24	18.9	23616	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052022\
Data File : BF128366.D
Acq On : 20 May 2022 16:09
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 23 04:02:35 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 21 05:28:09 2022
Response via : Initial Calibration

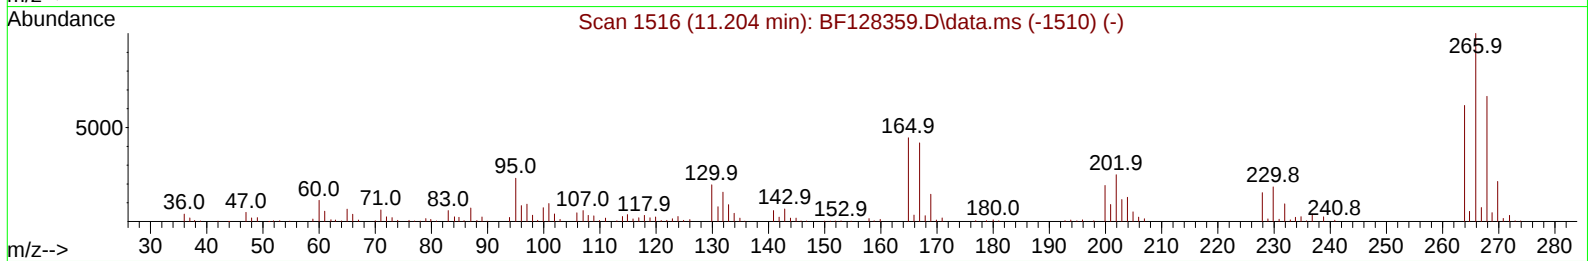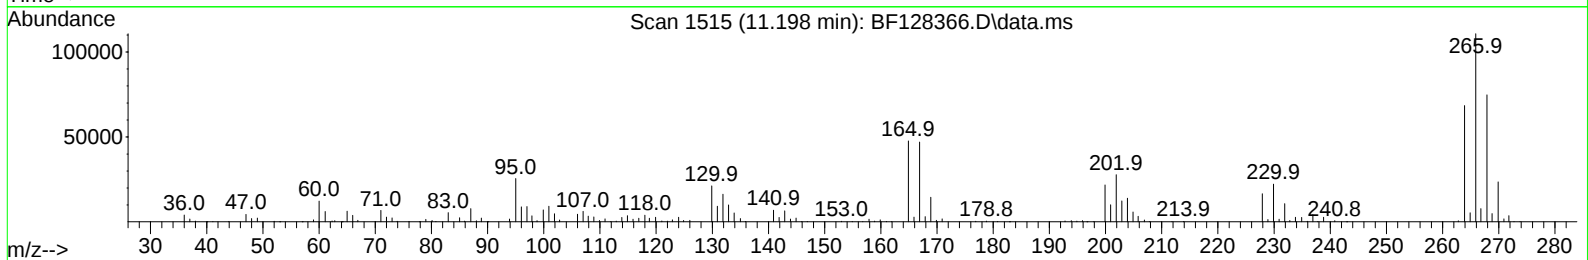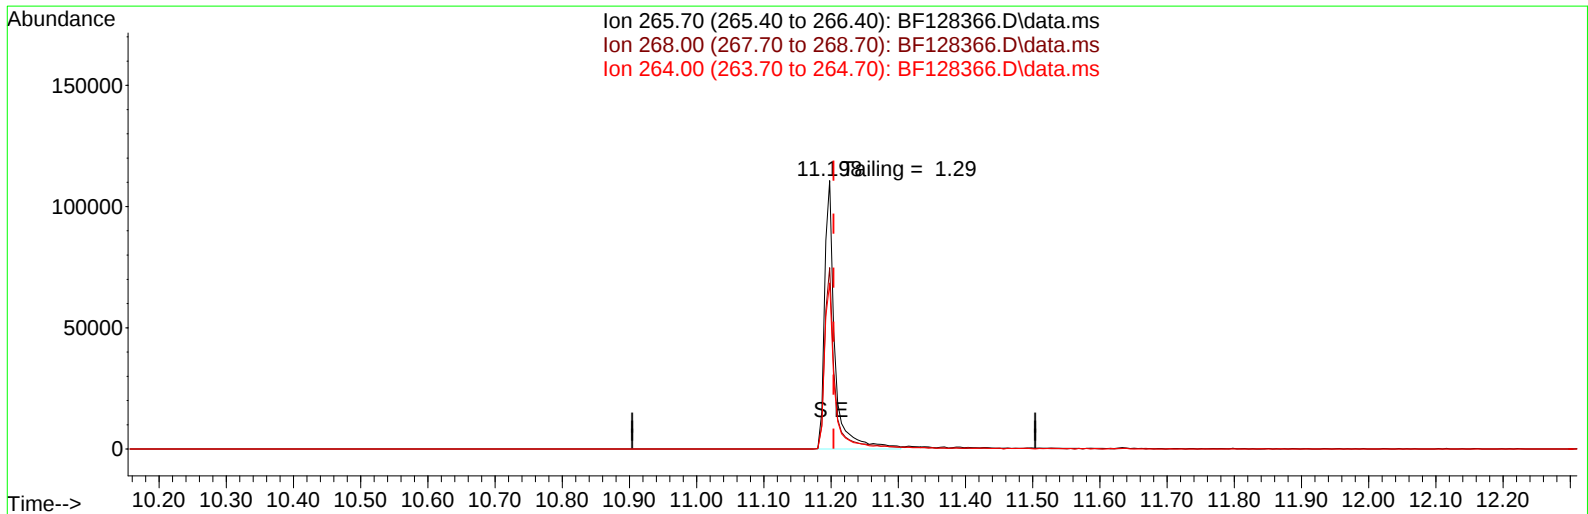

TIC: BF128366.D\data.ms

(70) Pentachlorophenol (C)

11.198min (-0.006) 38440.35 ng




response 118065

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.30	67.55
264.00	66.40	61.81
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052022\  
Data File : BF128366.D  
Acq On    : 20 May 2022  16:09  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 23 04:02:35 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 21 05:28:09 2022
Response via : Initial Calibration

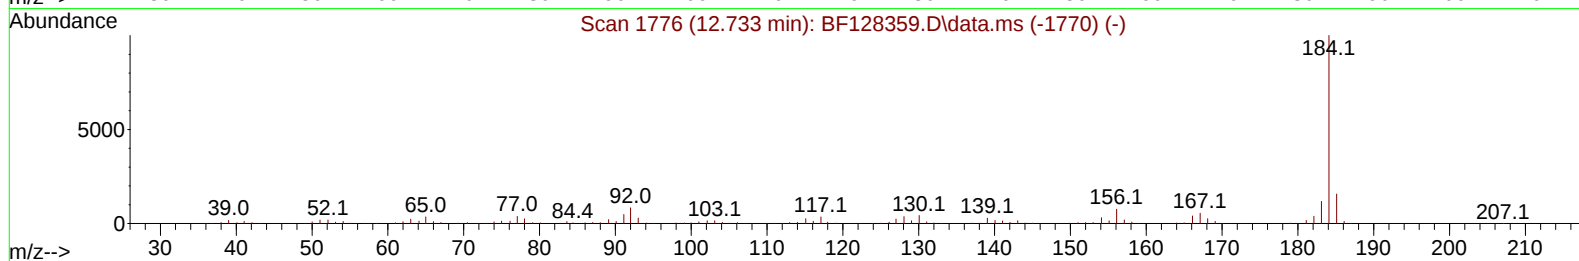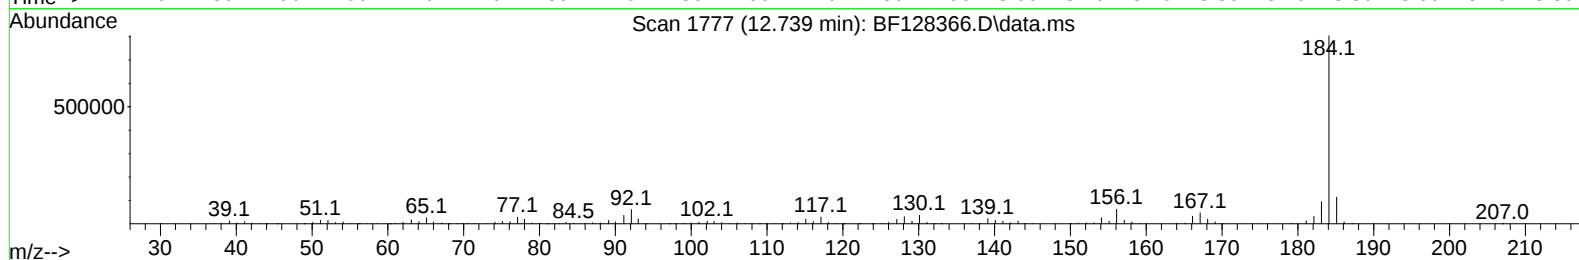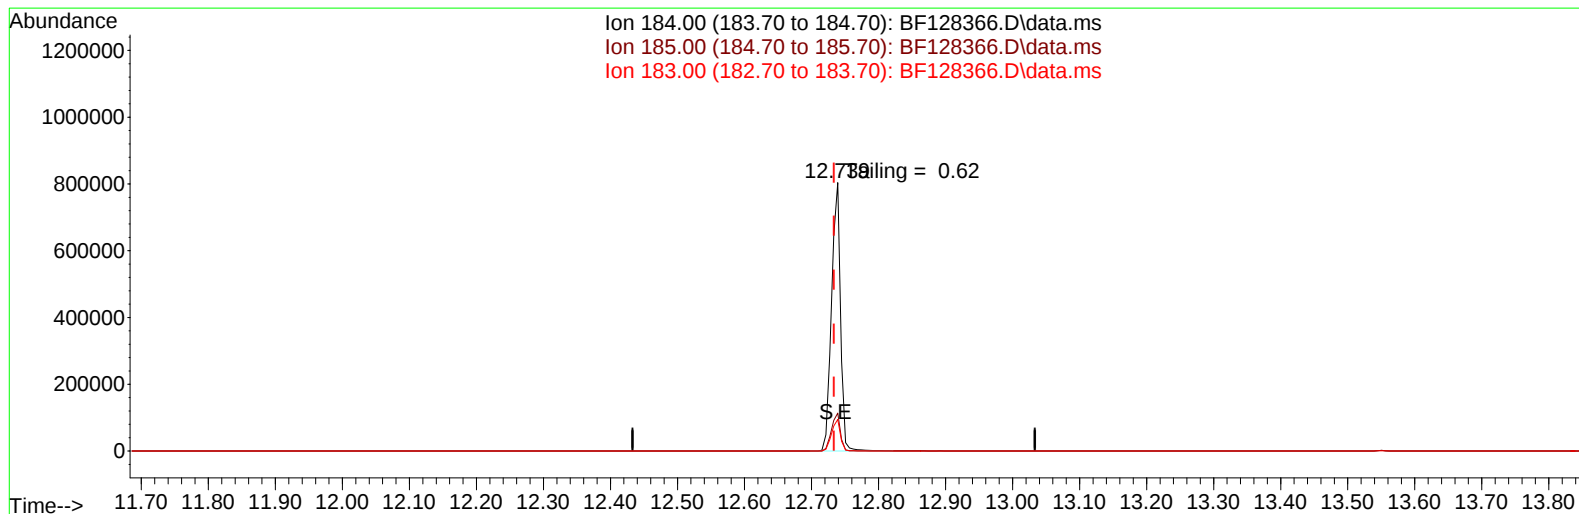

TIC: BF128366.D\data.ms

(77) Benzidine

12.739min (+ 0.006) 0.00 ng

response **747699**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.16
183.00	11.20	11.76
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/20/2022	BNA_F	<u>BF128366.D</u>
Compound Name	Response	Retention Time
DDT	363909	13.551
DDD	6819	13.251
DDE	1038	12.91
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7857	371766	2.11

Instrument :
BNA_F
ClientSampleId :
DFTPP