
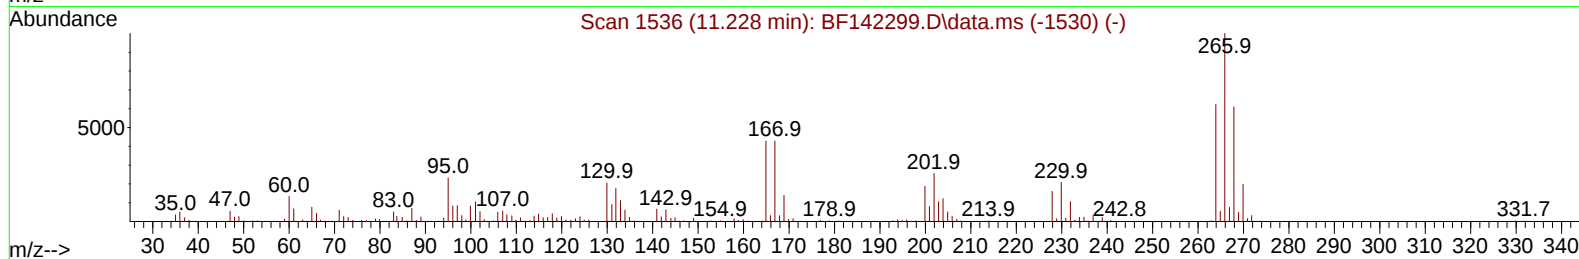
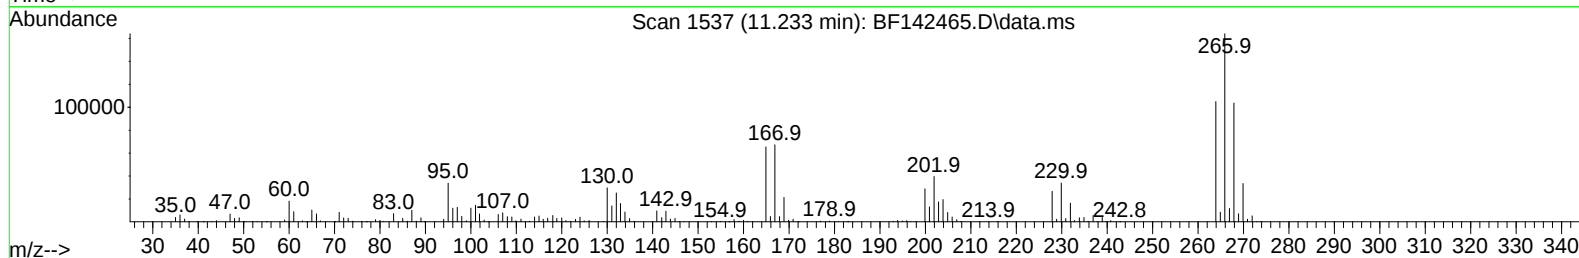


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052025\
Data File : BF142465.D
Acq On : 20 May 2025 11:13
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 20 14:09:04 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 05 18:41:44 2025
Response via : Initial Calibration

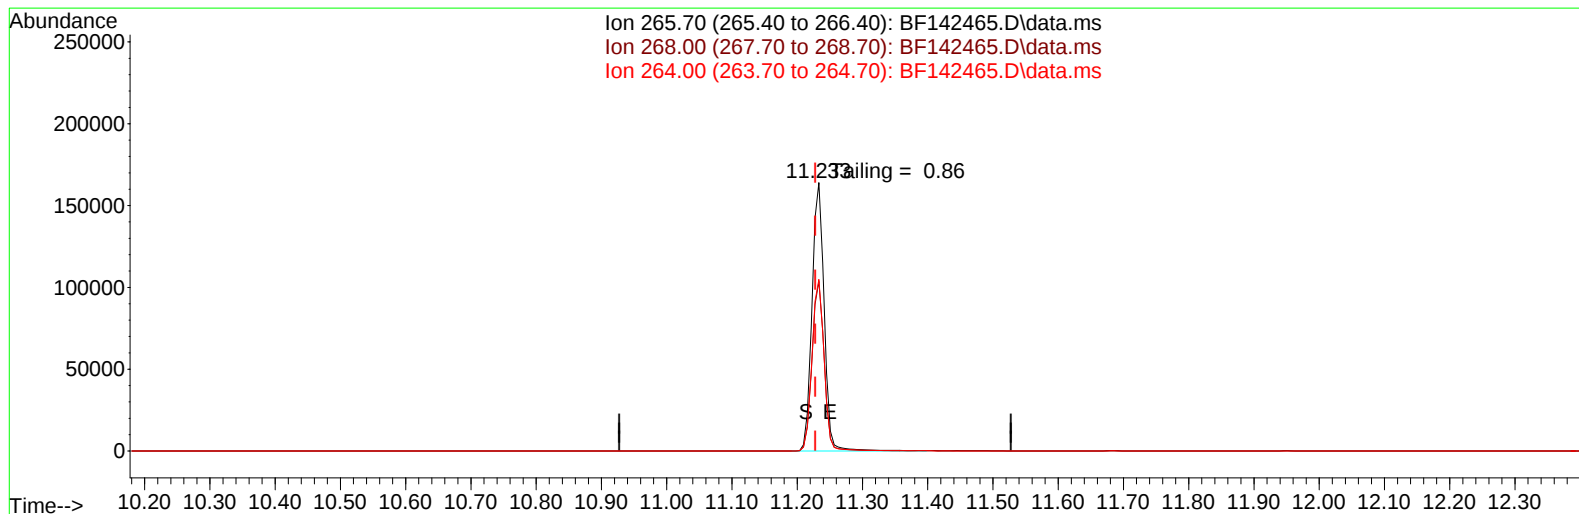

TIC: BF142465.D\data.ms




(70) Pentachlorophenol (C)

11.233min (+ 0.006) 45340.77 ng

response 213501

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	60.90	63.21
264.00	62.20	63.93
0.00	0.00	0.00

Quant Time: May 20 14:09:04 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 05 18:41:44 2025
Response via : Initial Calibration

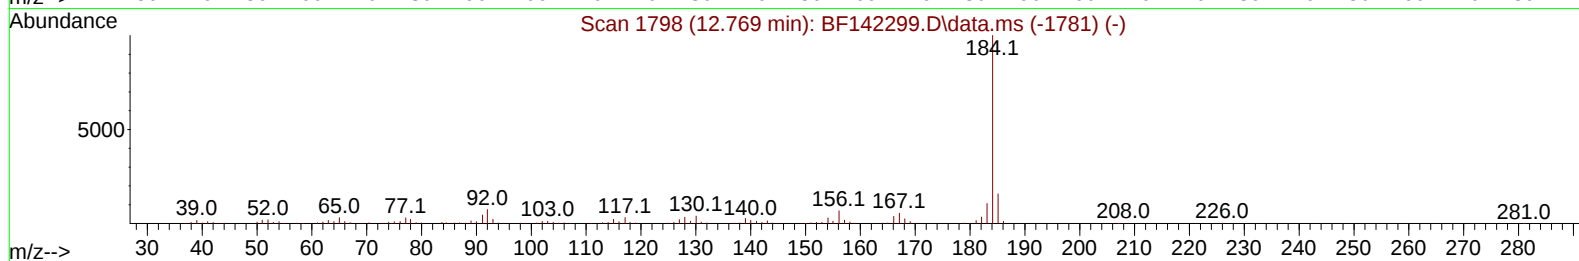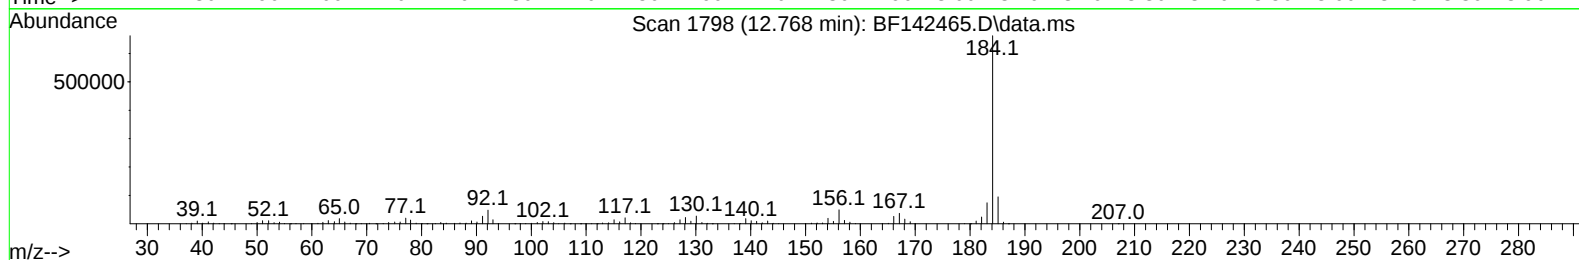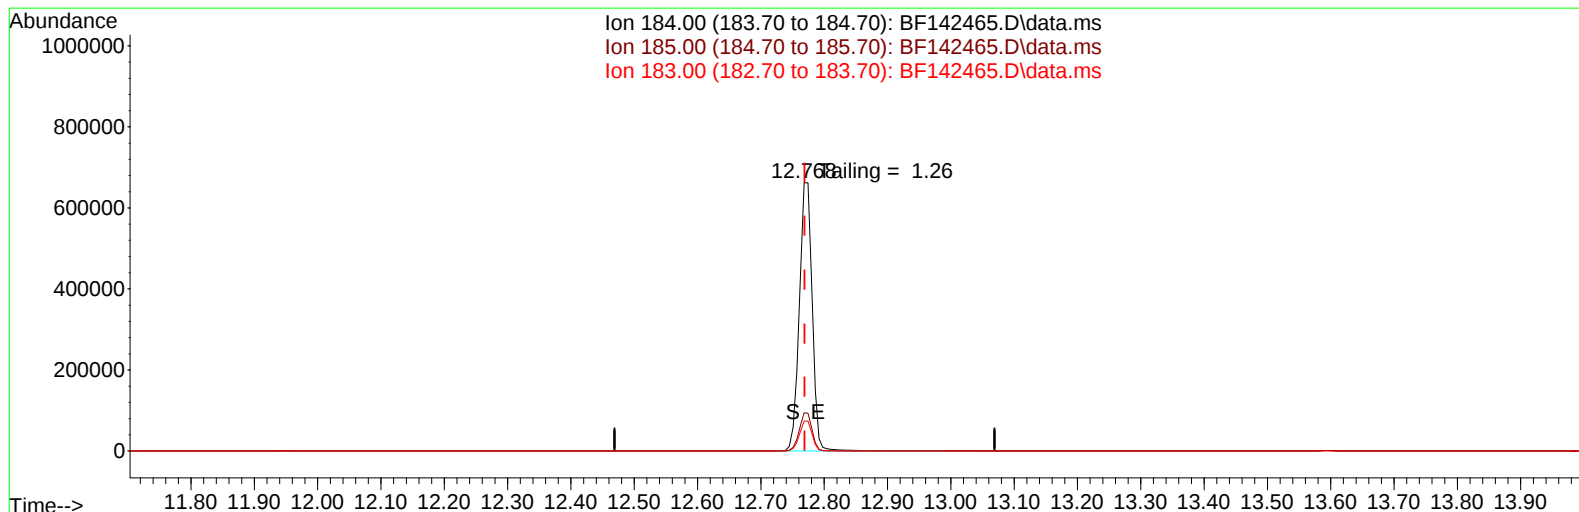

TIC: BF142465.D\data.ms

(77) Benzidine

12.768min (-0.001) 0.00 ng

response 942414

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.70	14.29
183.00	10.70	11.15
0.00	0.00	0.00