

Data Path : Z:\HPCHEM1\BNA_F\Data\BF052115\
 Data File : BF079404.D
 Acq On : 21 May 2015 15:46
 Operator : TP/IZ
 Sample : PB83521BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB83521BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF079404.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.610	35	37	46	rBV	1882633	3101334	50.13%	12.431%
2	1.724	46	47	80	rVB	3187527	6186512	100.00%	24.797%
3	4.810	316	317	323	rBV	87648	143577	2.32%	0.575%
4	5.347	362	364	367	rBV	1207771	1468390	23.74%	5.886%
5	6.650	475	478	480	rBV	1493117	1537109	24.85%	6.161%
6	6.776	487	489	492	rBV	1130818	1570623	25.39%	6.295%
7	7.073	513	515	517	rBV	362863	374848	6.06%	1.502%
8	7.256	529	531	533	rBV	1387354	1235606	19.97%	4.953%
9	7.770	573	576	578	rBV	851263	926300	14.97%	3.713%
10	8.651	651	653	655	rBV	523961	510974	8.26%	2.048%
11	9.999	768	771	773	rBV	1909590	1903953	30.78%	7.631%
12	10.822	840	843	845	rBV	450099	562130	9.09%	2.253%
13	11.794	926	928	931	rBV	1080353	1206036	19.49%	4.834%
14	12.651	1001	1003	1006	rBV	536005	604996	9.78%	2.425%
15	14.651	1175	1178	1181	rBV	2198708	2215701	35.82%	8.881%
16	15.966	1290	1293	1296	rBV	606416	688290	11.13%	2.759%
17	17.806	1451	1454	1457	rBV	542286	712601	11.52%	2.856%




Sum of corrected areas: 24948980

Data Path : Z:\HPCHEM1\BNA_F\Data\BF052115\
Data File : BF079404.D
Acq On : 21 May 2015 15:46
Operator : TP/IZ
Sample : PB83521BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB83521BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

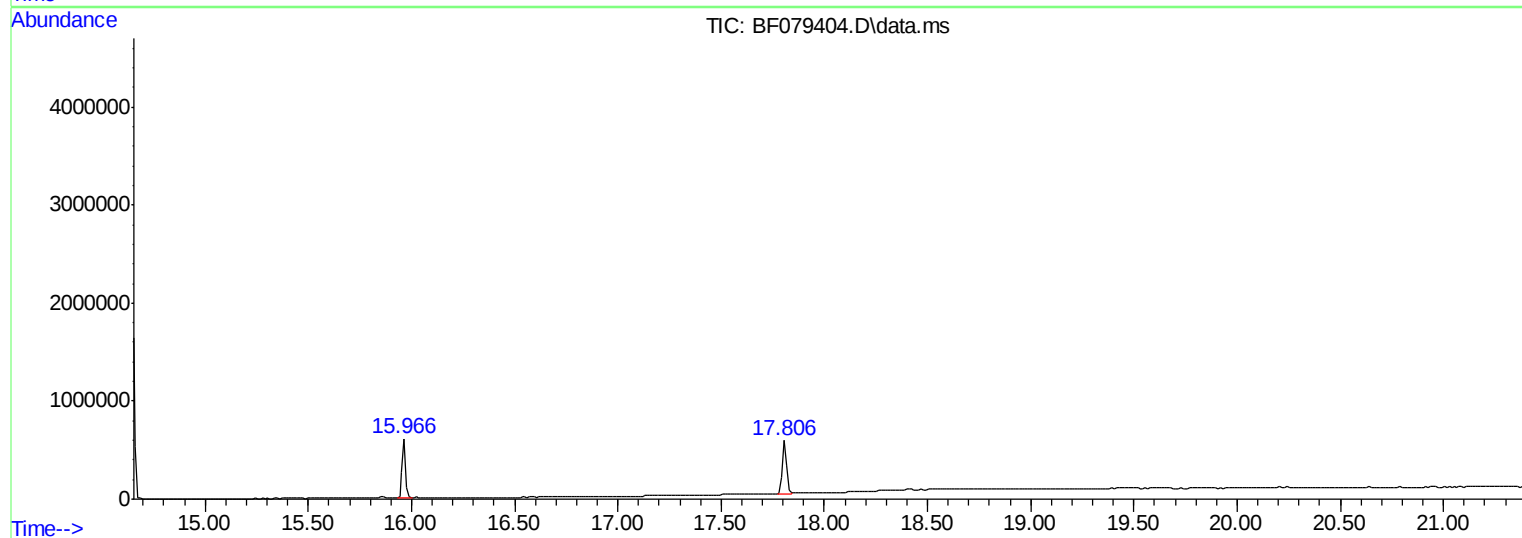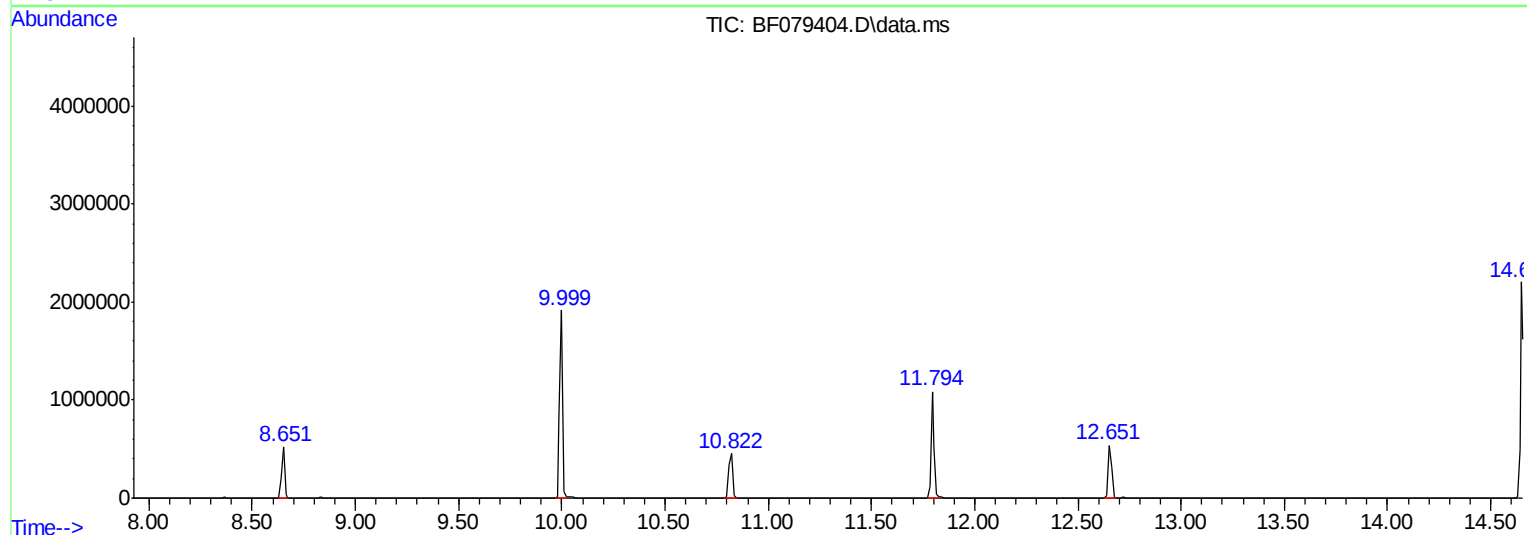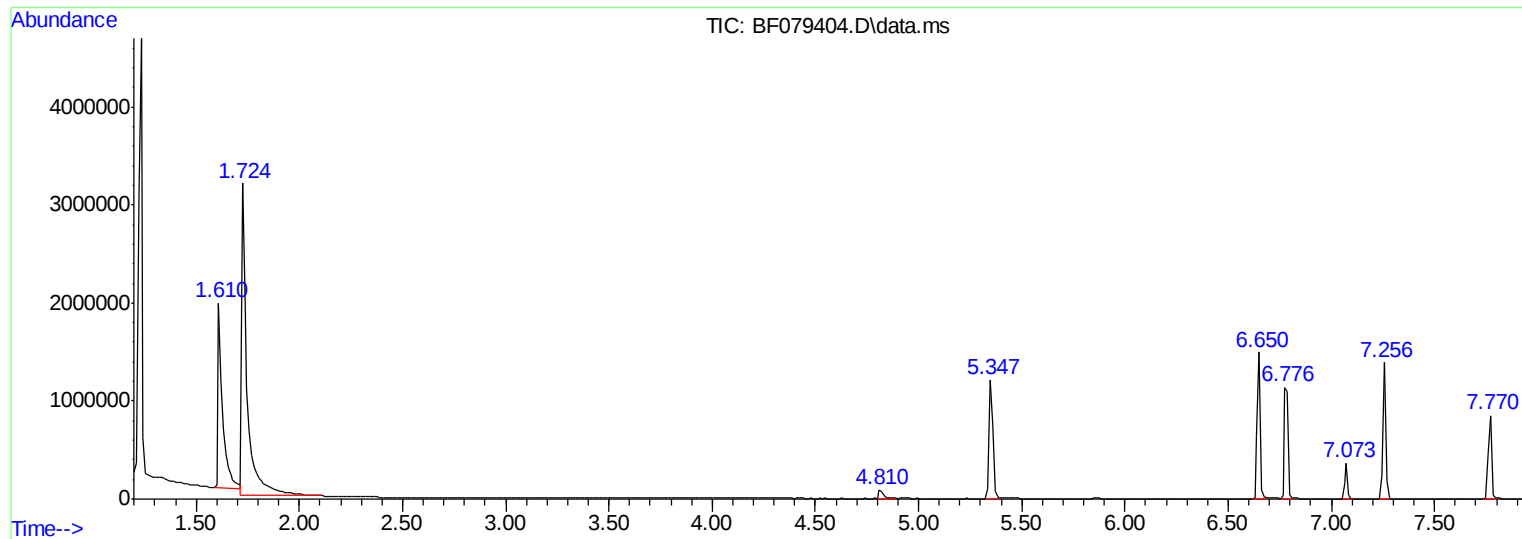

Data Path : Z:\HPCHEM1\BNA_F\Data\BF052115\
Data File : BF079404.D
Acq On : 21 May 2015 15:46
Operator : TP/IZ
Sample : PB83521BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB83521BL










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 5

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.810	7.66 ng	143577	1,4-Dichlorobenzene-d4	7.073

Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	59
2	2-Hexanol, 2-methyl-	116	C7H16O	000625-23-0	28
3	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	25
4	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	23
5	Diacetamide	101	C4H7NO2	000625-77-4	9

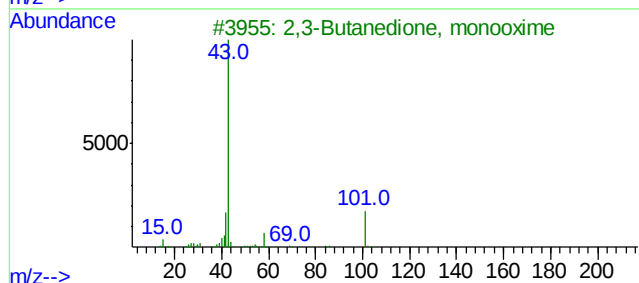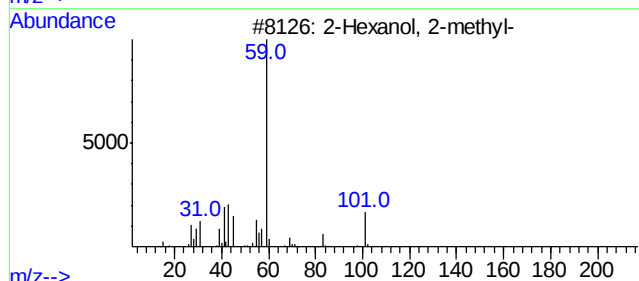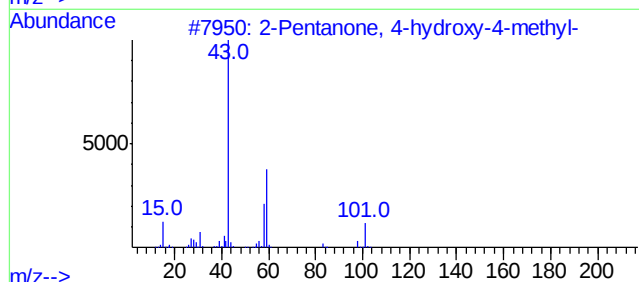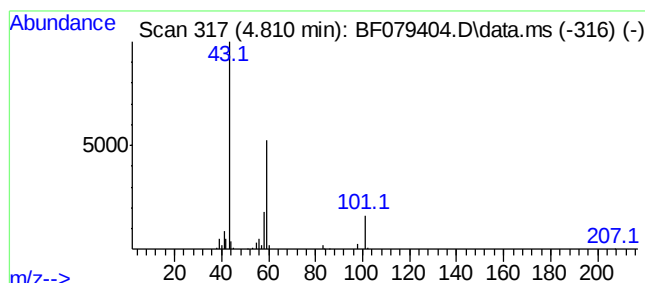

Data Path : Z:\HPCHEM1\BNA_F\Data\BF052115\
Data File : BF079404.D
Acq On : 21 May 2015 15:46
Operator : TP/IZ
Sample : PB83521BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB83521BL










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 4 unknown6.776 Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.776	83.80 ng	1570620	1,4-Dichlorobenzene-d4	7.073

Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2	5-Aminoindole	132	C8H8N2	005192-03-0	10
3	Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
4	Benzene, 1-ethenyl-3,5-dimethyl-	132	C10H12	005379-20-4	9
5	(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	9

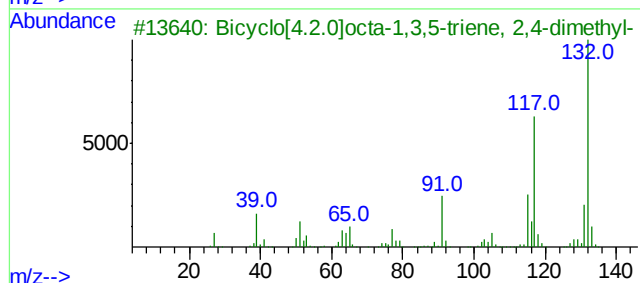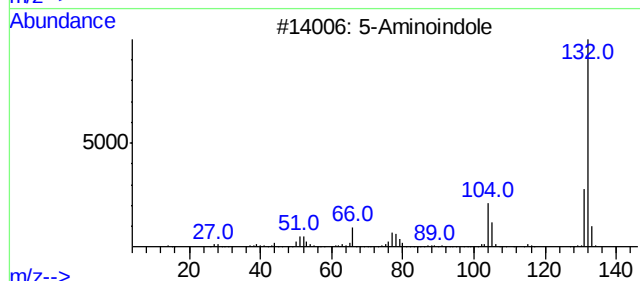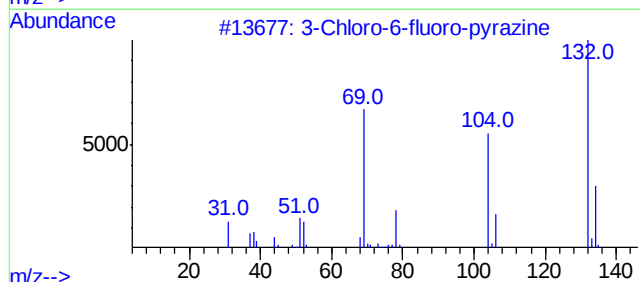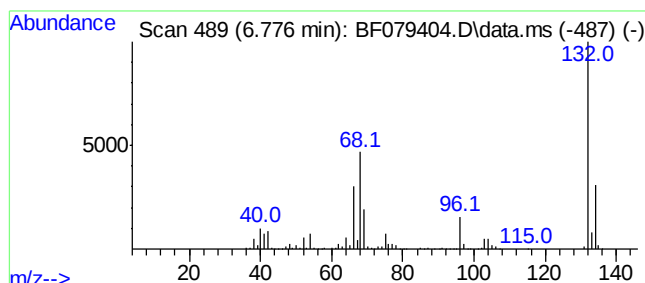

Data Path : Z:\HPCHEM1\BNA_F\Data\BF052115\
Data File : BF079404.D
Acq On : 21 May 2015 15:46
Operator : TP/IZ
Sample : PB83521BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB83521BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	4.810	7.7	ng	143577	1	7.073	374848	20.0
unknown6.776	6.776	83.8	ng	1570620	1	7.073	374848	20.0