

Data Path : Z:\HPCHEM1\BNA_F\Data\BF052115\
 Data File : BF079414.D
 Acq On : 21 May 2015 20:34
 Operator : TP/IZ
 Sample : G2325-06
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW5

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF079414.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.335	10	13	24	rVB2	272774	703824	7.32%	2.641%
2	1.495	24	27	30	rVB	693030	939861	9.77%	3.527%
3	1.610	36	37	45	rVV	622428	1047803	10.89%	3.932%
4	1.724	45	47	82	rVB	4524852	9618678	100.00%	36.091%
5	5.347	361	364	371	rBV	679190	743197	7.73%	2.789%
6	6.639	475	477	487	rBV	321749	460419	4.79%	1.728%
7	6.776	487	489	492	rBV	1345438	1453861	15.11%	5.455%
8	7.073	512	515	517	rBV	297613	341694	3.55%	1.282%
9	7.256	528	531	533	rBV	1551928	1456585	15.14%	5.465%
10	7.770	573	576	578	rBV	888862	1103491	11.47%	4.141%
11	8.650	650	653	655	rBV	378903	454327	4.72%	1.705%
12	9.999	768	771	773	rBV	1857167	2261555	23.51%	8.486%
13	10.811	840	842	845	rVB	428359	509188	5.29%	1.911%
14	11.794	925	928	931	rBV	1414902	1435034	14.92%	5.385%
15	12.651	1000	1003	1006	rBV	588679	553677	5.76%	2.077%
16	14.651	1175	1178	1180	rBV	2214819	2369682	24.64%	8.891%
17	15.954	1290	1292	1295	rBV	545156	592174	6.16%	2.222%
18	17.794	1450	1453	1456	rBV	445434	606092	6.30%	2.274%




Sum of corrected areas: 26651142

Data Path : Z:\HPCHEM1\BNA_F\Data\BF052115\
Data File : BF079414.D
Acq On : 21 May 2015 20:34
Operator : TP/IZ
Sample : G2325-06
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW5

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

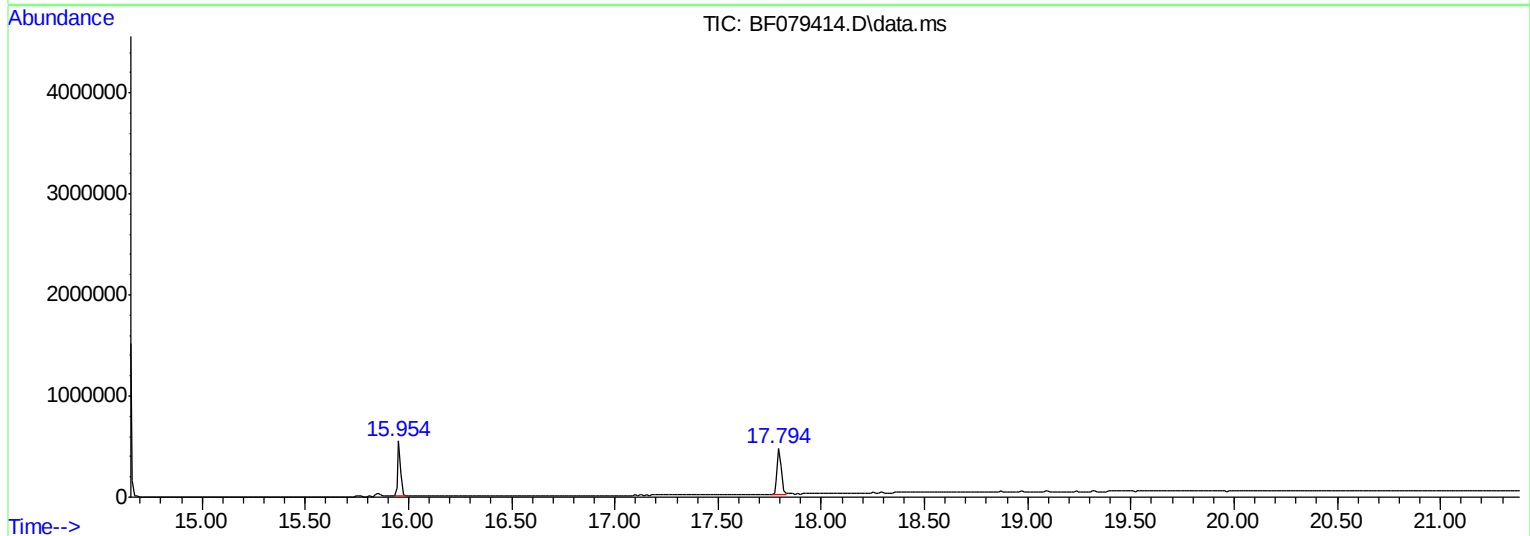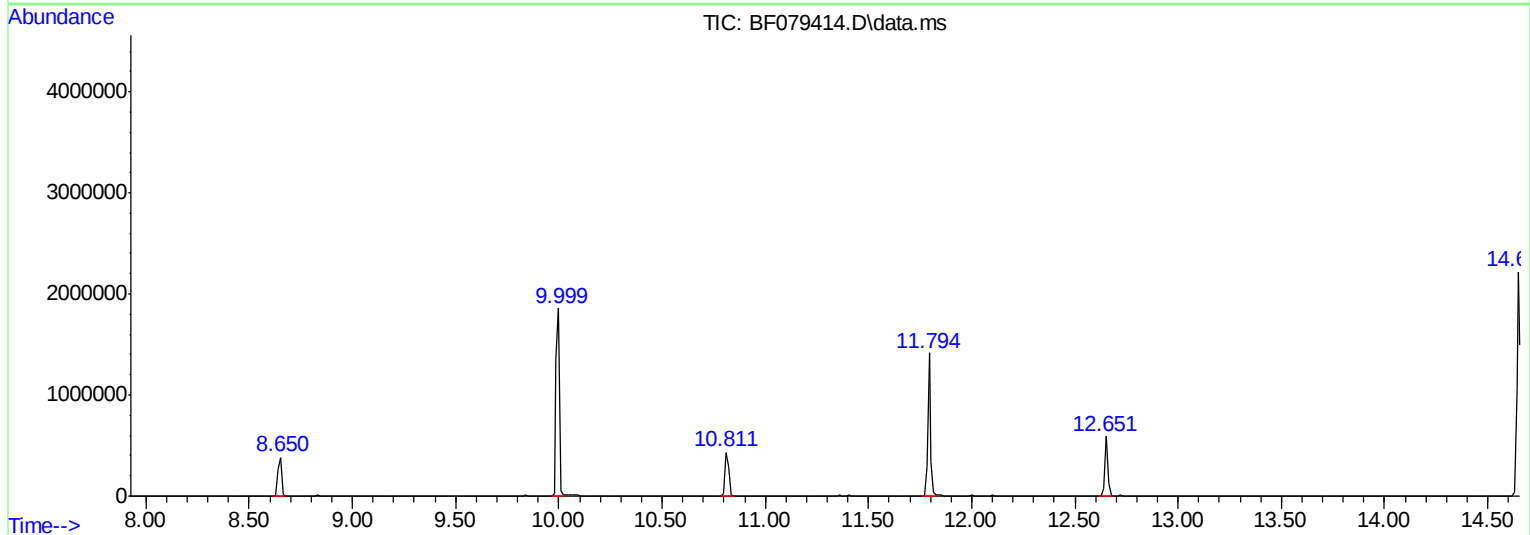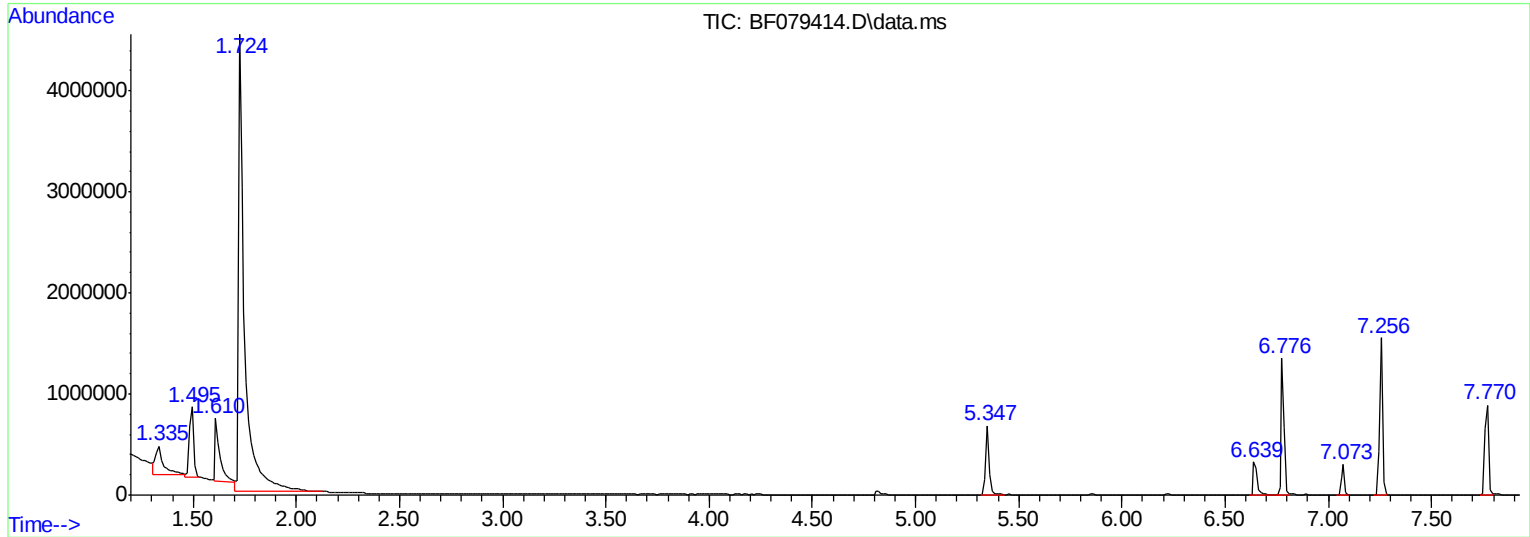

Data Path : Z:\HPCHEM1\BNA_F\Data\BF052115\
Data File : BF079414.D
Acq On : 21 May 2015 20:34
Operator : TP/IZ
Sample : G2325-06
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW5










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Butane, 2-methoxy-2-methyl- Concentration Rank 5

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.495	55.01 ng	939861	1,4-Dichlorobenzene-d4	7.073

Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
2	1,3-Dioxolane, 2-methyl-	88	C4H8O2	000497-26-7	25
3	Pentane, 3-methoxy-	102	C6H14O	036839-67-5	17
4	Silane, tetramethyl-	88	C4H12Si	000075-76-3	12
5	Borane, dimethoxy-	74	C2H7BO2	004542-61-4	9

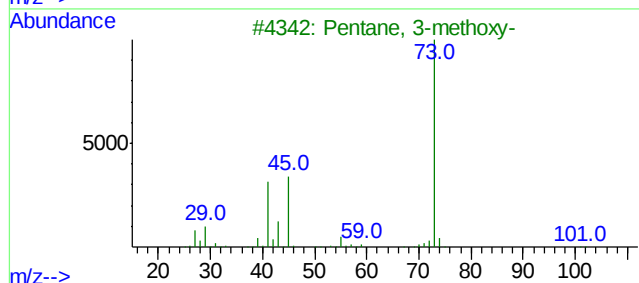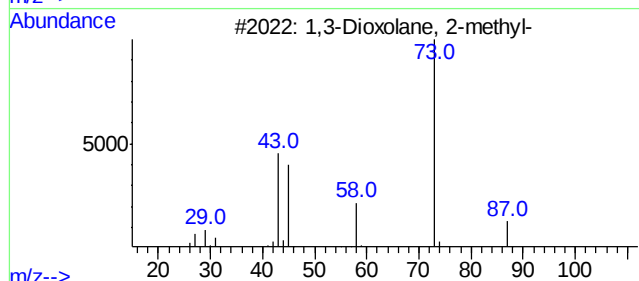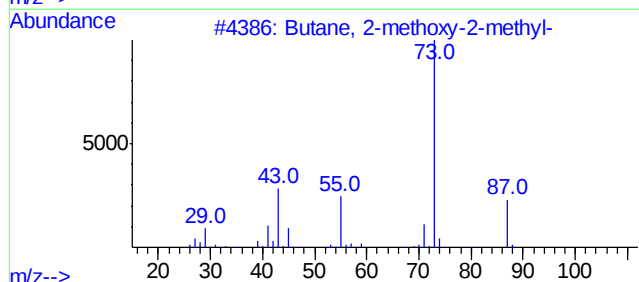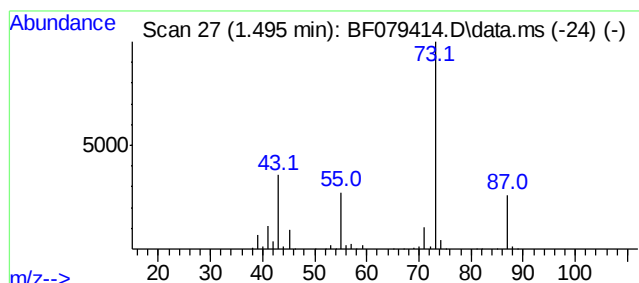

Data Path : Z:\HPCHEM1\BNA_F\Data\BF052115\
Data File : BF079414.D
Acq On : 21 May 2015 20:34
Operator : TP/IZ
Sample : G2325-06
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW5










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 5 unknown6.776 Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.776	85.10 ng	1453860	1,4-Dichlorobenzene-d4	7.073

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2			Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
3			1,3,4-Thiadiazole-2(3H)-thione, ...	132	C3H4N2S2	029490-19-5	9
4			5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9
5			(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	9

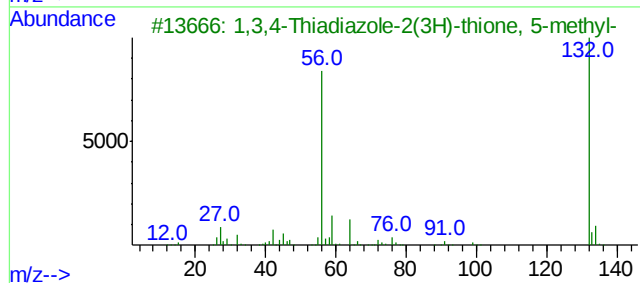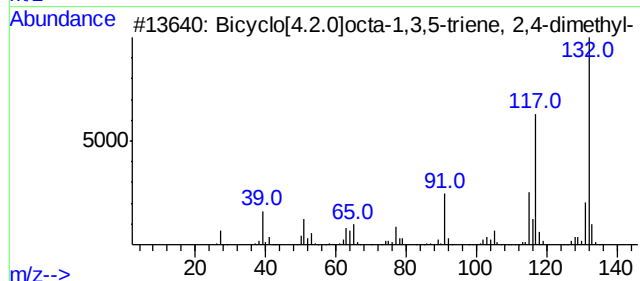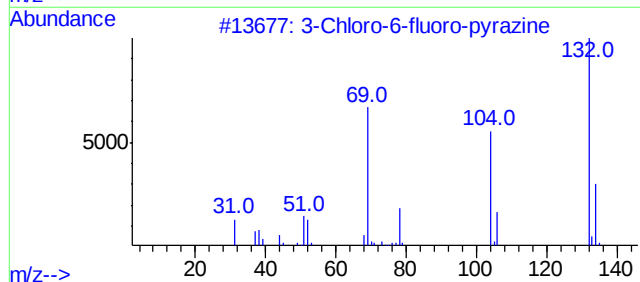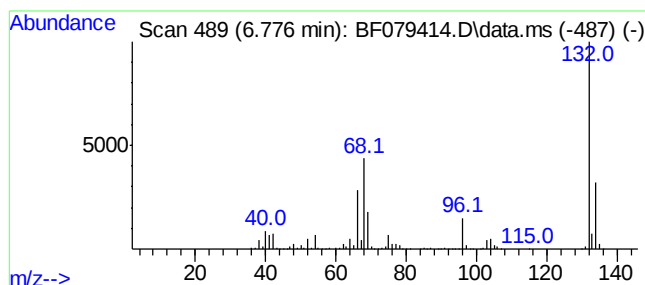

Data Path : Z:\HPCHEM1\BNA_F\Data\BF052115\
Data File : BF079414.D
Acq On : 21 May 2015 20:34
Operator : TP/IZ
Sample : G2325-06
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW5

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	1.495	55.0	ng	939861	1	7.073	341694	20.0
unknown6.776	6.776	85.1	ng	1453860	1	7.073	341694	20.0