

Data Path : Z:\HPCHEM1\BNA_F\Data\BF052115\
 Data File : BF079416.D
 Acq On : 21 May 2015 21:31
 Operator : TP/IZ
 Sample : G2325-09
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW18

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF079416.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.335	10	13	24	rVB2	256108	619329	7.33%	2.385%
2	1.495	24	27	30	rVB	720745	892670	10.57%	3.438%
3	1.610	36	37	45	rVV	430277	790690	9.36%	3.045%
4	1.724	45	47	95	rVB	3970634	8447472	100.00%	32.534%
5	5.347	361	364	372	rBV	766881	835312	9.89%	3.217%
6	6.639	475	477	480	rBV	465850	526526	6.23%	2.028%
7	6.776	487	489	492	rBV	1469572	1570923	18.60%	6.050%
8	7.073	512	515	517	rBV	288946	335532	3.97%	1.292%
9	7.256	528	531	533	rBV	1681276	1537642	18.20%	5.922%
10	7.770	573	576	578	rBV	977641	1181059	13.98%	4.549%
11	8.650	650	653	655	rBV	379626	451608	5.35%	1.739%
12	9.999	768	771	773	rBV	1860566	2405804	28.48%	9.266%
13	10.811	840	842	845	rVB	465686	508009	6.01%	1.957%
14	11.793	925	928	931	rBV	1527036	1546531	18.31%	5.956%
15	12.651	1000	1003	1006	rBV	572962	545993	6.46%	2.103%
16	14.651	1175	1178	1180	rBV	2170121	2591364	30.68%	9.980%
17	15.931	1288	1290	1293	rBV	463857	578648	6.85%	2.229%
18	17.691	1442	1444	1450	rBV	382170	599951	7.10%	2.311%




Sum of corrected areas: 25965063

Data Path : Z:\HPCHEM1\BNA_F\Data\BF052115\
Data File : BF079416.D
Acq On : 21 May 2015 21:31
Operator : TP/IZ
Sample : G2325-09
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW18

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

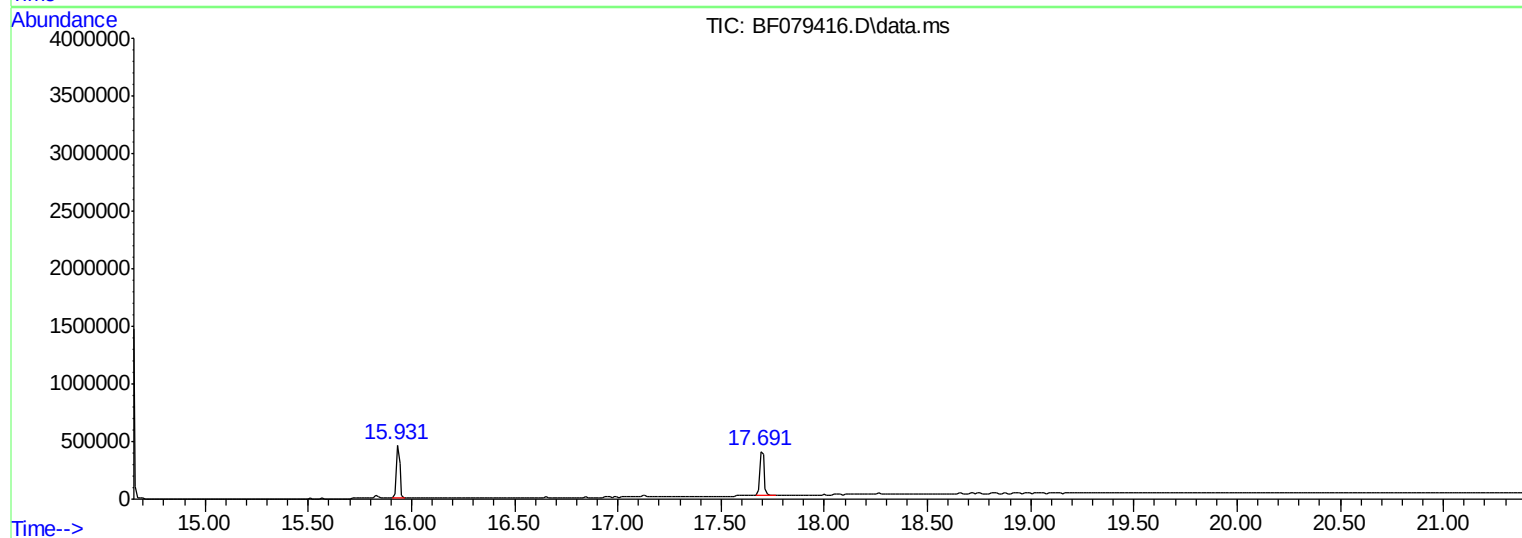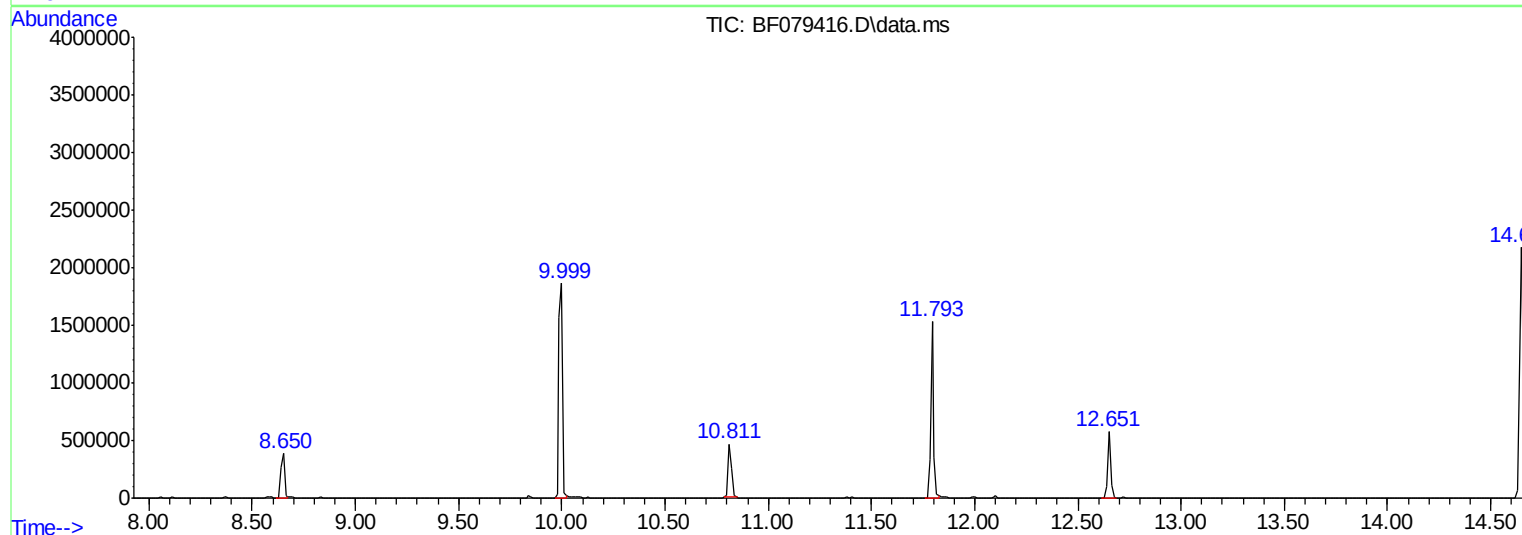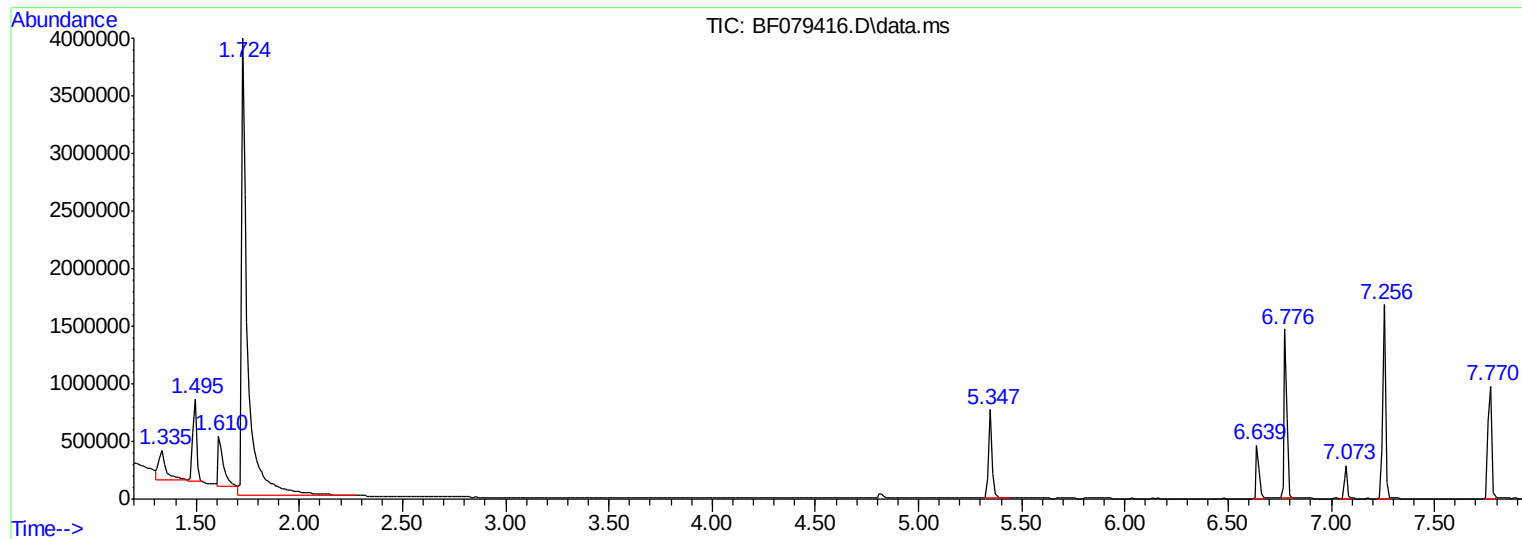

Data Path : Z:\HPCHEM1\BNA_F\Data\BF052115\
Data File : BF079416.D
Acq On : 21 May 2015 21:31
Operator : TP/IZ
Sample : G2325-09
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW18










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Butane, 2-methoxy-2-methyl- Concentration Rank 4

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.495	53.21 ng	892670	1,4-Dichlorobenzene-d4	7.073

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
2			1,3-Dioxolane, 2-methyl-	88	C4H8O2	000497-26-7	25
3			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	17
4			Silane, tetramethyl-	88	C4H12Si	000075-76-3	12
5			Borane, dimethoxy-	74	C2H7BO2	004542-61-4	9

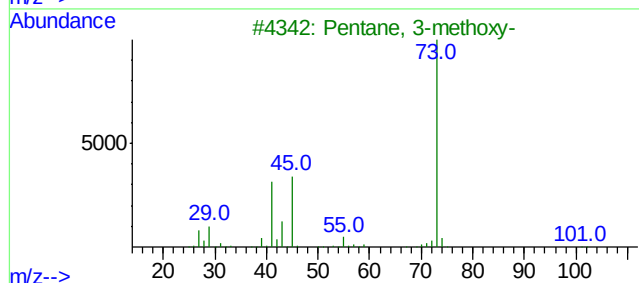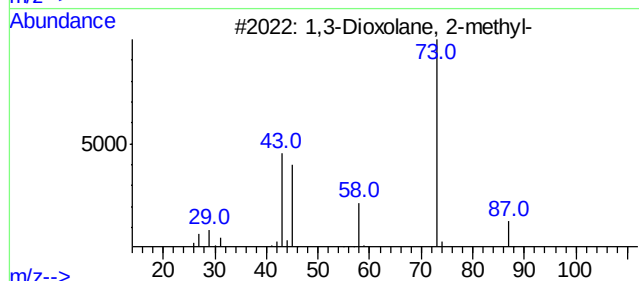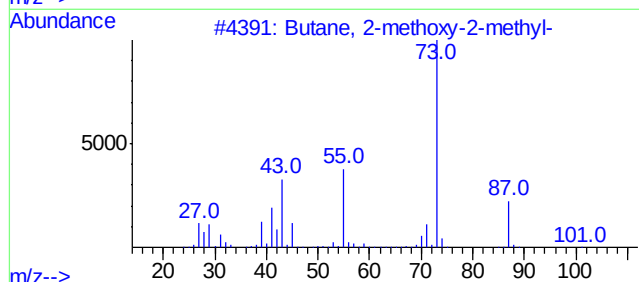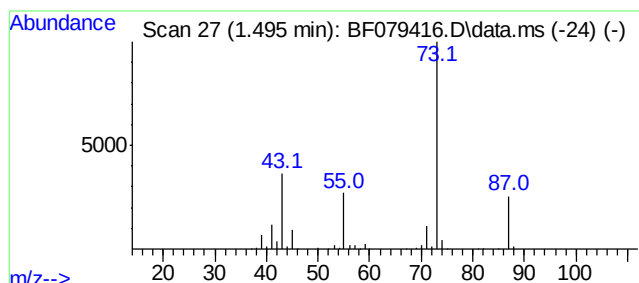

Data Path : Z:\HPCHEM1\BNA_F\Data\BF052115\
Data File : BF079416.D
Acq On : 21 May 2015 21:31
Operator : TP/IZ
Sample : G2325-09
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW18










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 5 unknown6.776 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.776	93.64 ng	1570920	1,4-Dichlorobenzene-d4	7.073

Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2	5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	16
3	5-Aminoindole	132	C8H8N2	005192-03-0	12
4	(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	9
5	Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9

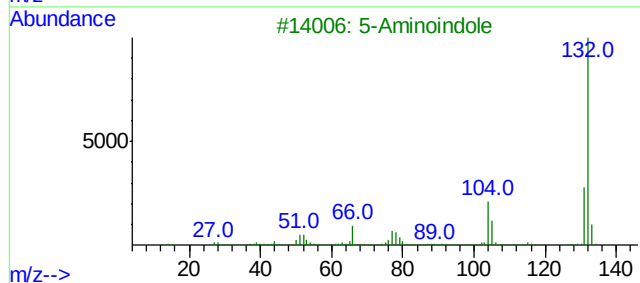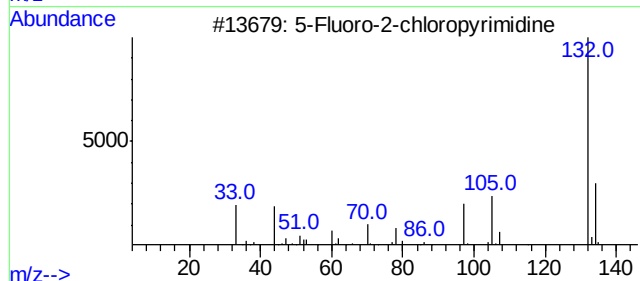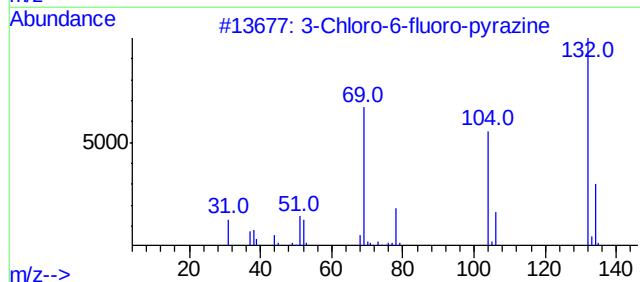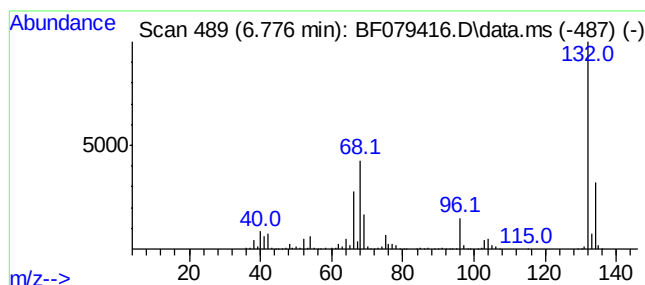

Data Path : Z:\HPCHEM1\BNA_F\Data\BF052115\
Data File : BF079416.D
Acq On : 21 May 2015 21:31
Operator : TP/IZ
Sample : G2325-09
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW18

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	1.495	53.2	ng	892670	1	7.073	335532	20.0
unknown6.776	6.776	93.6	ng	1570920	1	7.073	335532	20.0