

Data Path : Z:\HPCHEM1\BNA_F\Data\BF052115\
 Data File : BF079418.D
 Acq On : 21 May 2015 22:29
 Operator : TP/IZ
 Sample : PB83529BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB83529BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF079418.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.610	35	37	46	rBV	1644274	2751845	49.26%	11.460%
2	1.724	46	47	84	rVB	2825263	5586572	100.00%	23.265%
3	4.810	316	317	323	rBV	92091	150407	2.69%	0.626%
4	5.347	362	364	367	rBV	1415610	1519855	27.21%	6.329%
5	6.639	475	477	480	rBV	1118932	1506975	26.97%	6.276%
6	6.776	487	489	492	rBV	1547650	1617391	28.95%	6.736%
7	7.073	512	515	517	rBV	296439	341884	6.12%	1.424%
8	7.256	528	531	533	rBV	1386643	1307366	23.40%	5.444%
9	7.759	573	575	578	rBV	661908	945906	16.93%	3.939%
10	8.650	650	653	655	rBV	373418	461474	8.26%	1.922%
11	9.999	768	771	773	rBV	1404382	1947855	34.87%	8.112%
12	10.811	840	842	845	rBV	440346	513882	9.20%	2.140%
13	11.794	925	928	931	rBV	1276616	1276607	22.85%	5.316%
14	12.651	1001	1003	1006	rBV	578365	555129	9.94%	2.312%
15	14.651	1175	1178	1180	rBV	2113154	2332317	41.75%	9.713%
16	15.943	1288	1291	1293	rBV	405282	591210	10.58%	2.462%
17	17.703	1443	1445	1448	rBV	449911	606213	10.85%	2.525%




Sum of corrected areas: 24012888

Data Path : Z:\HPCHEM1\BNA_F\Data\BF052115\
Data File : BF079418.D
Acq On : 21 May 2015 22:29
Operator : TP/IZ
Sample : PB83529BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB83529BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

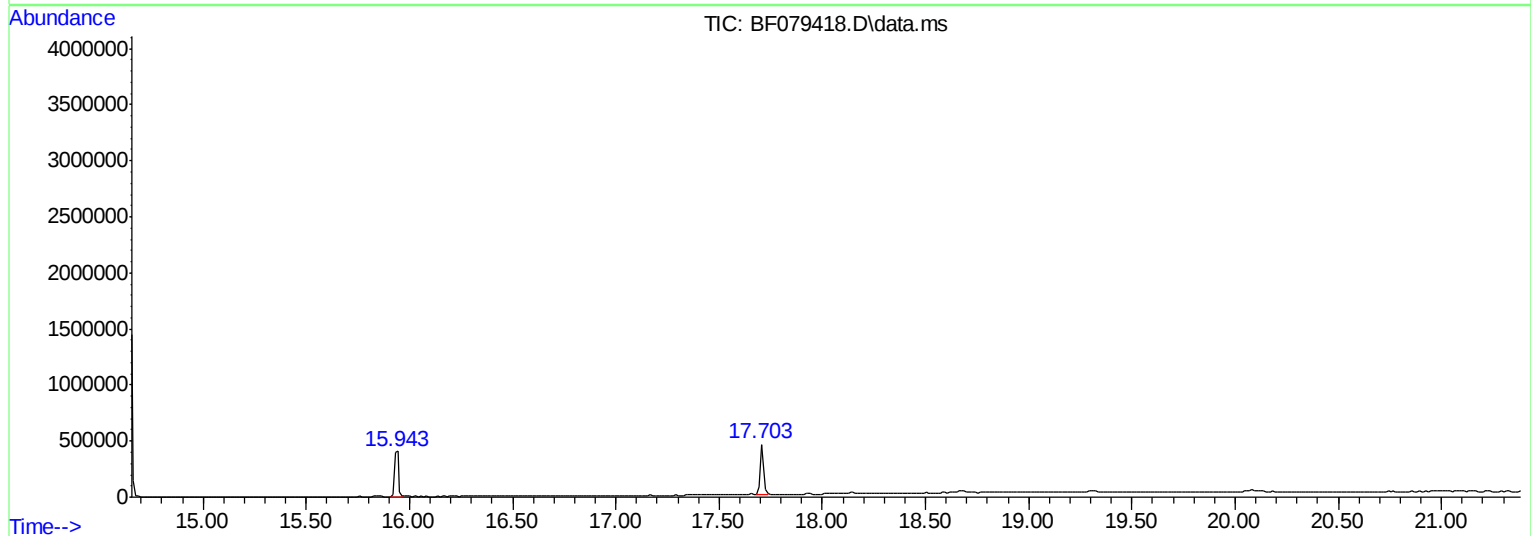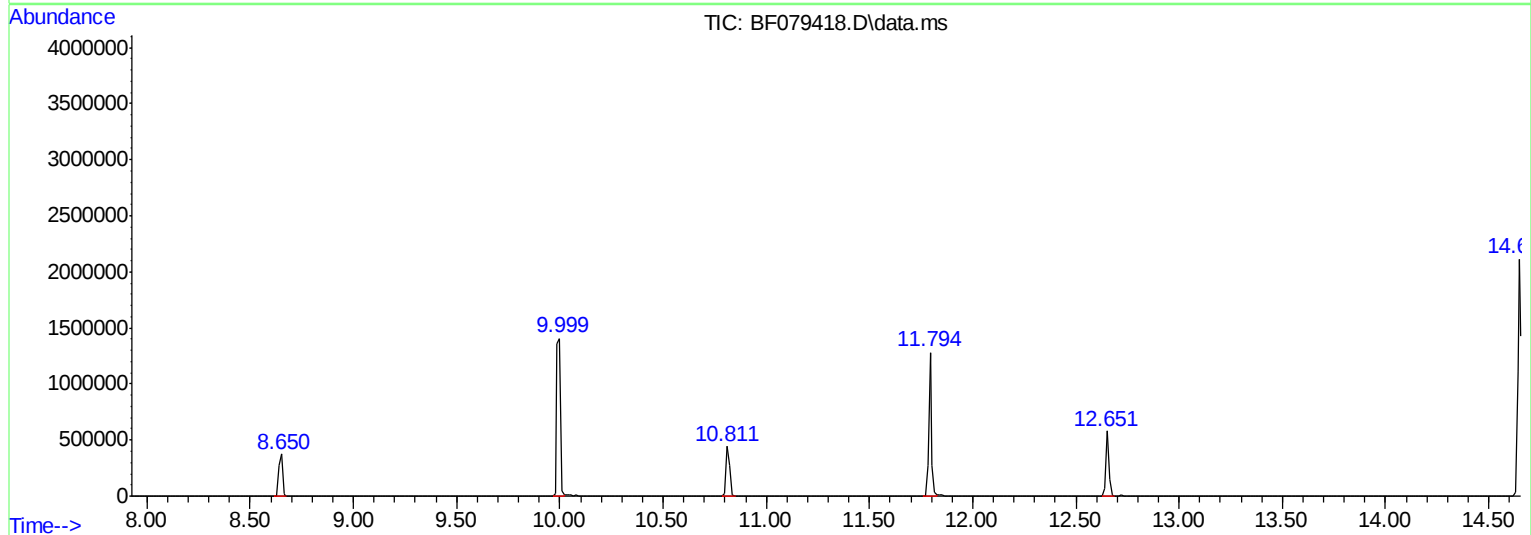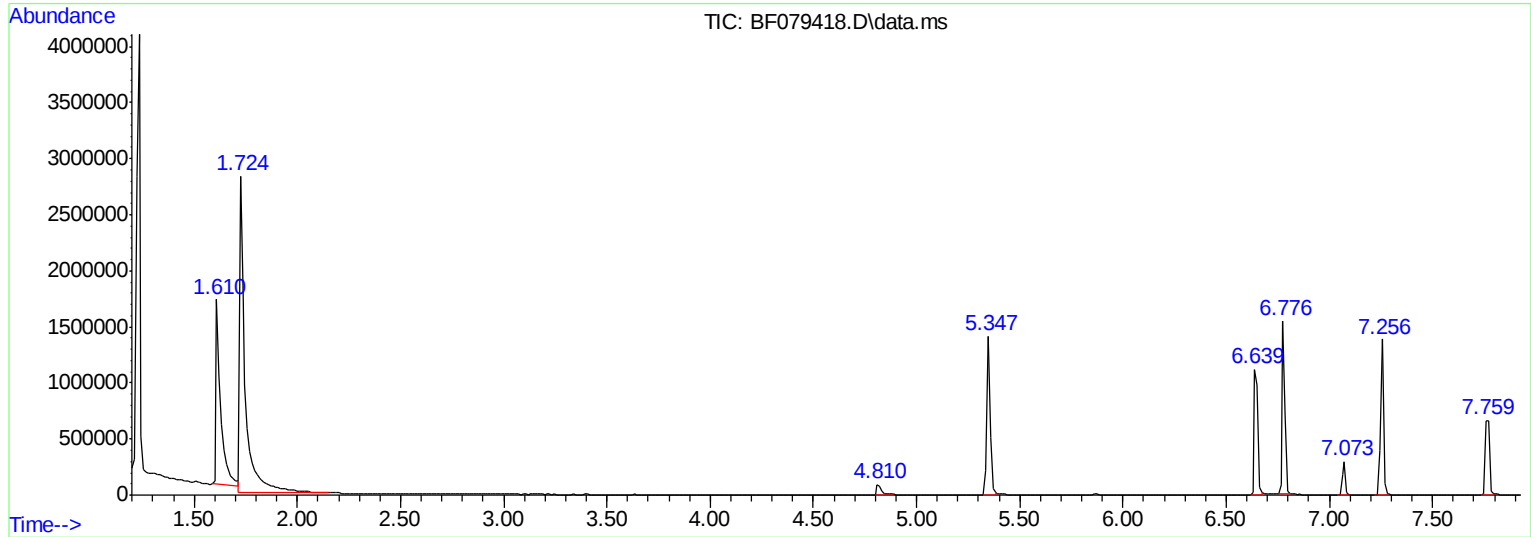

Data Path : Z:\HPCHEM1\BNA_F\Data\BF052115\
Data File : BF079418.D
Acq On : 21 May 2015 22:29
Operator : TP/IZ
Sample : PB83529BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB83529BL










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 5

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.810	8.80 ng	150407	1,4-Dichlorobenzene-d4	7.073

Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	64
2	Hydrazine, 1,1-bis(1-methylethyl)-	116	C6H16N2	000921-14-2	38
3	Butyl aldoxime, 3-methyl-, syn-	101	C5H11NO	005780-40-5	32
4	3-Hexanol, 4-methyl-	116	C7H16O	000615-29-2	28
5	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	25

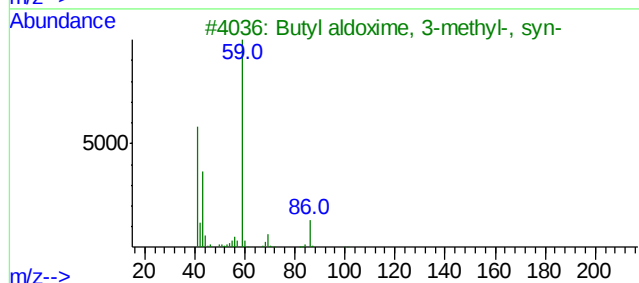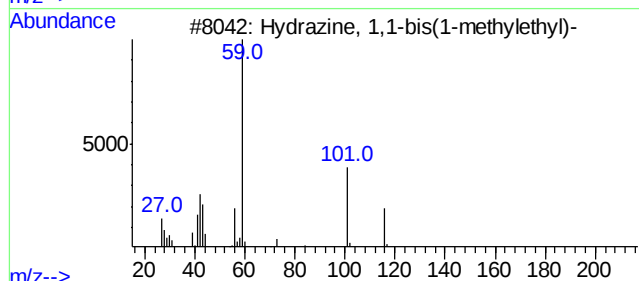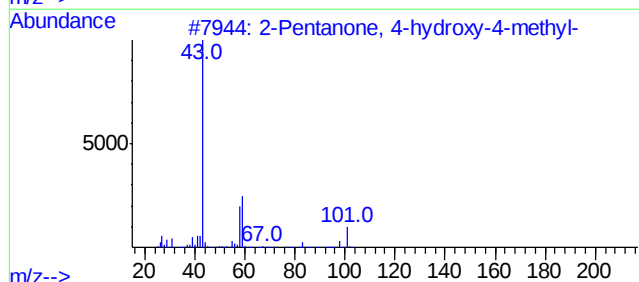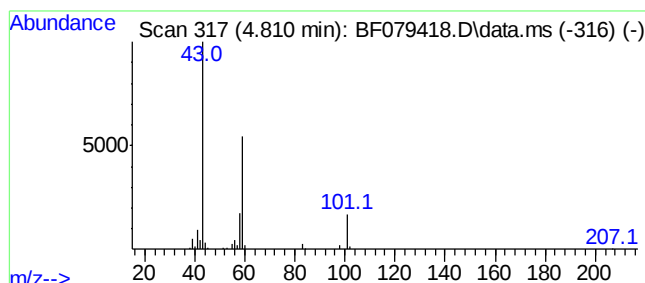

Data Path : Z:\HPCHEM1\BNA_F\Data\BF052115\
Data File : BF079418.D
Acq On : 21 May 2015 22:29
Operator : TP/IZ
Sample : PB83529BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB83529BL










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 4 unknown6.776 Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.776	94.62 ng	1617390	1,4-Dichlorobenzene-d4	7.073

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2			(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	9
3			Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
4			5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9
5			4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9

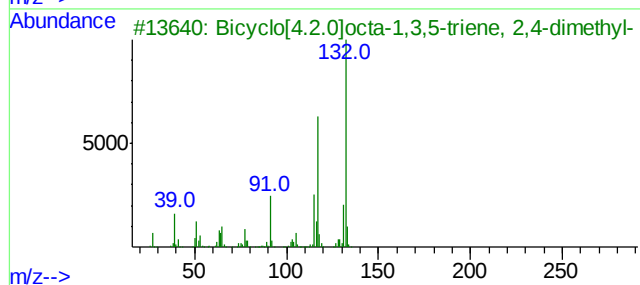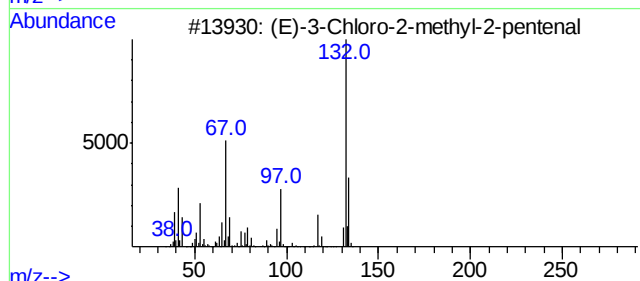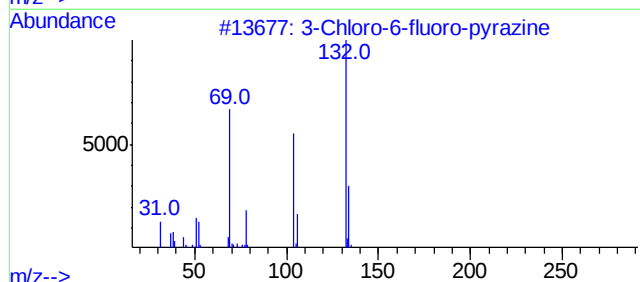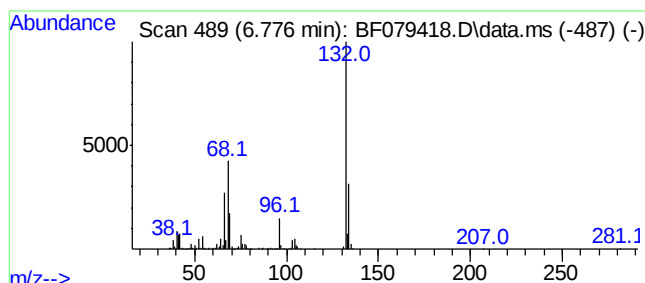

Data Path : Z:\HPCHEM1\BNA_F\Data\BF052115\
Data File : BF079418.D
Acq On : 21 May 2015 22:29
Operator : TP/IZ
Sample : PB83529BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB83529BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	4.810	8.8	ng	150407	1	7.073	341884	20.0
unknown6.776	6.776	94.6	ng	1617390	1	7.073	341884	20.0