


Data Path : Z:\HPCHEM1\BNA F\Data\BF052115\
 Data File : BF079401.D
 Acq On : 21 May 2015 13:20
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 20 05:08:22 2015

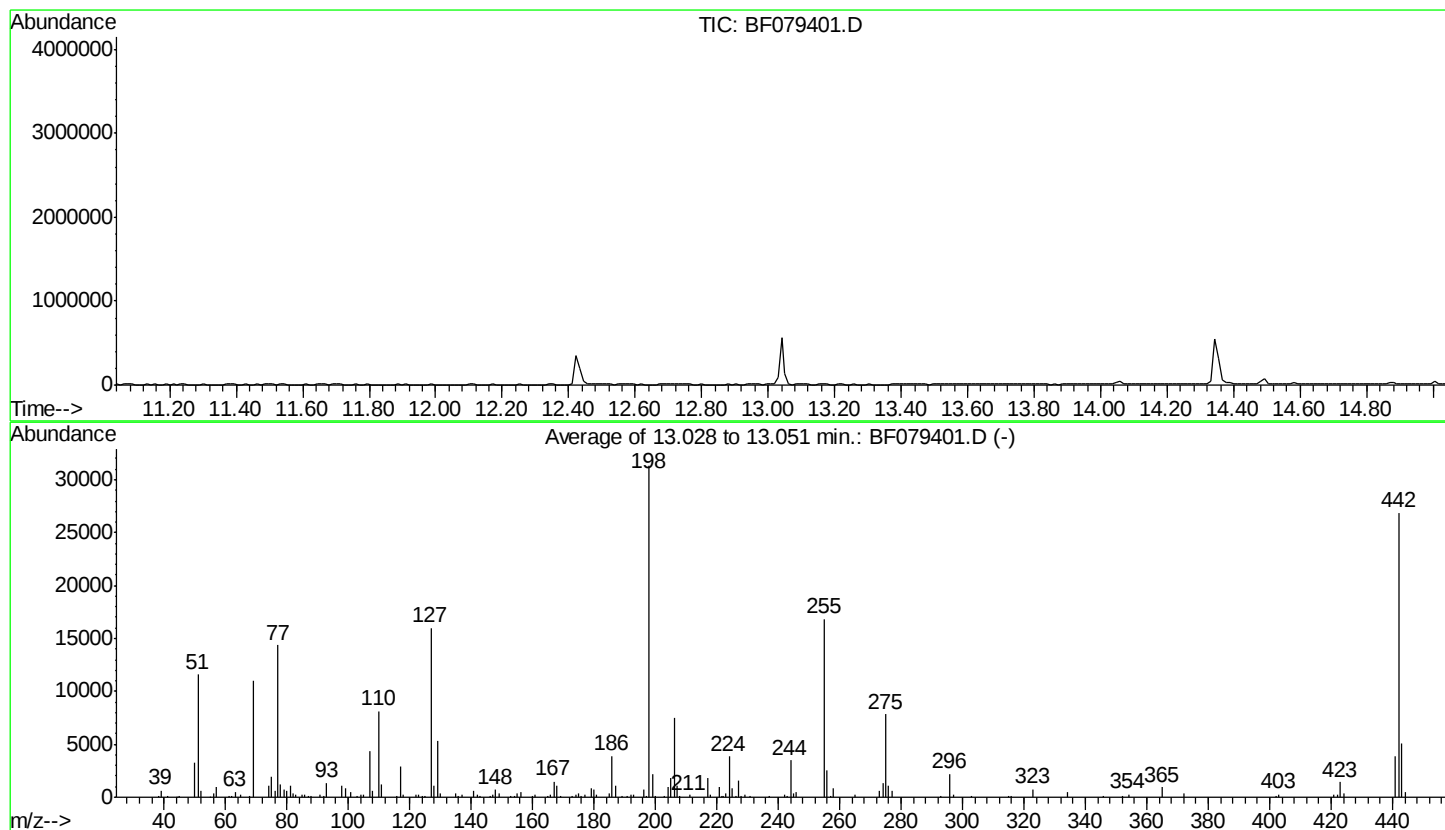

AutoFind: Scans 1036, 1037, 1038; Background Corrected with Scan 1033

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.0	11601	PASS
68	69	0.00	2	1.3	145	PASS
69	198	0.00	100	35.3	11069	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.1	16006	PASS
197	198	0.00	2	0.4	124	PASS
198	198	100	100	100.0	31332	PASS
199	198	5	9	7.0	2189	PASS
275	198	10	60	24.9	7815	PASS
365	198	1	100	3.1	960	PASS
441	442	0.01	24	14.6	3931	PASS
442	198	50	100	85.9	26905	PASS
443	442	15	24	19.0	5105	PASS