

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF052120\  
 Data File : BF120379.D  
 Acq On : 21 May 2020 14:25  
 Operator : MA/SJ  
 Sample : PB129032BL  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 PB129032BL

Integration Parameters: rteint.p  
 Integrator: RTE  
 Smoothing : ON Filtering: 5  
 Sampling : 1 Min Area: 3 % of largest Peak  
 Start Thrs: 0.2 Max Peaks: 100  
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF051420.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.198       | 525           | 529         | 558          | rBV      | 4656352        | 5219367       | 88.57%          | 12.049%       |
| 2         | 6.245       | 703           | 707         | 735          | rBV      | 4082530        | 5003340       | 84.91%          | 11.551%       |
| 3         | 6.586       | 762           | 765         | 782          | rBV      | 966810         | 1259007       | 21.36%          | 2.907%        |
| 4         | 6.745       | 787           | 792         | 815          | rBV      | 3636201        | 4186324       | 71.04%          | 9.665%        |
| 5         | 7.157       | 857           | 862         | 882          | rBV      | 2437299        | 3255667       | 55.25%          | 7.516%        |
| 6         | 7.875       | 979           | 984         | 1006         | rBV      | 1406156        | 1702773       | 28.90%          | 3.931%        |
| 7         | 8.957       | 1162          | 1168        | 1184         | rBV      | 4796272        | 5824254       | 98.84%          | 13.446%       |
| 8         | 9.622       | 1276          | 1281        | 1293         | rBV      | 1613591        | 1837810       | 31.19%          | 4.243%        |
| 9         | 10.416      | 1411          | 1416        | 1434         | rBV      | 2957431        | 3472406       | 58.93%          | 8.016%        |
| 10        | 11.110      | 1528          | 1534        | 1551         | rBV      | 1823285        | 1958422       | 33.23%          | 4.521%        |
| 11        | 12.698      | 1798          | 1804        | 1821         | rBV      | 5252127        | 5892863       | 100.00%         | 13.604%       |
| 12        | 13.745      | 1978          | 1982        | 1996         | rBV      | 1769741        | 1816056       | 30.82%          | 4.193%        |
| 13        | 14.821      | 2161          | 2165        | 2169         | rBV      | 57238          | 59415         | 1.01%           | 0.137%        |
| 14        | 15.133      | 2213          | 2218        | 2229         | rBV      | 1144434        | 1667570       | 28.30%          | 3.850%        |
| 15        | 15.539      | 2282          | 2287        | 2291         | rBV      | 64479          | 86010         | 1.46%           | 0.199%        |
| 16        | 15.980      | 2358          | 2362        | 2369         | rVB      | 47035          | 74914         | 1.27%           | 0.173%        |


Sum of corrected areas: 43316198

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF052120\  
Data File : BF120379.D  
Acq On : 21 May 2020 14:25  
Operator : MA/SJ  
Sample : PB129032BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
PB129032BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF051420.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

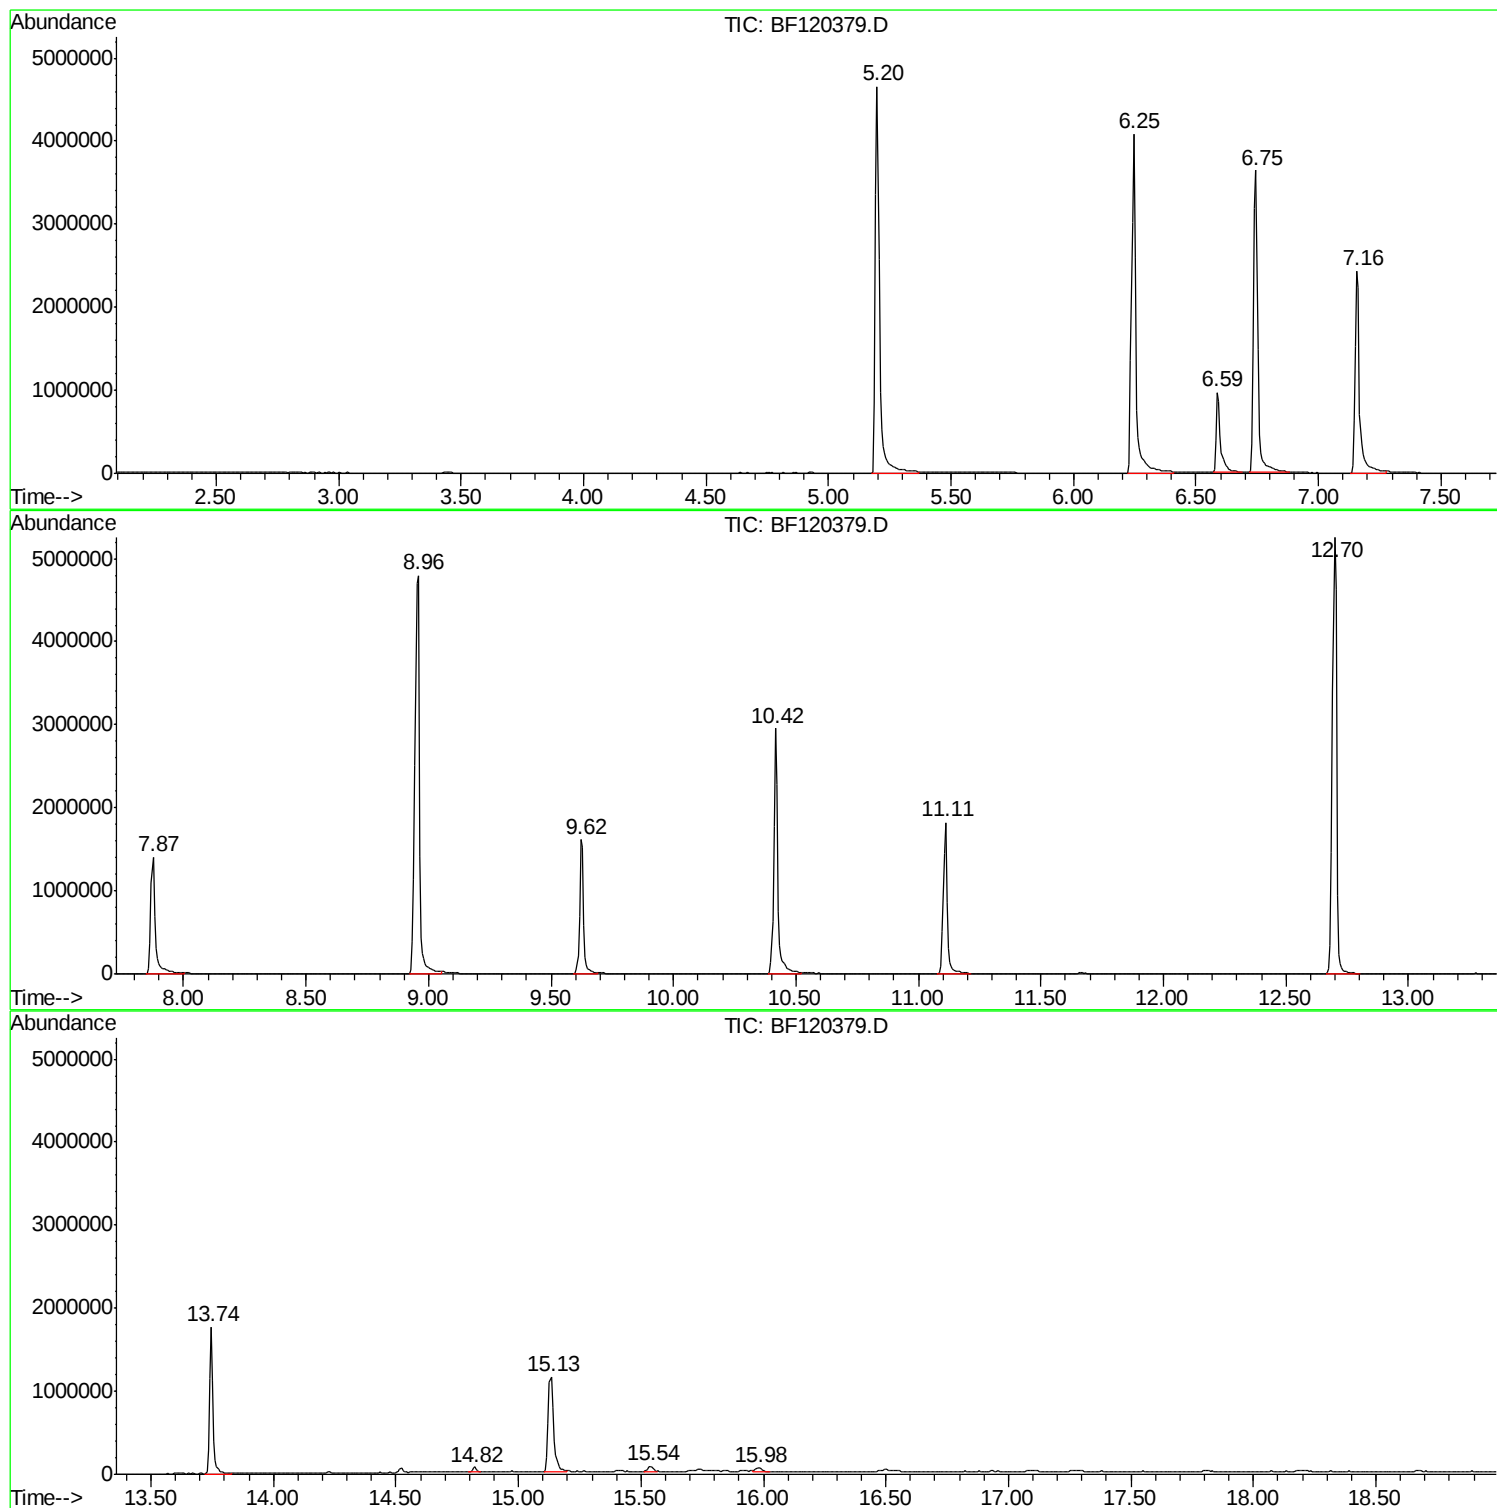

Data\_Path : Z:\SVOASRV\HPCHEM1\BNA\_F\DATA\BF052120\  
Data\_File : BF120379.D  
Acq\_On : 21\_May, 2020 14:255  
Operator : MA/SJJ  
Sample : PB129032BLL  
Misc :  
ALS\_Vial : 3 Sample\_Multiplier: 11

Instrument :  
BNA\_F  
ClientSampleId :  
PB129032BL

Quant\_Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF051420.MM  
Quant\_Title : ASP\_BNA\_STANDARDS\_FOR\_5\_POINT\_CALIBRATIONN

TIC\_Library : C:\DATABASE\NIST11.LL  
TIC\_Integration\_Parameters: LSCINT.PP

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|

No Library Search Compounds Detected

\*\*\*\*\*