


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF052120\
 Data File : BF120377.D
 Acq On : 21 May 2020 11:56
 Operator : MA/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051420.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 21 14:56:56 2020

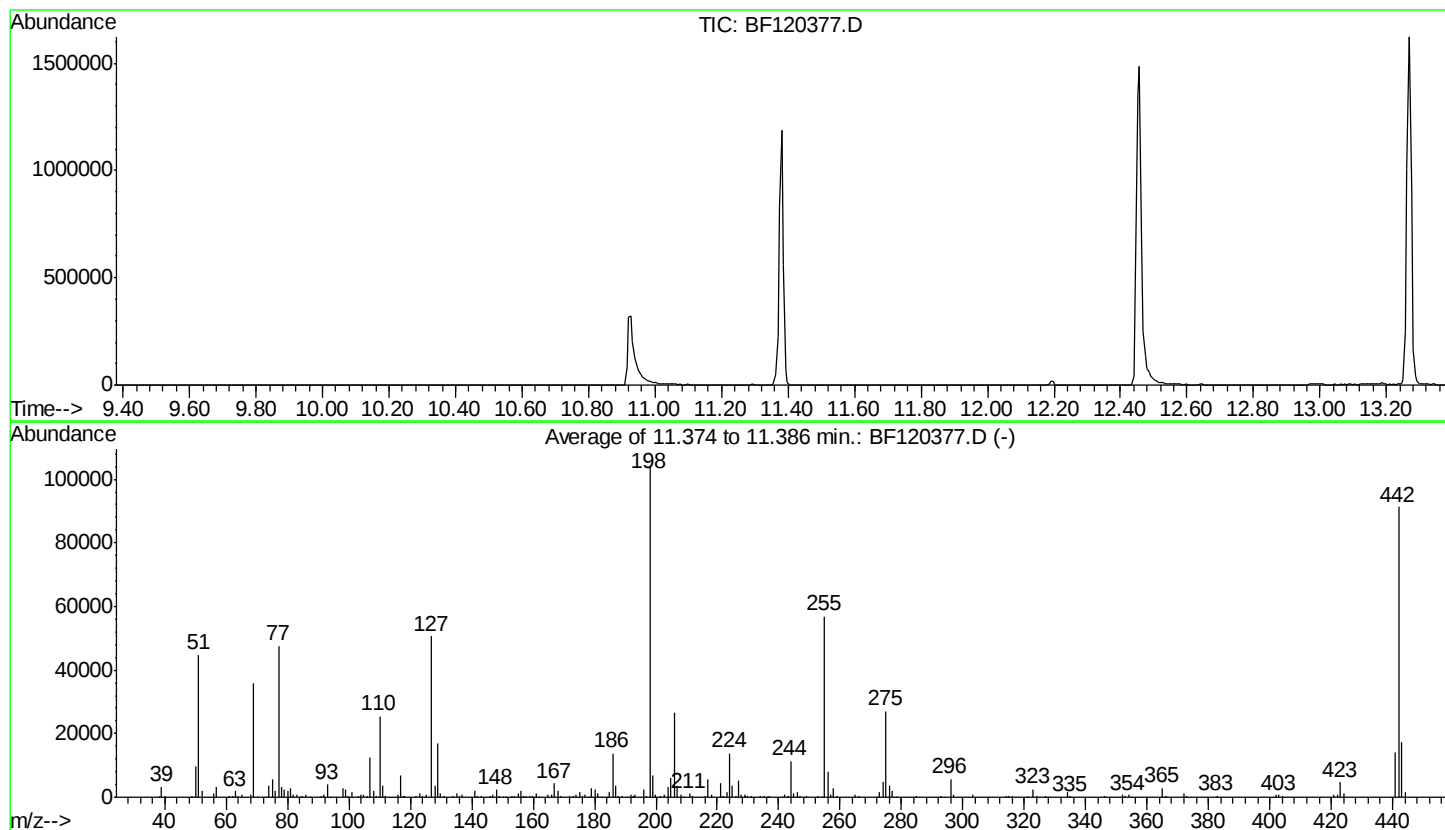

AutoFind: Scans 1579, 1580, 1581; Background Corrected with Scan 1573

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.9	44741	PASS
68	69	0.00	2	1.8	636	PASS
69	198	0.00	100	34.4	35912	PASS
70	69	0.00	2	0.3	105	PASS
127	198	10	80	48.5	50581	PASS
197	198	0.00	2	0.6	605	PASS
198	198	100	100	100.0	104277	PASS
199	198	5	9	6.8	7048	PASS
275	198	10	60	26.0	27125	PASS
365	198	1	100	2.8	2879	PASS
441	198	0.01	100	13.7	14235	PASS
442	198	50	100	87.6	91330	PASS
443	442	15	24	19.2	17499	PASS