
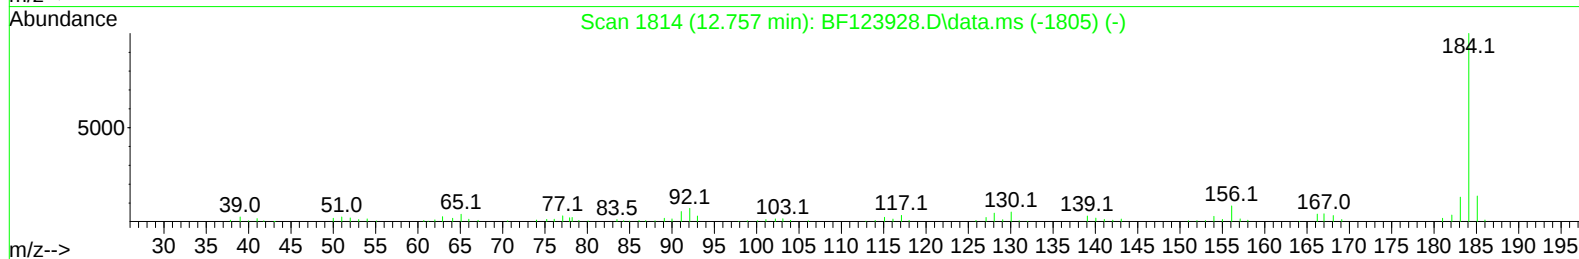
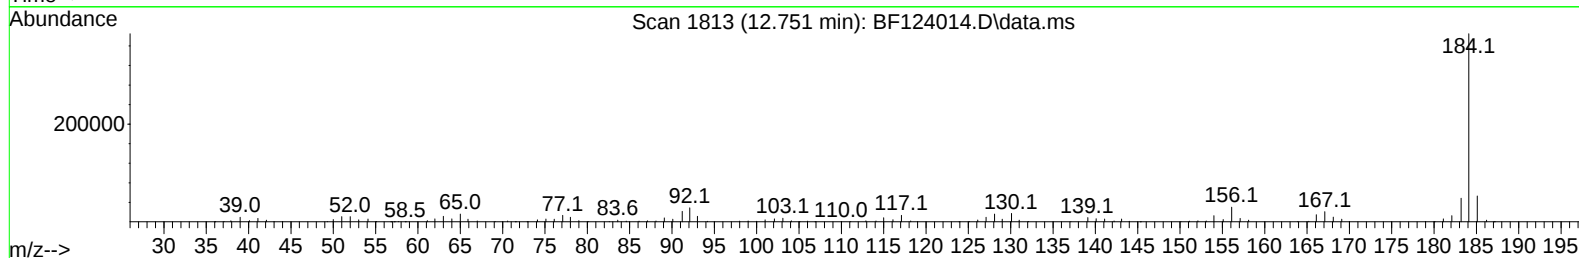


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052121\
Data File : BF124014.D
Acq On : 21 May 2021 11:06
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 21 11:39:44 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 14 19:05:57 2021
Response via : Initial Calibration

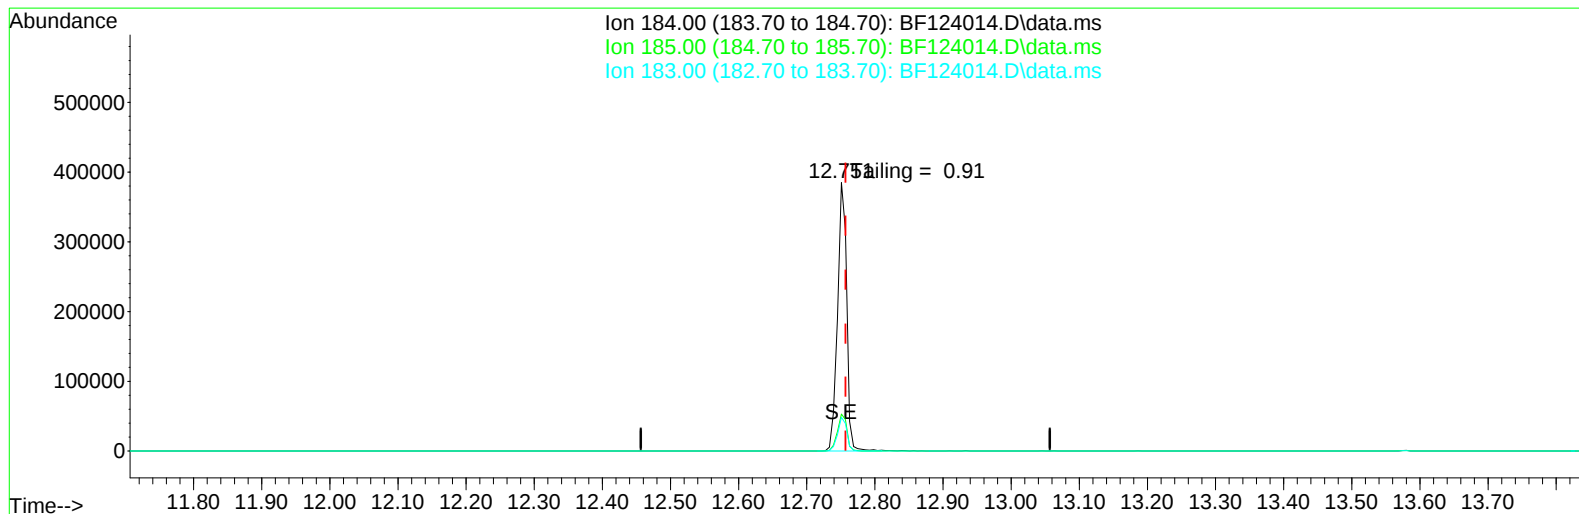

TIC: BF124014.D\data.ms

(77) Benzidine




12.751min (-0.006) 0.00 ng

response 358409

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	13.80
183.00	9.80	12.60#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052121\
Data File : BF124014.D
Acq On : 21 May 2021 11:06
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 21 11:39:44 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 14 19:05:57 2021
Response via : Initial Calibration

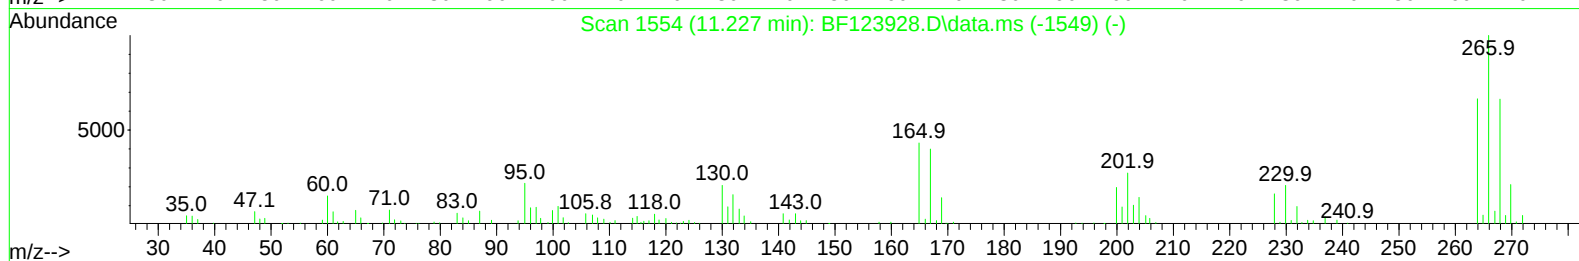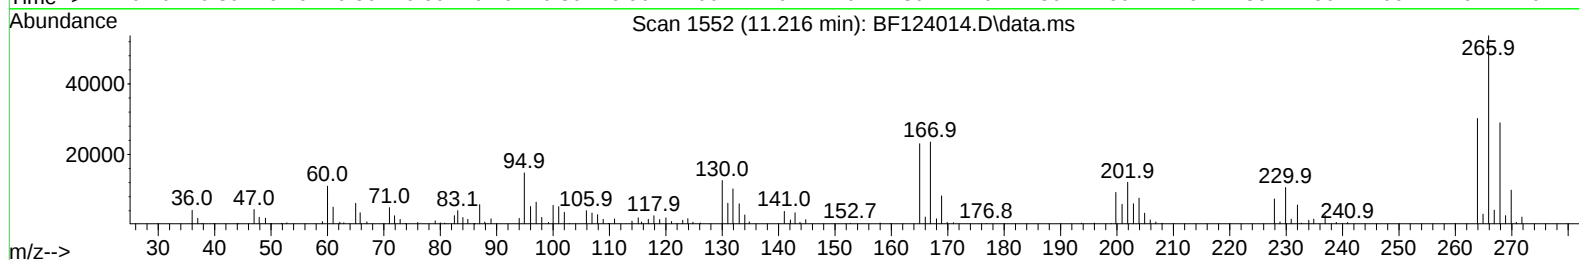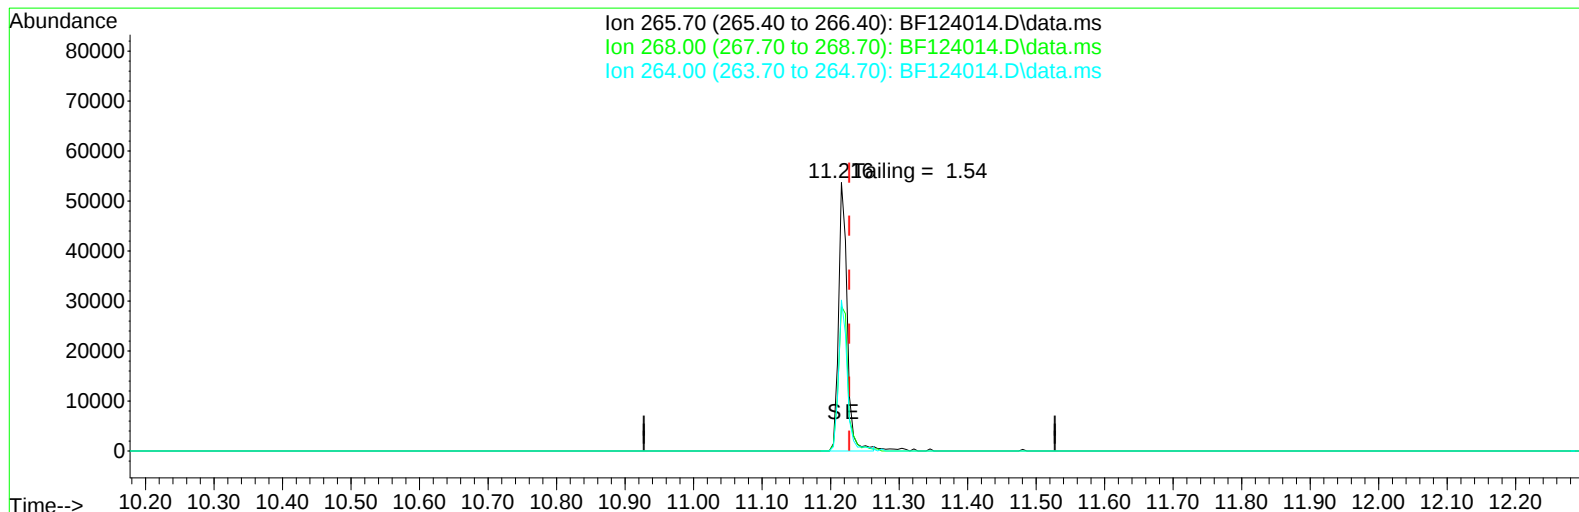

TIC: BF124014.D\data.ms

(70) Pentachlorophenol (C)

11.216min (-0.012) 24338.45 ng

response 47843

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	53.97
264.00	65.70	56.24
0.00	0.00	0.00