

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052121\
 Data File : BF124025.D
 Acq On : 21 May 2021 18:52
 Operator : JU/CG
 Sample : M2467-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 IDW-BR3-SO-051921

Quant Time: May 22 01:39:02 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 14 19:05:57 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.887	152	45659	20.00	ng	-0.02
21) Naphthalene-d8	8.169	136	183038	20.00	ng	#-0.02
39) Acenaphthene-d10	9.928	164	109997	20.00	ng	-0.02
64) Phenanthrene-d10	11.416	188	213164	20.00	ng	-0.01
76) Chrysene-d12	14.057	240	180932	20.00	ng	-0.01
86) Perylene-d12	15.545	264	149521	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.516	112	357744	110.01	ng	0.00
7) Phenol-d6	6.516	99	407882	96.69	ng	0.00
23) Nitrobenzene-d5	7.451	82	369032	86.87	ng	-0.01
42) 2,4,6-Tribromophenol	10.716	330	181301	137.23	ng	-0.01
45) 2-Fluorobiphenyl	9.251	172	700662	78.39	ng	-0.01
79) Terphenyl-d14	13.004	244	978670	81.92	ng	-0.01
Target Compounds						
50) Dimethylphthalate	9.639	163	30218	3.44	ng	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052121\
Data File : BF124025.D
Acq On : 21 May 2021 18:52
Operator : JU/CG
Sample : M2467-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
IDW-BR3-SO-051921

Quant Time: May 22 01:39:02 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 14 19:05:57 2021
Response via : Initial Calibration




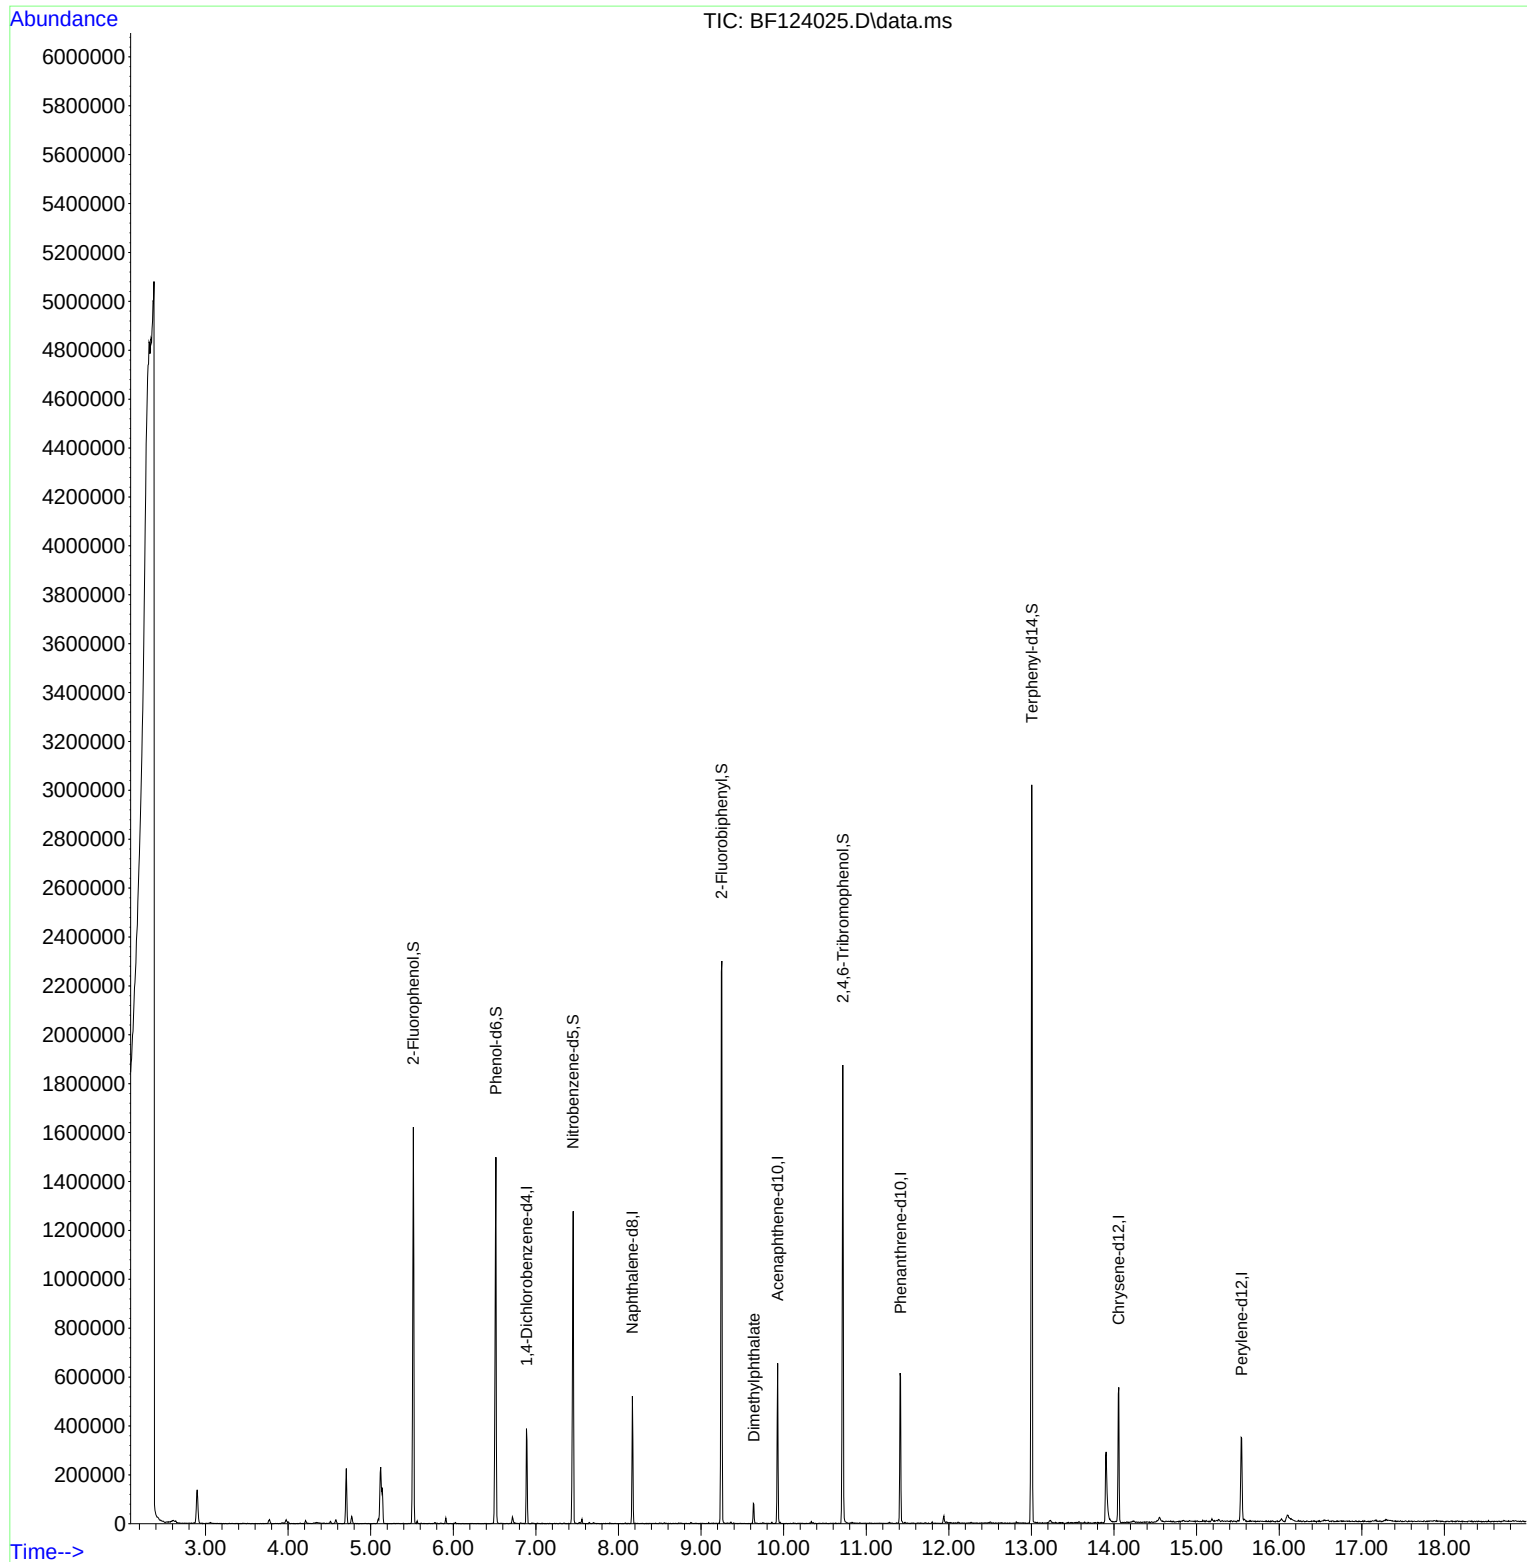




#1
1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.887 min Scan# 816
Delta R.T. -0.017 min
Lab File: BF124025.D
Acq: 21 May 2021 18:52




Instrument :
BNA_F
ClientSampleId :
IDW-BR3-SO-051921


Tgt Ion:152 Resp: 45659
Ion Ratio Lower Upper
152 100
150 171.5 127.0 190.6
115 79.2 54.3 81.5

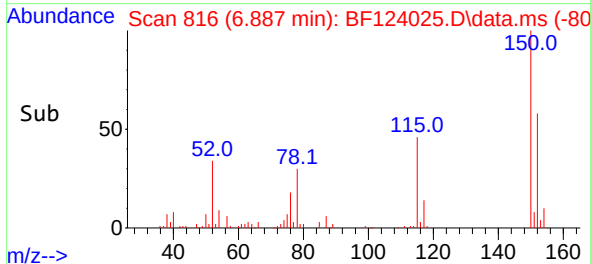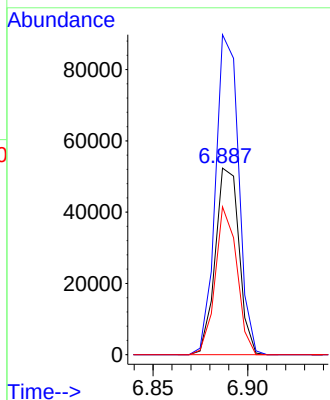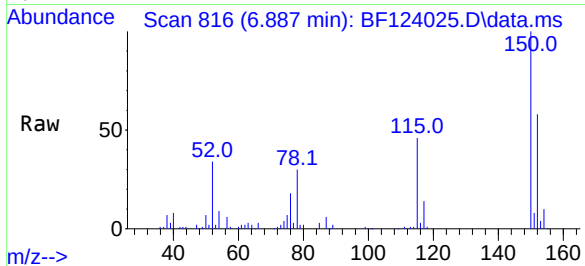

#5
2-Fluorophenol
Concen: 110.01 ng
RT: 5.516 min Scan# 583
Delta R.T. 0.006 min
Lab File: BF124025.D
Acq: 21 May 2021 18:52

Tgt Ion:112 Resp: 357744
Ion Ratio Lower Upper
112 100
64 78.5 61.4 92.0
63 41.2 33.0 49.4

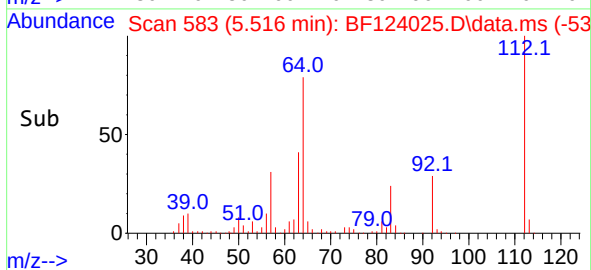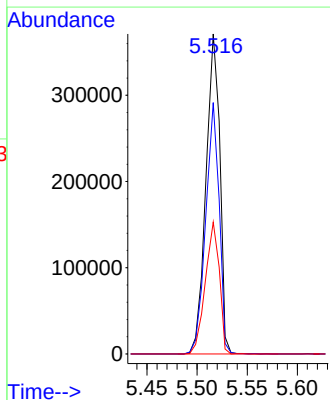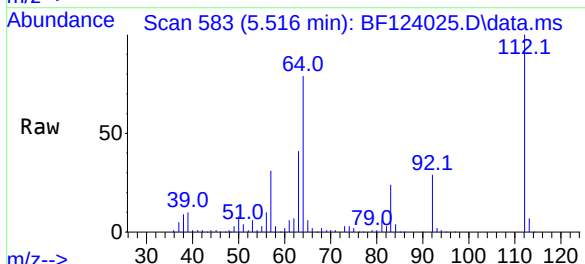







#7
Phenol-d6
Concen: 96.69 ng
RT: 6.516 min Scan# 753
Delta R.T. -0.006 min
Lab File: BF124025.D
Acq: 21 May 2021 18:52

Instrument :
BNA_F
ClientSampleId :
IDW-BR3-SO-051921

Tgt Ion: 99 Resp: 407882




Ion	Ratio	Lower	Upper
99	100		
42	25.9	19.8	29.8
71	43.1	31.1	46.7

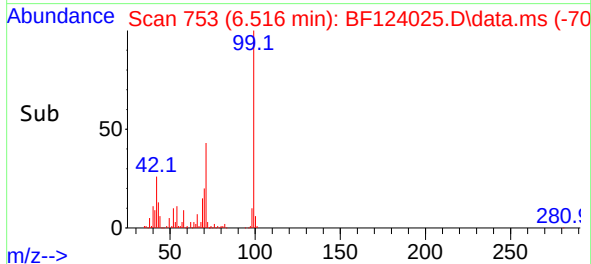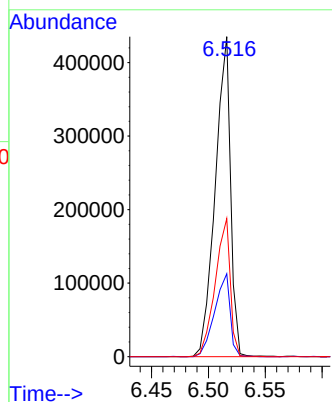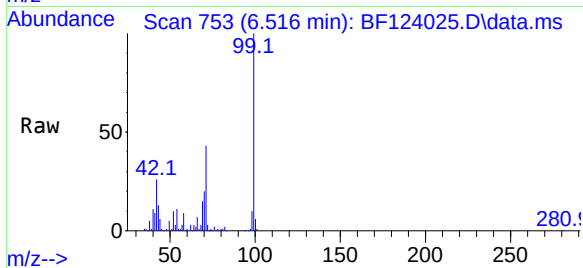


#21
Naphthalene-d8
Concen: 20.00 ng
RT: 8.169 min Scan# 1034
Delta R.T. -0.017 min
Lab File: BF124025.D
Acq: 21 May 2021 18:52

Tgt Ion: 136 Resp: 183038

Ion	Ratio	Lower	Upper
136	100		
137	10.5	8.7	13.1
54	14.3	9.8	14.6
68	6.8	4.1	6.1


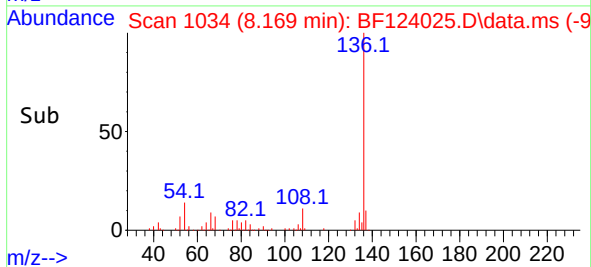
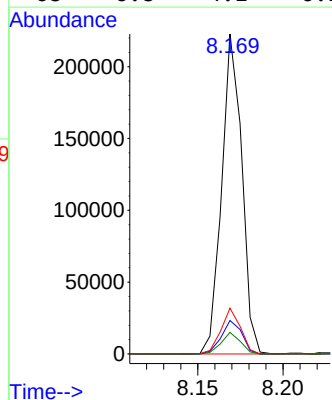
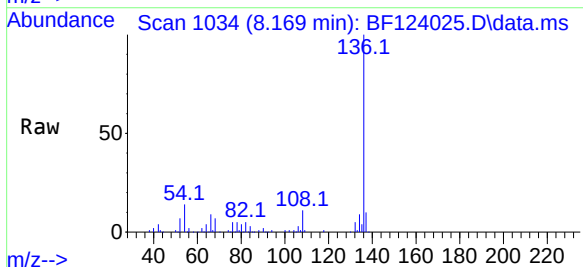


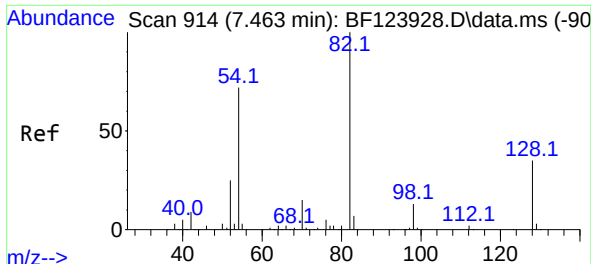

#23
Nitrobenzene-d5
Concen: 86.87 ng
RT: 7.451 min Scan# 912
Delta R.T. -0.012 min
Lab File: BF124025.D
Acq: 21 May 2021 18:52




Instrument :
BNA_F
ClientSampleId :
IDW-BR3-SO-051921


Tgt Ion: 82 Resp: 369032
Ion Ratio Lower Upper
82 100
128 37.6 29.4 44.2
54 70.6 54.1 81.1

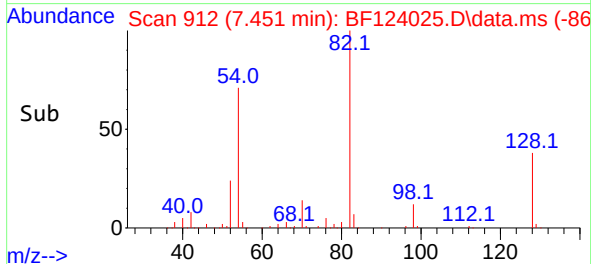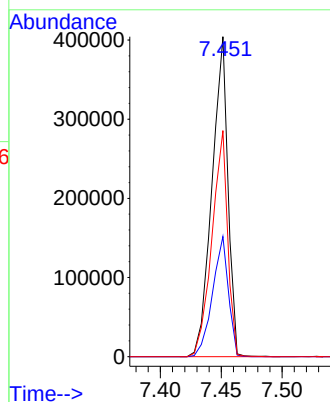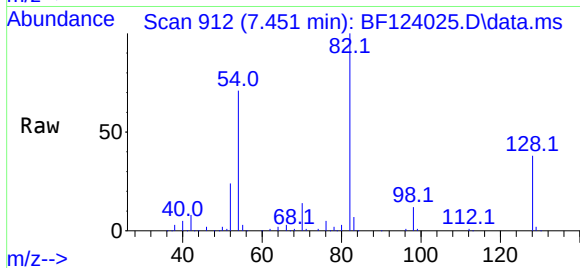

#39
Acenaphthene-d10
Concen: 20.00 ng
RT: 9.928 min Scan# 1333
Delta R.T. -0.017 min
Lab File: BF124025.D
Acq: 21 May 2021 18:52

Tgt Ion:164 Resp: 109997
Ion Ratio Lower Upper
164 100
162 94.3 80.7 121.1
160 42.1 37.3 55.9


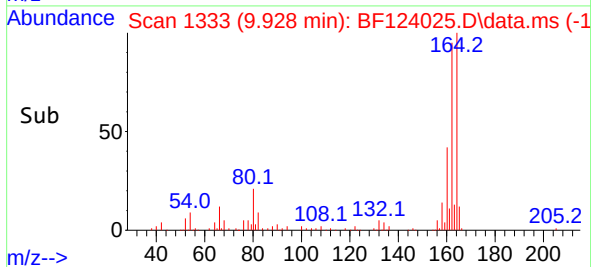
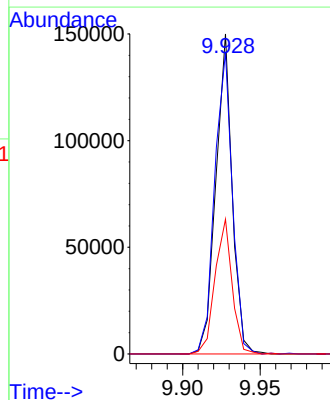
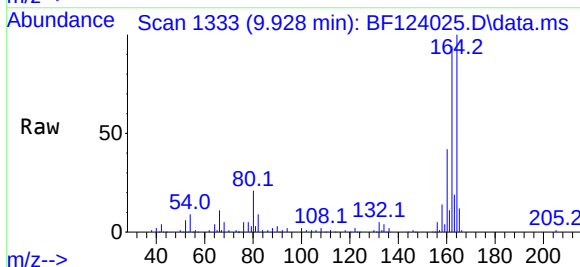




#42
2,4,6-Tribromophenol
Concen: 137.23 ng
RT: 10.716 min Scan# 1467
Delta R.T. -0.012 min
Lab File: BF124025.D
Acq: 21 May 2021 18:52




Instrument :
BNA_F
ClientSampleId :
IDW-BR3-SO-051921


Tgt Ion: 330 Resp: 181301
Ion Ratio Lower Upper
330 100
332 99.4 77.1 115.7
141 37.6 27.9 41.9

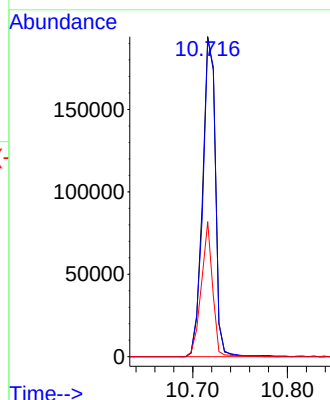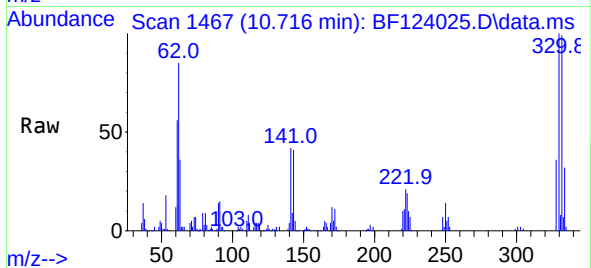

#45
2-Fluorobiphenyl
Concen: 78.39 ng
RT: 9.251 min Scan# 1218
Delta R.T. -0.012 min
Lab File: BF124025.D
Acq: 21 May 2021 18:52

Tgt Ion: 172 Resp: 700662
Ion Ratio Lower Upper
172 100
171 36.2 28.1 42.1
170 23.0 19.2 28.8


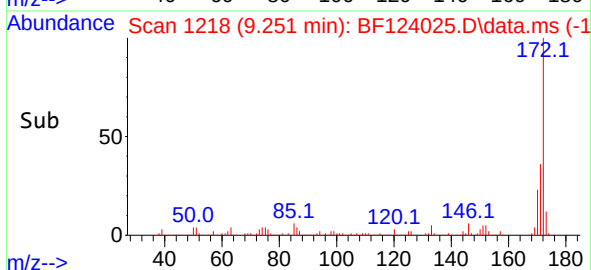
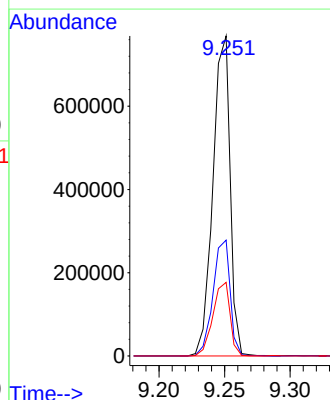





#50
Dimethylphthalate
Concen: 3.44 ng
RT: 9.639 min Scan# 1284
Delta R.T. -0.023 min
Lab File: BF124025.D
Acq: 21 May 2021 18:52




Instrument :
BNA_F
ClientSampleId :
IDW-BR3-SO-051921


Tgt Ion:163	Resp:	30218
Ion Ratio	Lower	Upper
163	100	
194	4.6	3.1 4.7
164	9.7	8.2 12.2

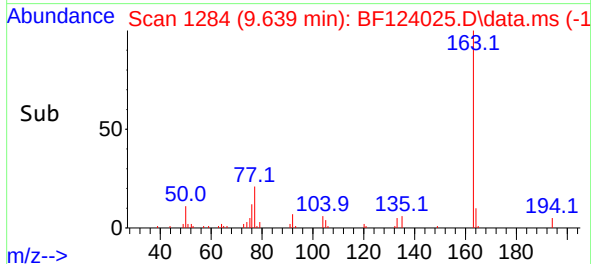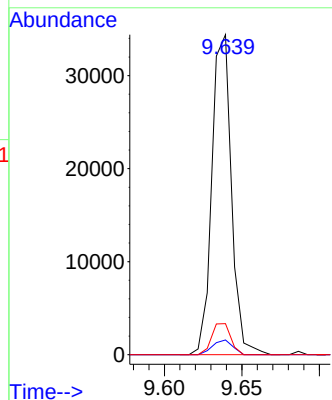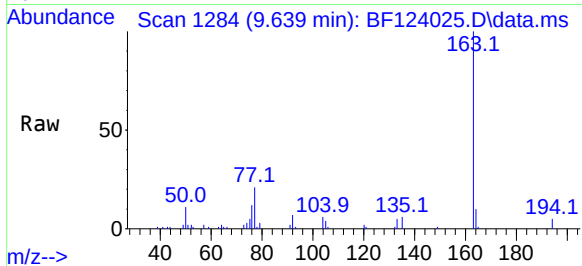

#64
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.416 min Scan# 1586
Delta R.T. -0.011 min
Lab File: BF124025.D
Acq: 21 May 2021 18:52

Tgt Ion:188	Resp:	213164
Ion Ratio	Lower	Upper
188	100	
94	9.2	6.9 10.3
80	8.5	8.2 12.2


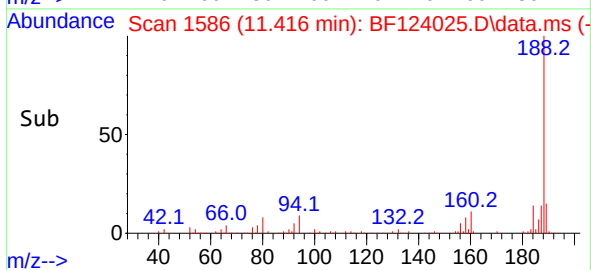
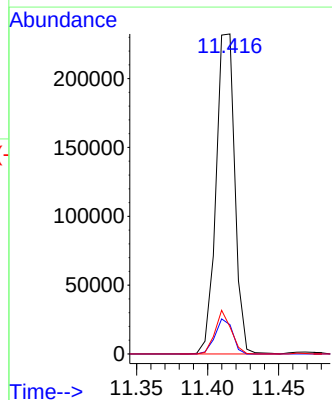
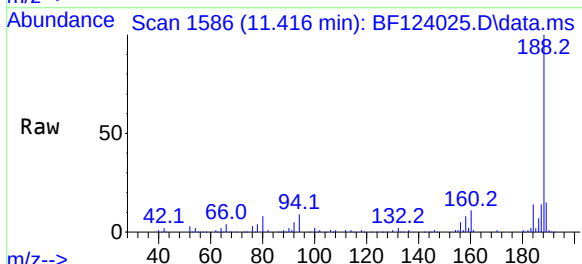




#76
Chrysene-d12
Concen: 20.00 ng
RT: 14.057 min Scan# 2035
Delta R.T. -0.012 min
Lab File: BF124025.D
Acq: 21 May 2021 18:52




Instrument :
BNA_F
ClientSampleId :
IDW-BR3-SO-051921


Tgt Ion:240 Resp: 180932
Ion Ratio Lower Upper
240 100
120 9.3 7.2 10.8
236 25.6 19.0 28.4

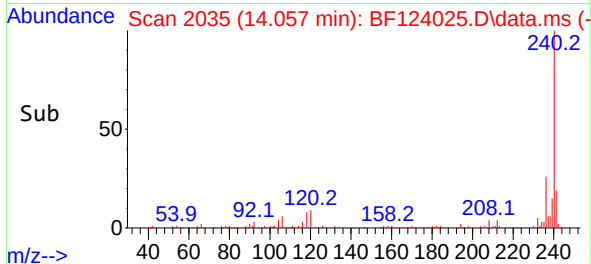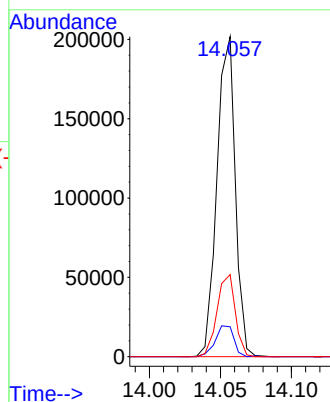

#79
Terphenyl-d14
Concen: 81.92 ng
RT: 13.004 min Scan# 1856
Delta R.T. -0.012 min
Lab File: BF124025.D
Acq: 21 May 2021 18:52

Tgt Ion:244 Resp: 978670
Ion Ratio Lower Upper
244 100
212 7.9 5.7 8.5
122 12.4 9.7 14.5

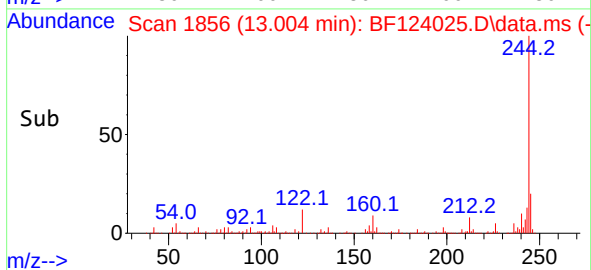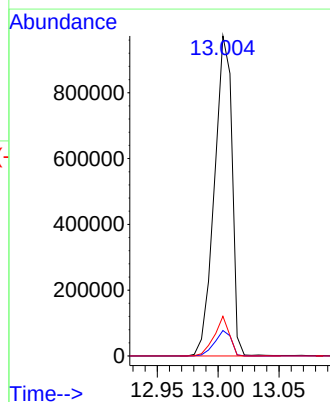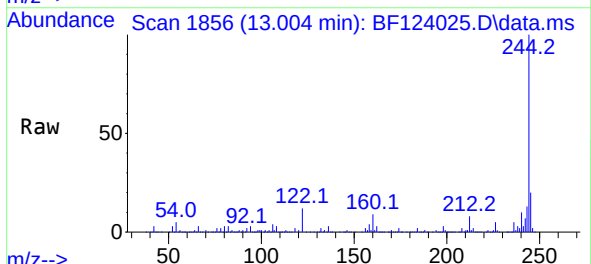

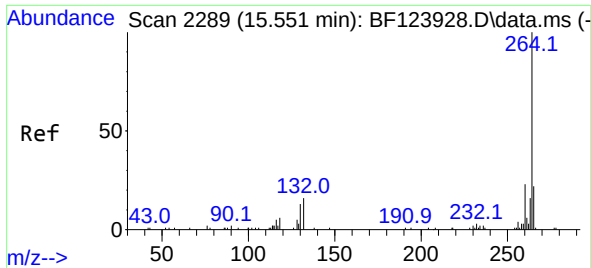

#86
Perylene-d12
Concen: 20.00 ng
RT: 15.545 min Scan# 2288
Delta R.T. -0.006 min
Lab File: BF124025.D
Acq: 21 May 2021 18:52

Instrument :
BNA_F
ClientSampleId :
IDW-BR3-SO-051921

Tgt Ion:264	Resp:	149521
Ion	Ratio	Lower Upper
264	100	
260	24.6	18.7 28.1
265	19.4	17.8 26.8

