

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052121\
 Data File : BF124026.D
 Acq On : 21 May 2021 19:26
 Operator : JU/CG
 Sample : M2482-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 BU-02-052021

Quant Time: May 22 01:39:13 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 14 19:05:57 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.886	152	57741	20.00	ng	-0.02
21) Naphthalene-d8	8.175	136	237373	20.00	ng	-0.01
39) Acenaphthene-d10	9.927	164	139604	20.00	ng	-0.02
64) Phenanthrene-d10	11.416	188	262786	20.00	ng	-0.01
76) Chrysene-d12	14.057	240	158220	20.00	ng	-0.01
86) Perylene-d12	15.545	264	147603	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.504	112	122423	29.77	ng	0.00
7) Phenol-d6	6.510	99	333562	62.53	ng	-0.01
23) Nitrobenzene-d5	7.451	82	260990	47.37	ng	-0.01
42) 2,4,6-Tribromophenol	10.710	330	13027	7.77	ng	-0.02
45) 2-Fluorobiphenyl	9.245	172	500910	44.15	ng	-0.02
79) Terphenyl-d14	13.004	244	516293	49.42	ng	-0.01
Target Compounds						
50) Dimethylphthalate	9.639	163	84231	7.56	ng	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052121\
Data File : BF124026.D
Acq On : 21 May 2021 19:26
Operator : JU/CG
Sample : M2482-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
BU-02-052021

Quant Time: May 22 01:39:13 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 14 19:05:57 2021
Response via : Initial Calibration



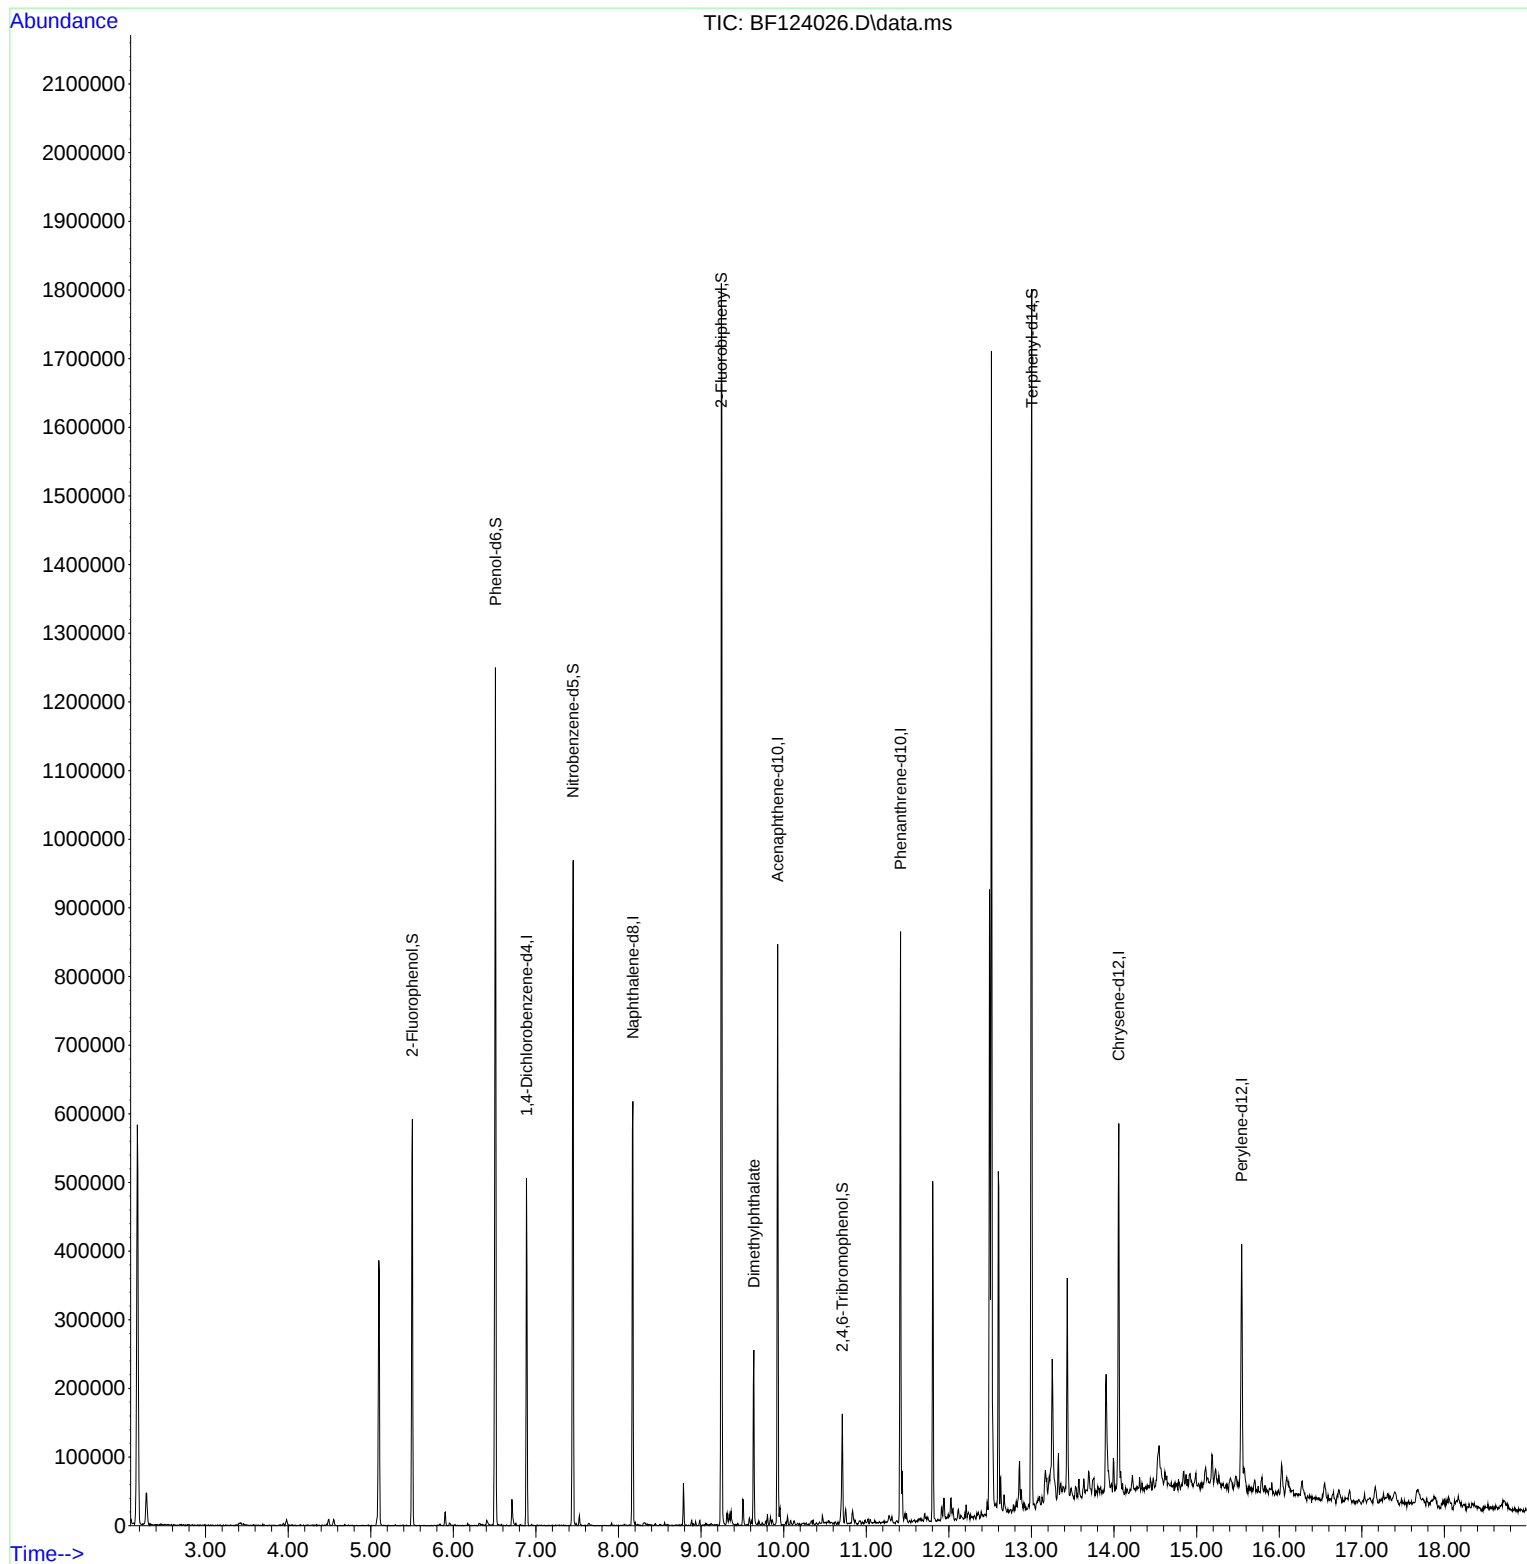


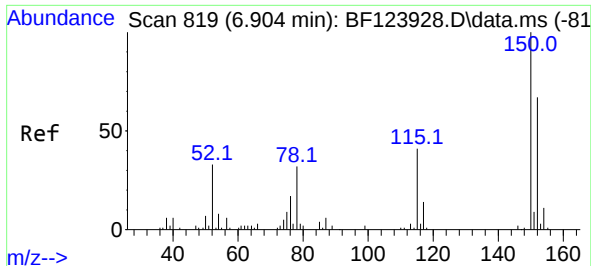

#1
1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.886 min Scan# 816
Delta R.T. -0.018 min
Lab File: BF124026.D
Acq: 21 May 2021 19:26




Instrument :
BNA_F
ClientSampleId :
BU-02-052021


Tgt Ion:152 Resp: 57741
Ion Ratio Lower Upper
152 100
150 171.4 127.0 190.6
115 72.2 54.3 81.5

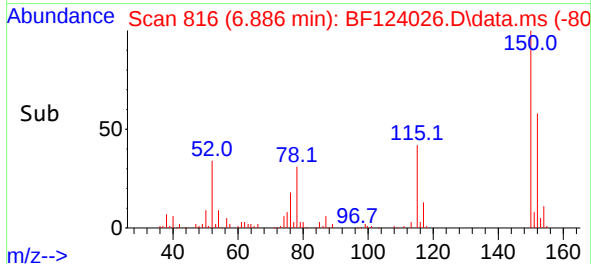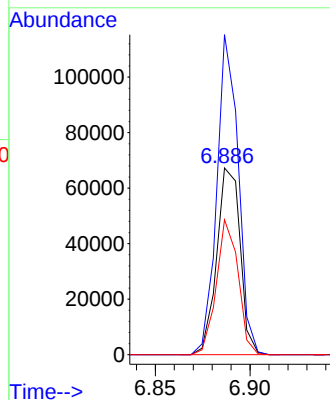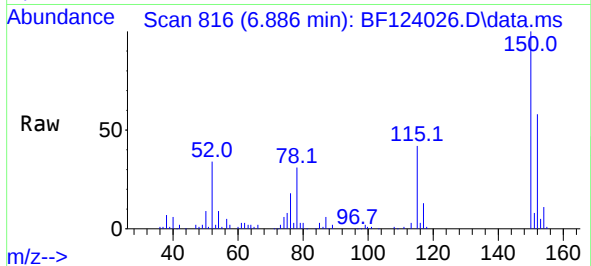

#5
2-Fluorophenol
Concen: 29.77 ng
RT: 5.504 min Scan# 581
Delta R.T. -0.006 min
Lab File: BF124026.D
Acq: 21 May 2021 19:26

Tgt Ion:112 Resp: 122423
Ion Ratio Lower Upper
112 100
64 69.2 61.4 92.0
63 36.7 33.0 49.4


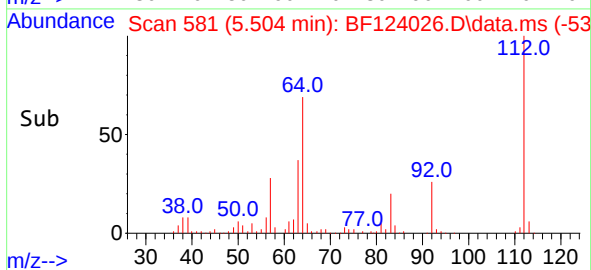
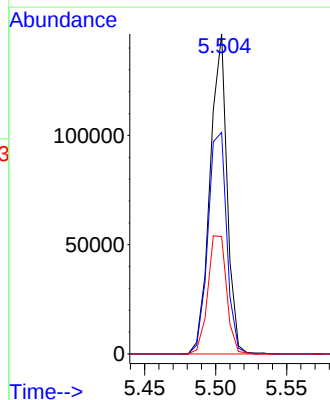
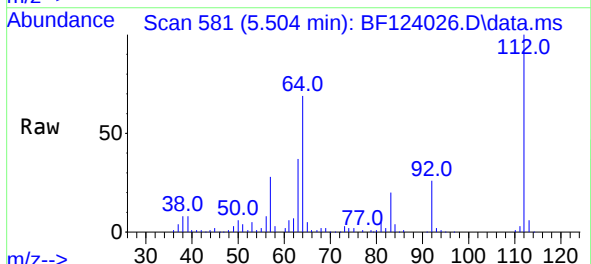


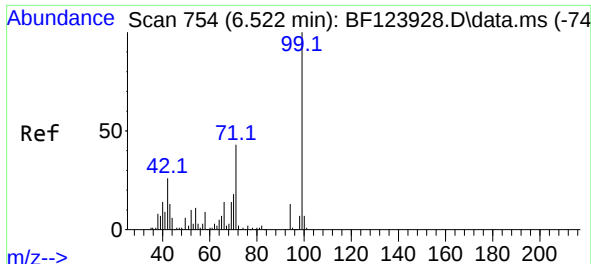

#7
Phenol-d6
Concen: 62.53 ng
RT: 6.510 min Scan# 752
Delta R.T. -0.012 min
Lab File: BF124026.D
Acq: 21 May 2021 19:26




Instrument :
BNA_F
ClientSampleId :
BU-02-052021


Tgt Ion: 99 Resp: 333562
Ion Ratio Lower Upper
99 100
42 27.0 19.8 29.8
71 42.5 31.1 46.7

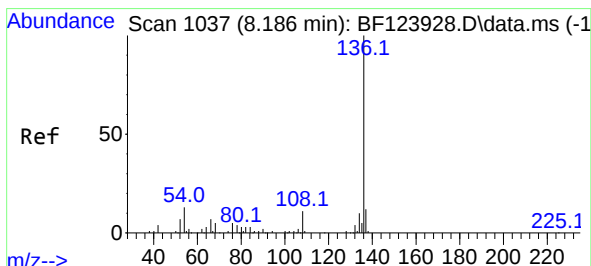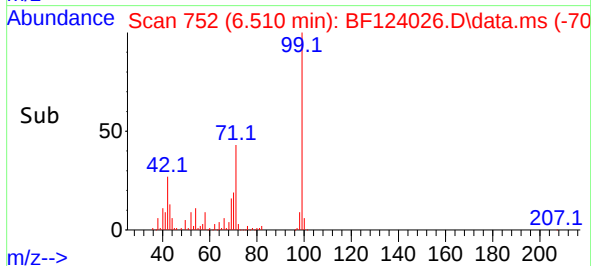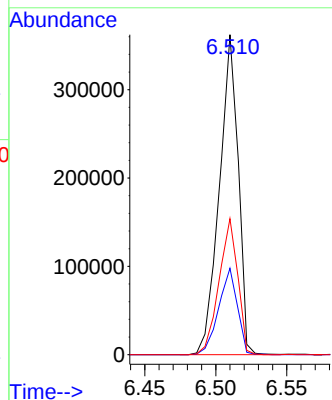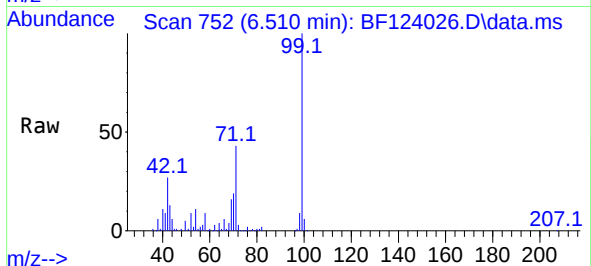

#21
Naphthalene-d8
Concen: 20.00 ng
RT: 8.175 min Scan# 1035
Delta R.T. -0.011 min
Lab File: BF124026.D
Acq: 21 May 2021 19:26

Tgt Ion: 136 Resp: 237373
Ion Ratio Lower Upper
136 100
137 9.9 8.7 13.1
54 10.4 9.8 14.6
68 6.0 4.1 6.1


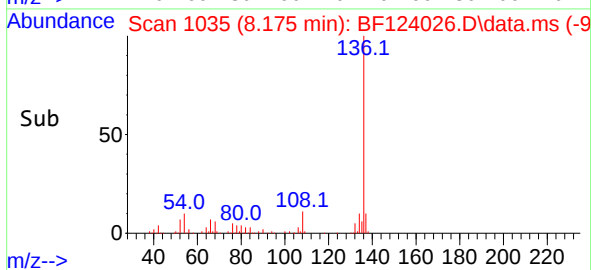
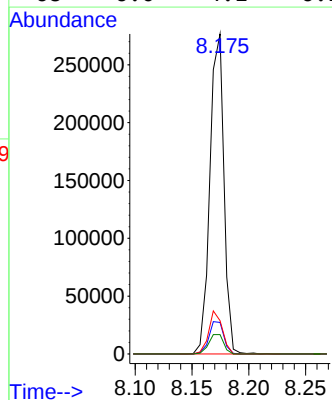
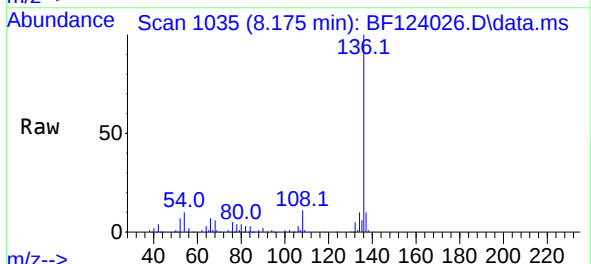


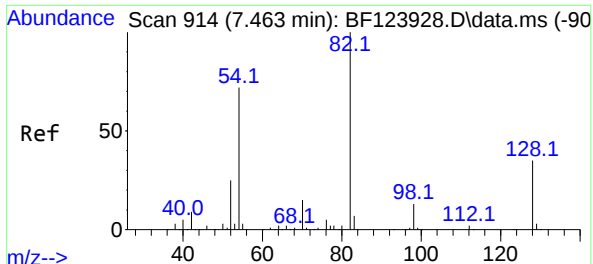

#23
Nitrobenzene-d5
Concen: 47.37 ng
RT: 7.451 min Scan# 912
Delta R.T. -0.012 min
Lab File: BF124026.D
Acq: 21 May 2021 19:26




Instrument :
BNA_F
ClientSampleId :
BU-02-052021


Tgt Ion: 82 Resp: 260990
Ion Ratio Lower Upper
82 100
128 40.1 29.4 44.2
54 68.2 54.1 81.1

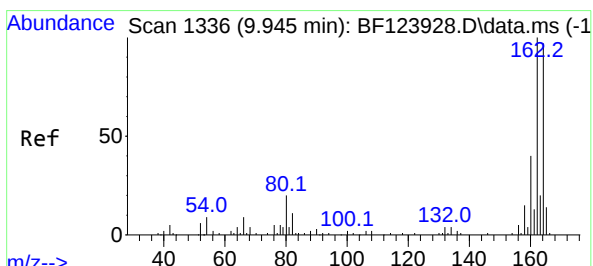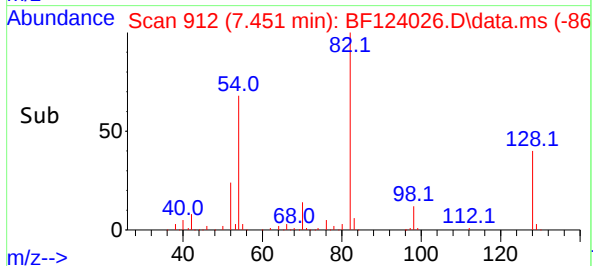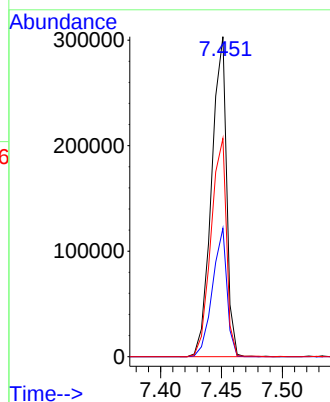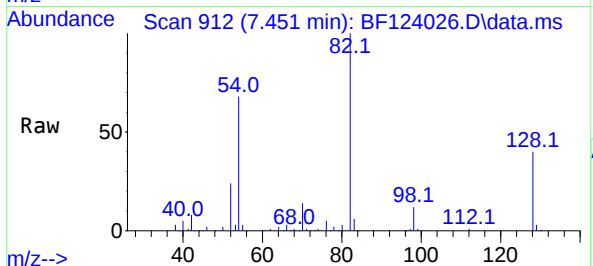

#39
Acenaphthene-d10
Concen: 20.00 ng
RT: 9.927 min Scan# 1333
Delta R.T. -0.018 min
Lab File: BF124026.D
Acq: 21 May 2021 19:26

Tgt Ion:164 Resp: 139604
Ion Ratio Lower Upper
164 100
162 104.4 80.7 121.1
160 45.1 37.3 55.9


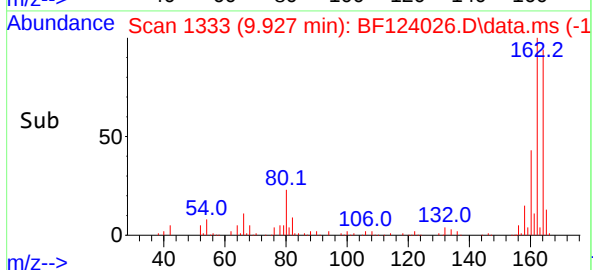
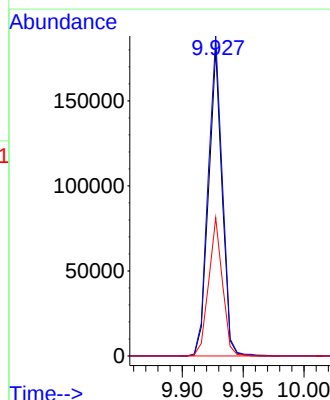
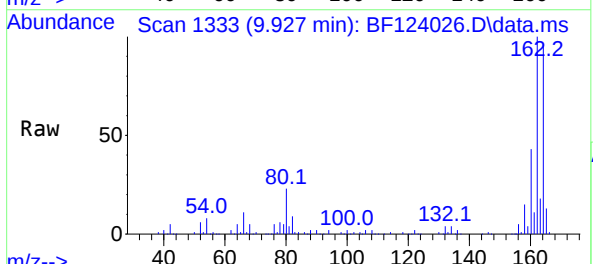


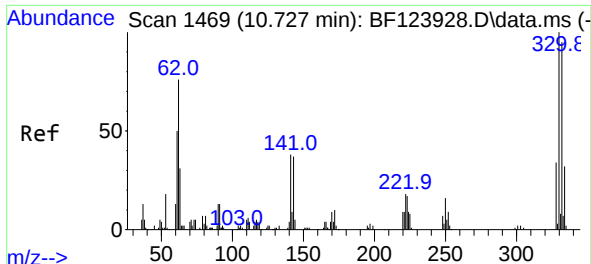

#42
2,4,6-Tribromophenol
Concen: 7.77 ng
RT: 10.710 min Scan# 1466
Delta R.T. -0.018 min
Lab File: BF124026.D
Acq: 21 May 2021 19:26




Instrument :
BNA_F
ClientSampleId :
BU-02-052021


Tgt Ion:	330	Resp:	13027
Ion Ratio	Lower	Upper	
330	100		
332	94.9	77.1	115.7
141	36.5	27.9	41.9

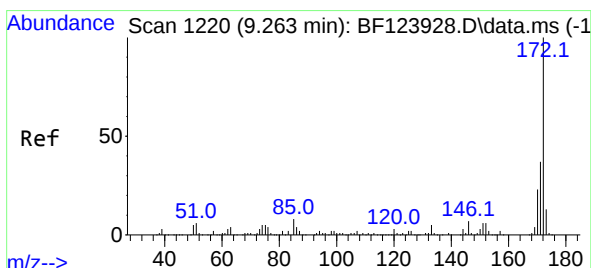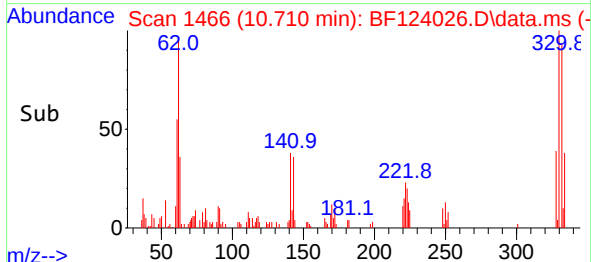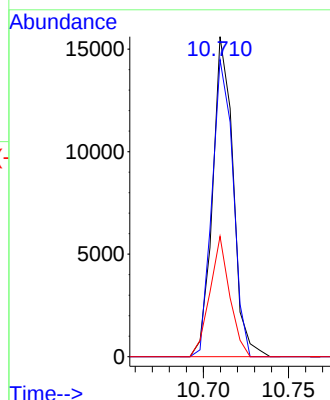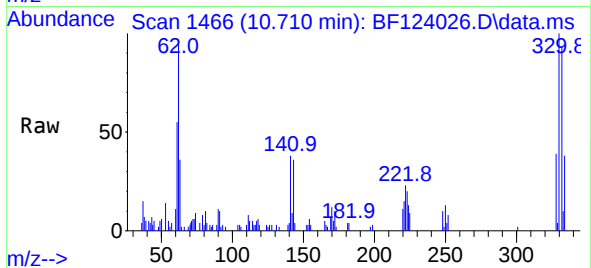

#45
2-Fluorobiphenyl
Concen: 44.15 ng
RT: 9.245 min Scan# 1217
Delta R.T. -0.018 min
Lab File: BF124026.D
Acq: 21 May 2021 19:26

Tgt Ion:	172	Resp:	500910
Ion Ratio	Lower	Upper	
172	100		
171	36.3	28.1	42.1
170	22.6	19.2	28.8


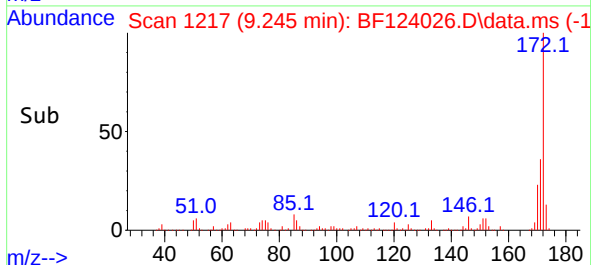
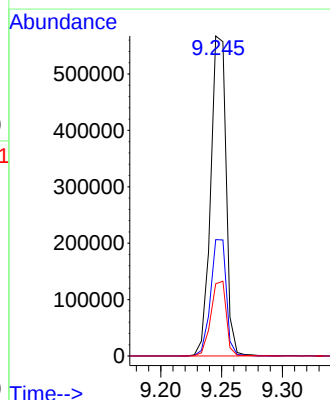
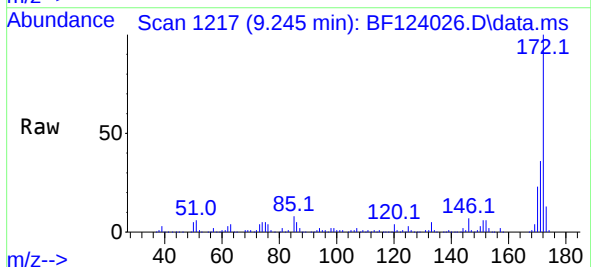


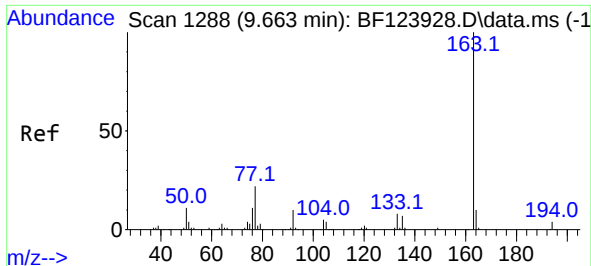

#50
Dimethylphthalate
Concen: 7.56 ng
RT: 9.639 min Scan# 1284
Delta R.T. -0.024 min
Lab File: BF124026.D
Acq: 21 May 2021 19:26




Instrument :
BNA_F
ClientSampleId :
BU-02-052021


Tgt Ion:163 Resp: 84231
Ion Ratio Lower Upper
163 100
194 3.6 3.1 4.7
164 8.8 8.2 12.2

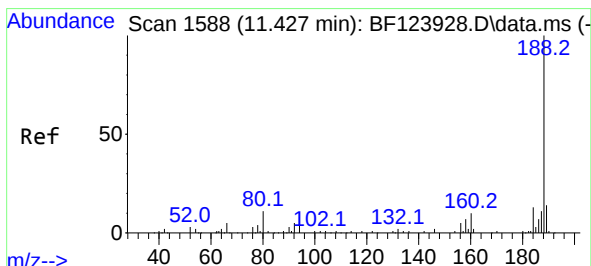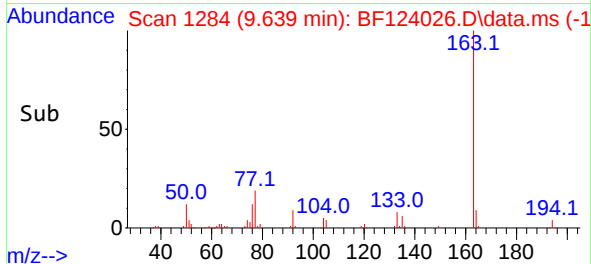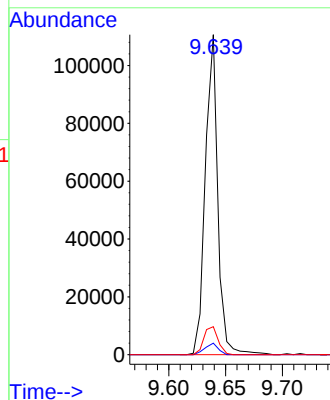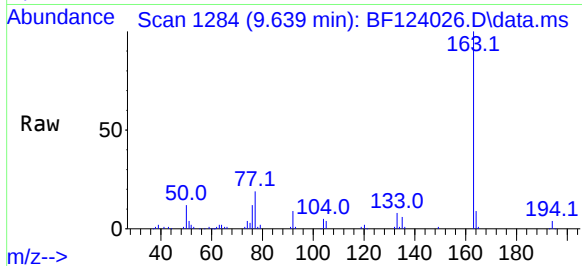

#64
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.416 min Scan# 1586
Delta R.T. -0.011 min
Lab File: BF124026.D
Acq: 21 May 2021 19:26

Tgt Ion:188 Resp: 262786
Ion Ratio Lower Upper
188 100
94 8.6 6.9 10.3
80 9.7 8.2 12.2


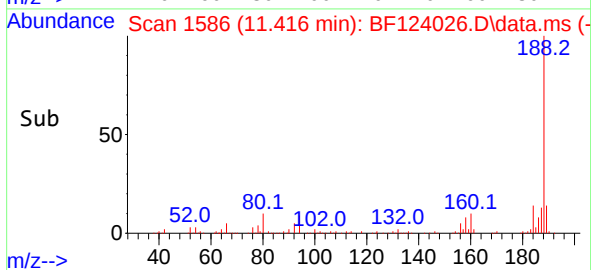
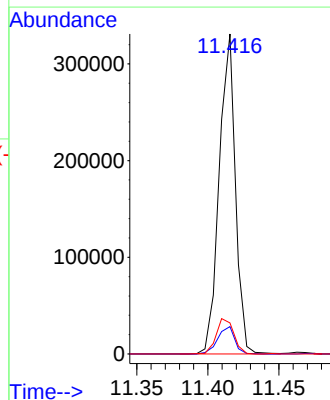
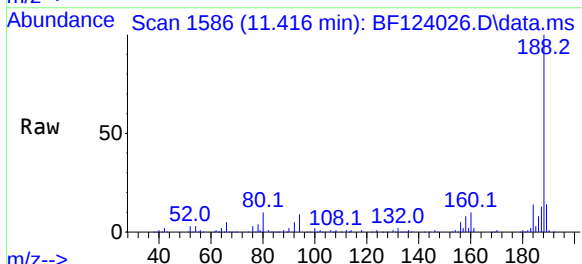


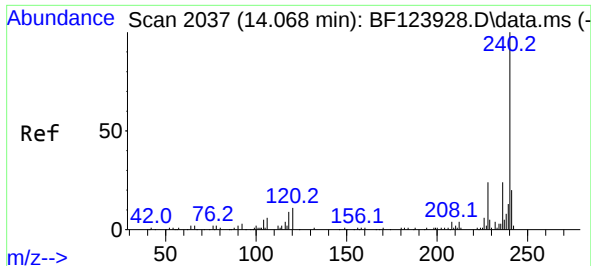

#76
Chrysene-d12
Concen: 20.00 ng
RT: 14.057 min Scan# 2035
Delta R.T. -0.012 min
Lab File: BF124026.D
Acq: 21 May 2021 19:26




Instrument :
BNA_F
ClientSampleId :
BU-02-052021


Tgt Ion:240 Resp: 158220
Ion Ratio Lower Upper
240 100
120 8.8 7.2 10.8
236 24.1 19.0 28.4

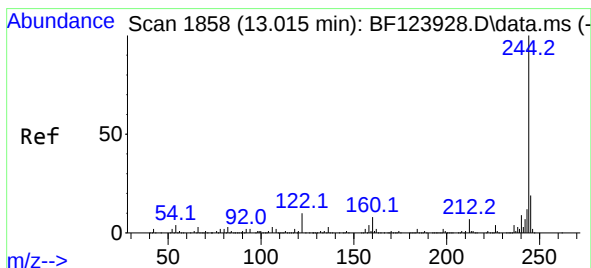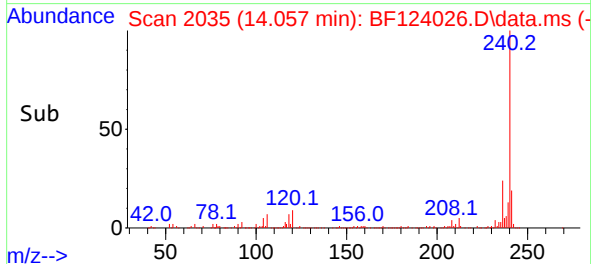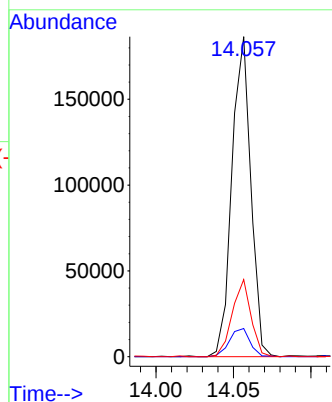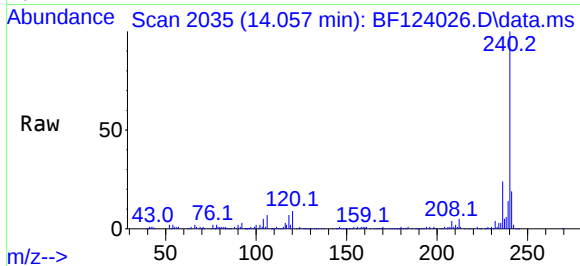

#79
Terphenyl-d14
Concen: 49.42 ng
RT: 13.004 min Scan# 1856
Delta R.T. -0.012 min
Lab File: BF124026.D
Acq: 21 May 2021 19:26


Tgt Ion:244 Resp: 516293
Ion Ratio Lower Upper
244 100
212 7.0 5.7 8.5
122 10.3 9.7 14.5

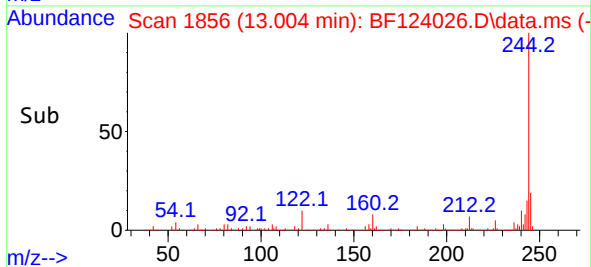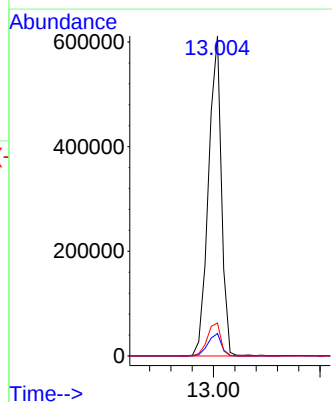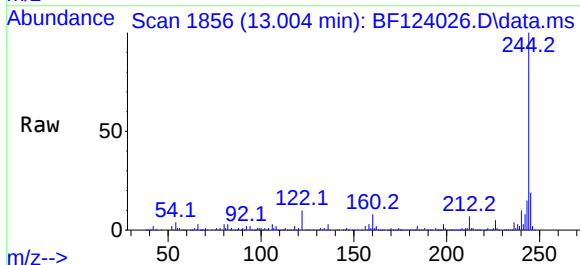

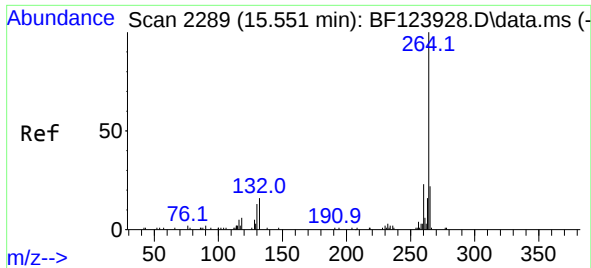

#86
Perylene-d12
Concen: 20.00 ng
RT: 15.545 min Scan# 2288
Delta R.T. -0.006 min
Lab File: BF124026.D
Acq: 21 May 2021 19:26

Instrument :
BNA_F
ClientSampleId :
BU-02-052021

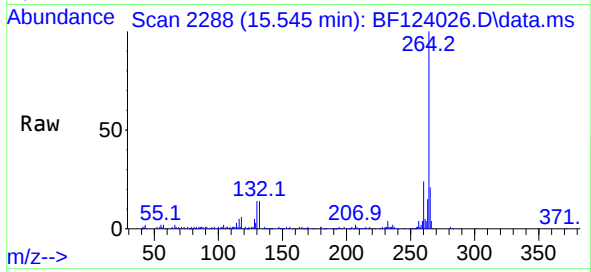

Tgt Ion:264 Resp: 147603

Ion	Ratio	Lower	Upper
264	100		
260	24.1	18.7	28.1
265	21.1	17.8	26.8

