

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052121\
 Data File : BF124016.D
 Acq On : 21 May 2021 13:16
 Operator : JU/CG
 Sample : PB136581BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB136581BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF124016.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.293	25	35	39	rVB	75074	109123	3.96%	0.658%
2	5.522	579	584	587	rBV	2197594	2365027	85.79%	14.266%
3	6.516	747	753	756	rBV	1921388	2339746	84.87%	14.114%
4	6.887	813	816	820	rBV	485545	448472	16.27%	2.705%
5	7.451	906	912	915	rBV	1401442	1540931	55.90%	9.295%
6	8.175	1030	1035	1038	rBV	633879	571085	20.72%	3.445%
7	9.251	1211	1218	1221	rBV	3244863	2756777	100.00%	16.629%
8	9.928	1328	1333	1336	rBV	831095	651252	23.62%	3.928%
9	10.716	1461	1467	1471	rBV	1750456	1674087	60.73%	10.098%
10	11.416	1582	1586	1589	rBV	776416	633146	22.97%	3.819%
11	13.004	1851	1856	1859	rBV	2941708	2660530	96.51%	16.049%
12	14.057	2031	2035	2038	rVB	526002	455761	16.53%	2.749%
13	15.545	2283	2288	2291	rBV	312142	371986	13.49%	2.244%




Sum of corrected areas: 16577923

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052121\
Data File : BF124016.D
Acq On : 21 May 2021 13:16
Operator : JU/CG
Sample : PB136581BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB136581BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

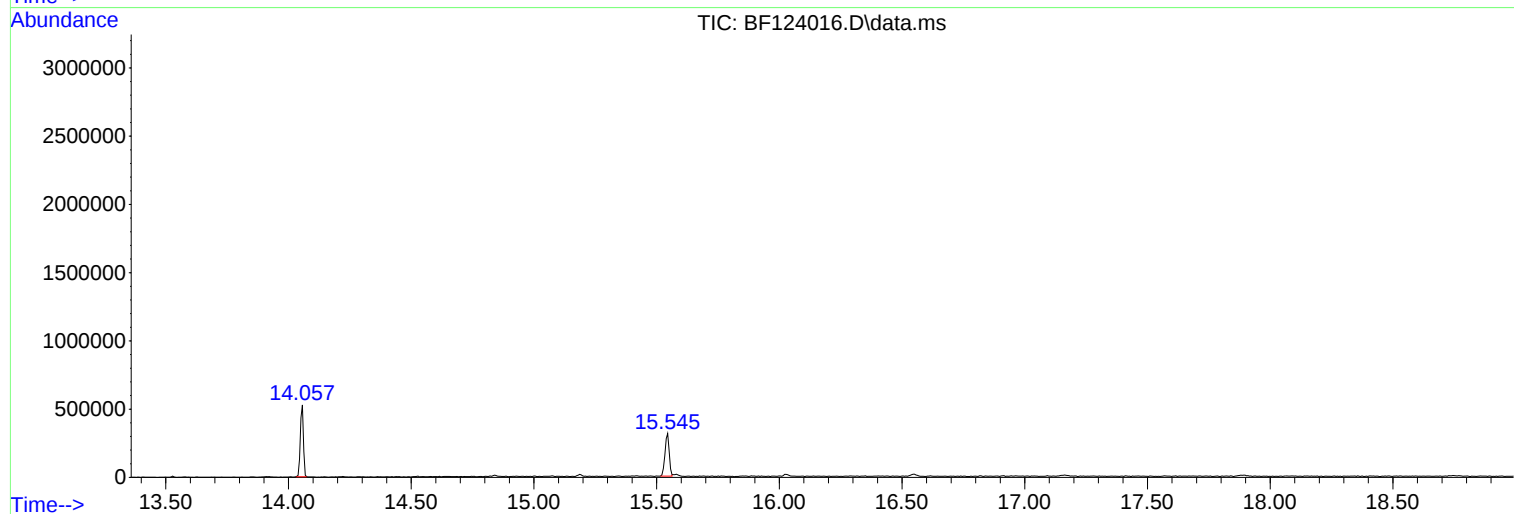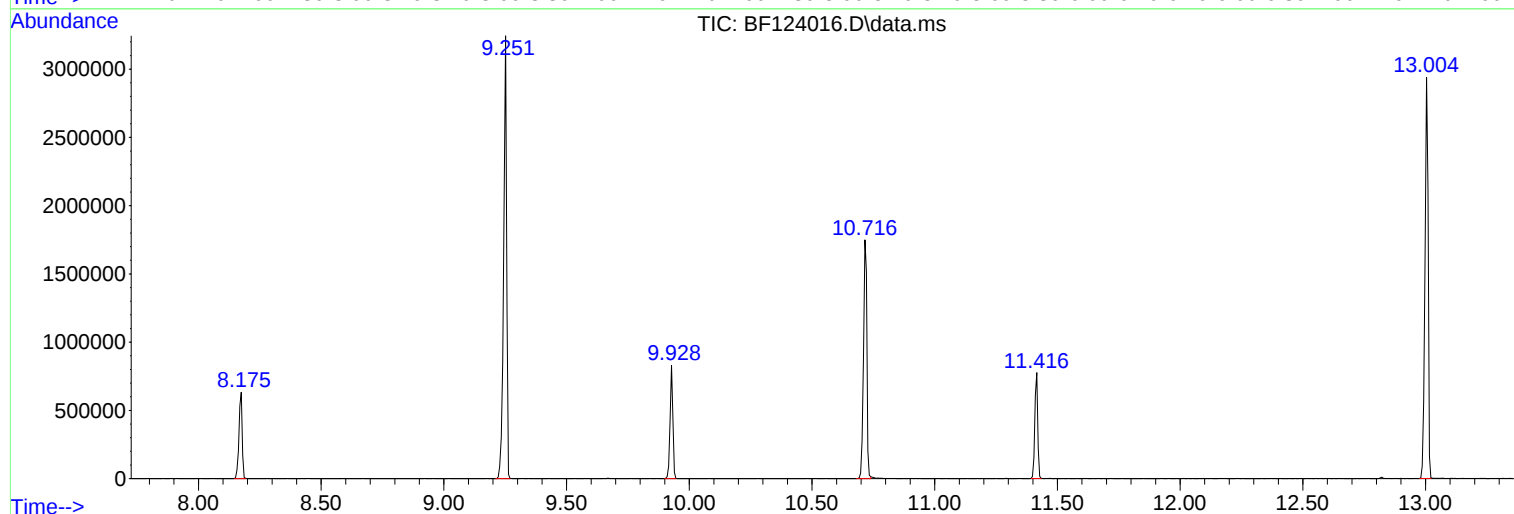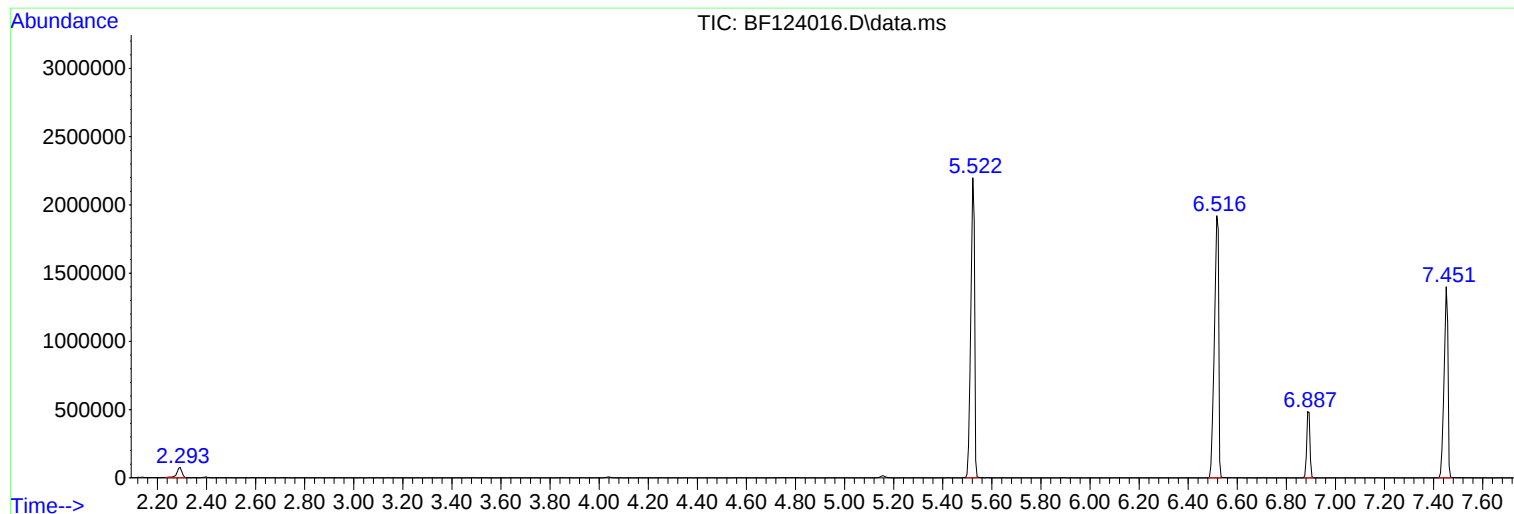

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052121\
Data File : BF124016.D
Acq On : 21 May 2021 13:16
Operator : JU/CG
Sample : PB136581BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB136581BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.293	4.87 ng	109123	1,4-Dichlorobenzene-d4	6.893

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	74
2			2-Methyl-5-hexen-3-ol	114	C7H14O	032815-70-6	43
3			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	38
4			3-Hexanol, 2,4-dimethyl-	130	C8H18O	013432-25-2	28
5			3-Pentanol, 2,4-dimethyl-	116	C7H16O	000600-36-2	25

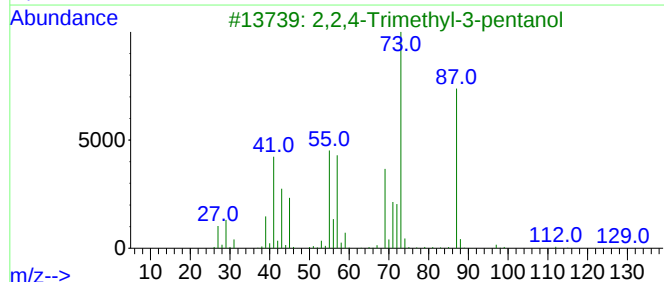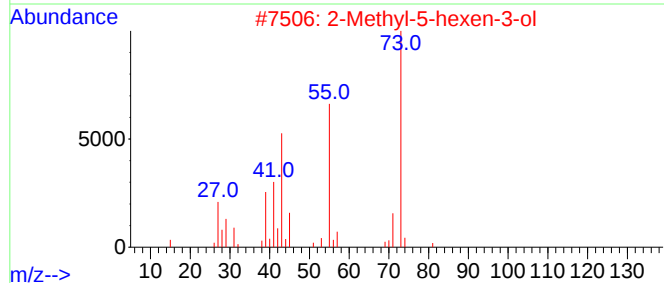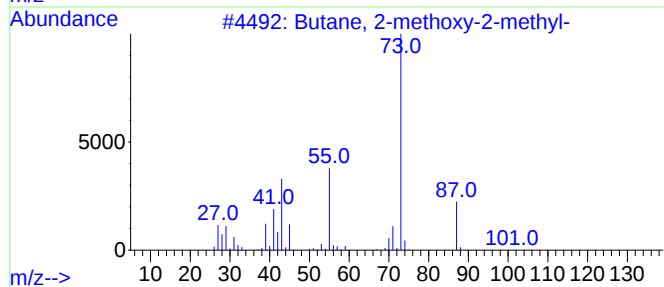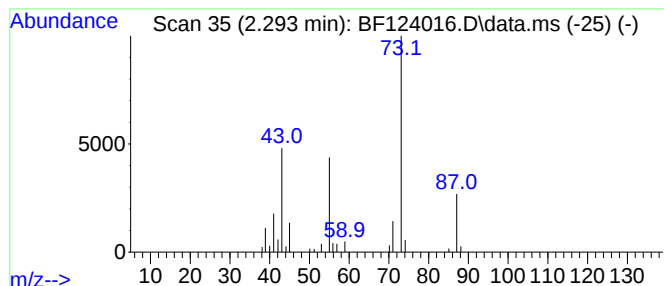

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052121\
Data File : BF124016.D
Acq On : 21 May 2021 13:16
Operator : JU/CG
Sample : PB136581BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB136581BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.293	4.9	ng	109123	1	6.893	448472	20.0